




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044859.D
Acq On : 01 Apr 2024 11:20
Operator : MA/JU
Sample : P1925-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PMW-6(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 12:12:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

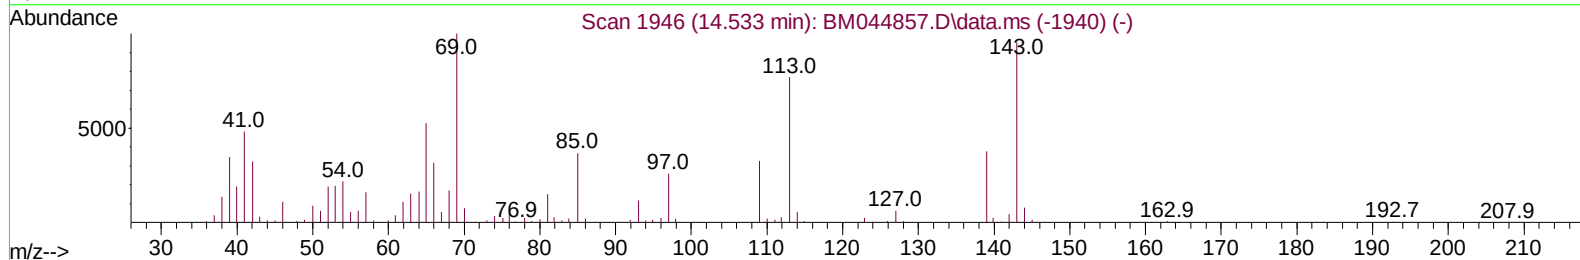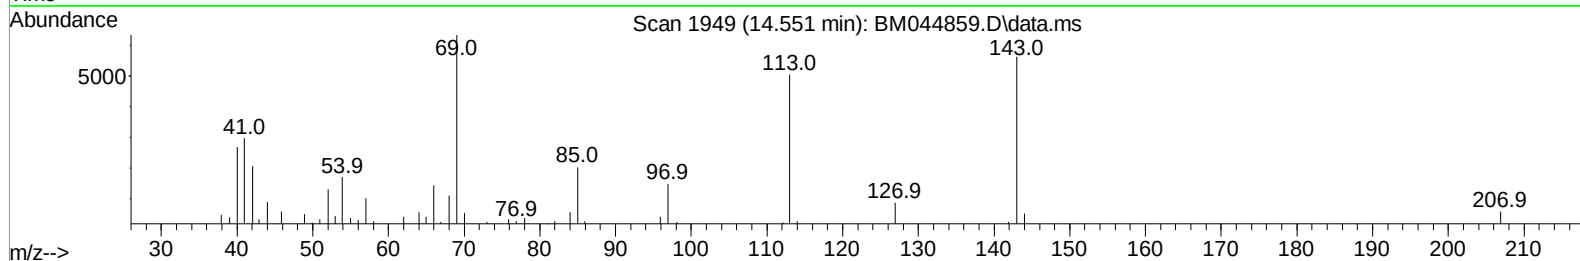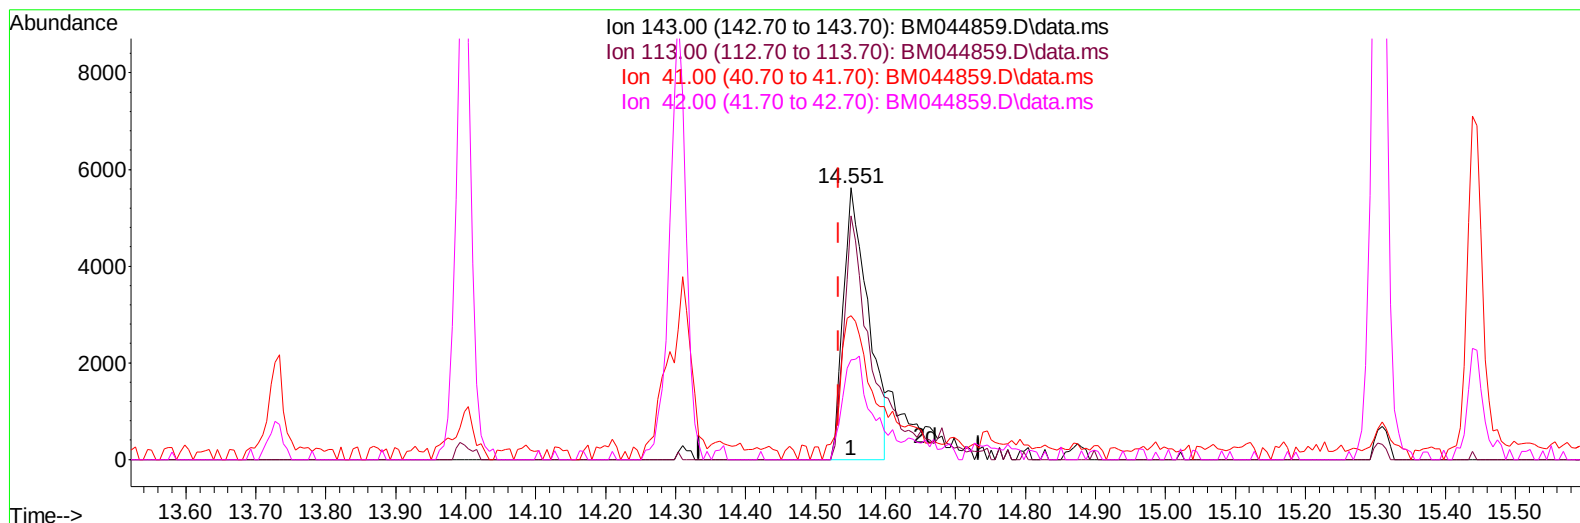

TIC: BM044859.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.018) 3.77 ng/ul

response 13829

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	89.66#
41.00	38.40	52.87#
42.00	26.60	36.58#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044859.D
Acq On : 01 Apr 2024 11:20
Operator : MA/JU
Sample : P1925-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PMW-6(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 12:12:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

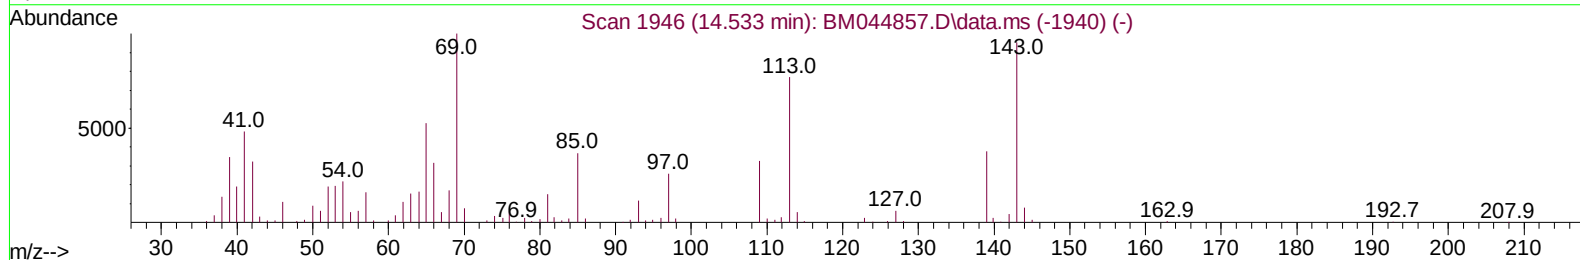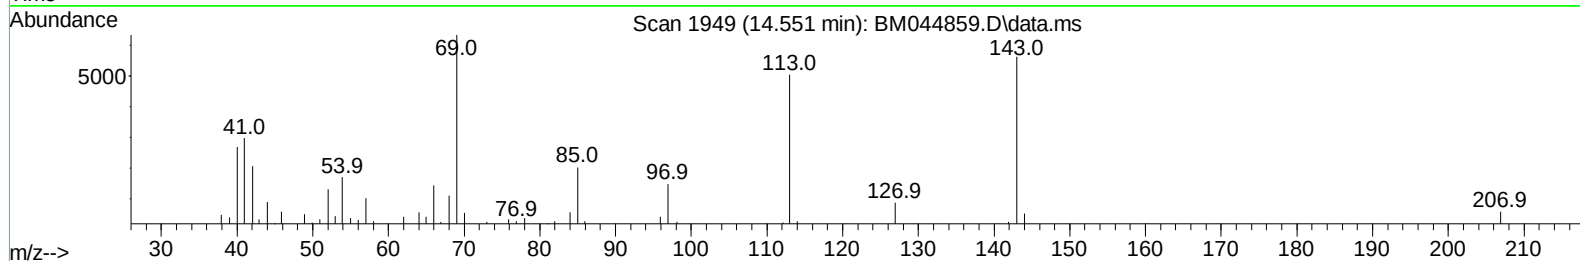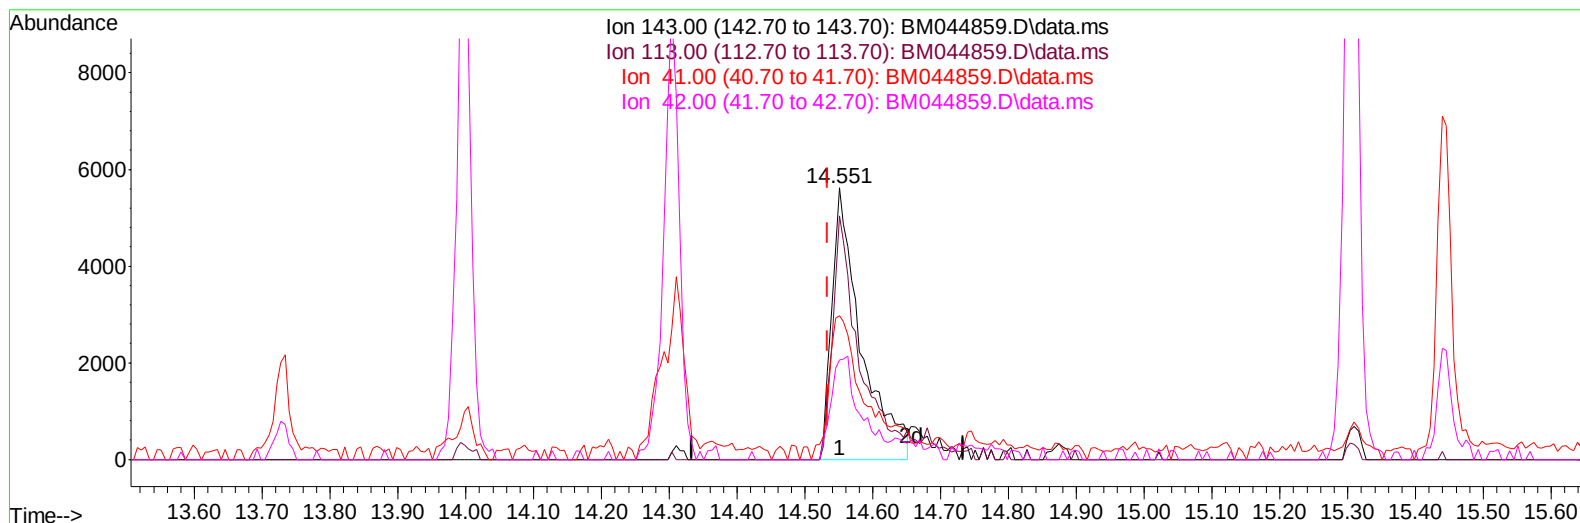

TIC: BM044859.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.018) 4.57 ng/ul m

response 16775

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	89.66#
41.00	38.40	52.87#
42.00	26.60	36.58#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
 Data File : BM044859.D
 Acq On : 01 Apr 2024 11:20
 Operator : MA/JU
 Sample : P1925-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PMW-6(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 12:17:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 13:54:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	99190	20.000	ng/ul	0.00
20) Naphthalene-d8	10.439	136	395415	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164	225710	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.063	188	410098	20.000	ng/ul	0.00
79) Chrysene-d12	21.262	240	340857	20.000	ng/ul	0.00
88) Perylene-d12	23.492	264	412907	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	13158	4.499	ng/uL	0.00
4) Pyridine-d5	3.640	84	56955	6.617	ng/ul	0.00
7) Phenol-d5	6.840	99	72343	7.094	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.010	67	207150	32.886	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	190225	25.383	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	125865	15.716	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	119440	35.872	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	126221	35.164	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	192503	31.512	ng/ul	0.00
31) 4-Chloroaniline-d4	10.592	131	237953	23.453	ng/ul	0.00
46) Dimethylphthalate-d6	13.727	166	608068	34.343	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	696393	34.391	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	16775m	4.569	ng/ul	0.02
60) Fluorene-d10	15.304	176	510807	34.331	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.445	200	83150	31.235	ng/ul	0.00
73) Anthracene-d10	17.163	188	775648	39.569	ng/ul	0.00
81) Pyrene-d10	19.462	212	838474	40.107	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.356	264	866577	39.929	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044859.D
Acq On : 01 Apr 2024 11:20
Operator : MA/JU
Sample : P1925-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PMW-6(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 12:17:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

