




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
 Data File : BM044860.D
 Acq On : 01 Apr 2024 11:56
 Operator : MA/JU
 Sample : P1925-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PMW-4(20240326)

Manual IntegrationsAPPROVED

Quant Time: Apr 01 12:35:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 13:54:26 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
 Supervised By :mohammad ahmed 04/02/2024

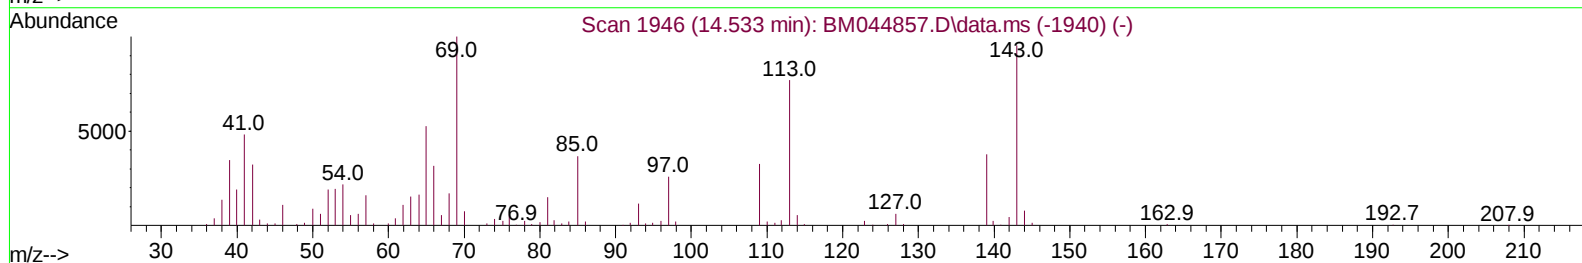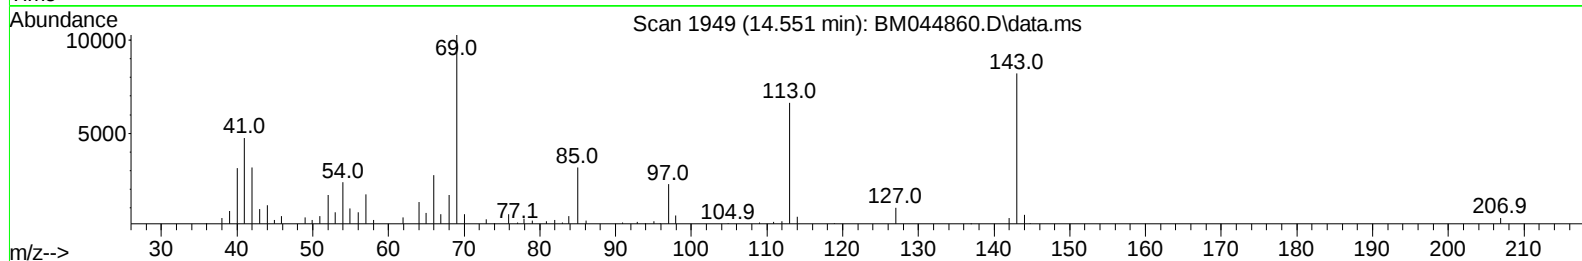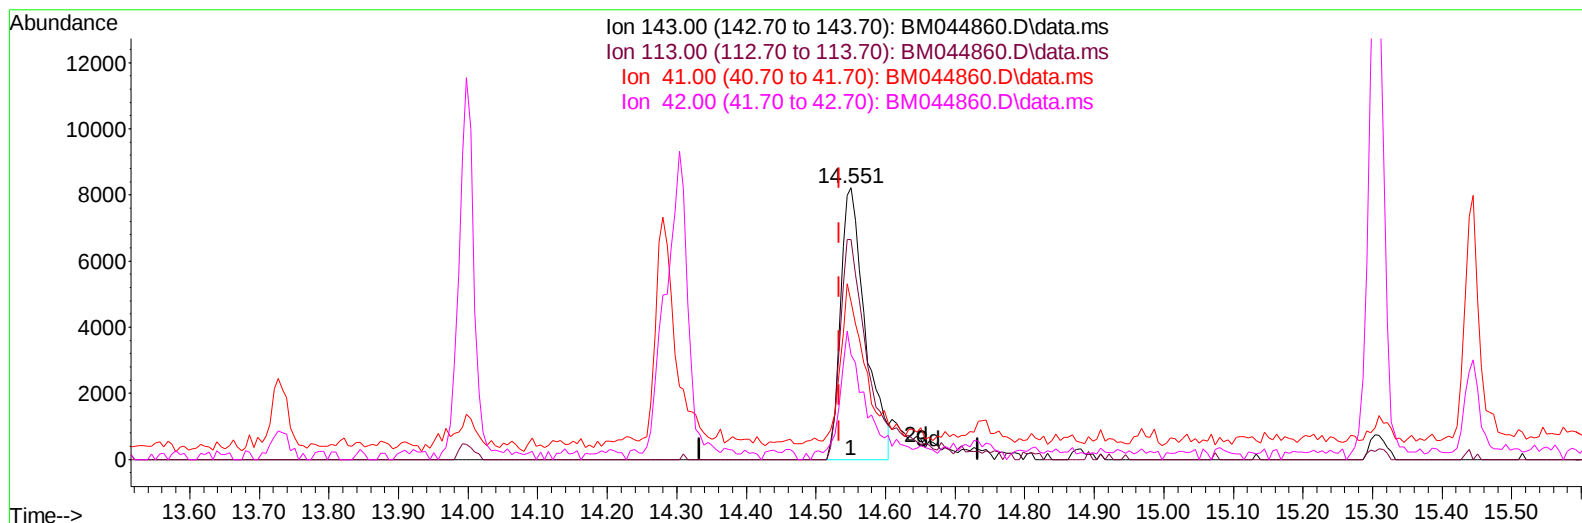

TIC: BM044860.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.018) 5.81 ng/u1

response 20284

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	80.96#
41.00	38.40	58.08#
42.00	26.60	38.62#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044860.D
Acq On : 01 Apr 2024 11:56
Operator : MA/JU
Sample : P1925-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PMW-4(20240326)

Manual IntegrationsAPPROVED

Quant Time: Apr 01 12:35:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

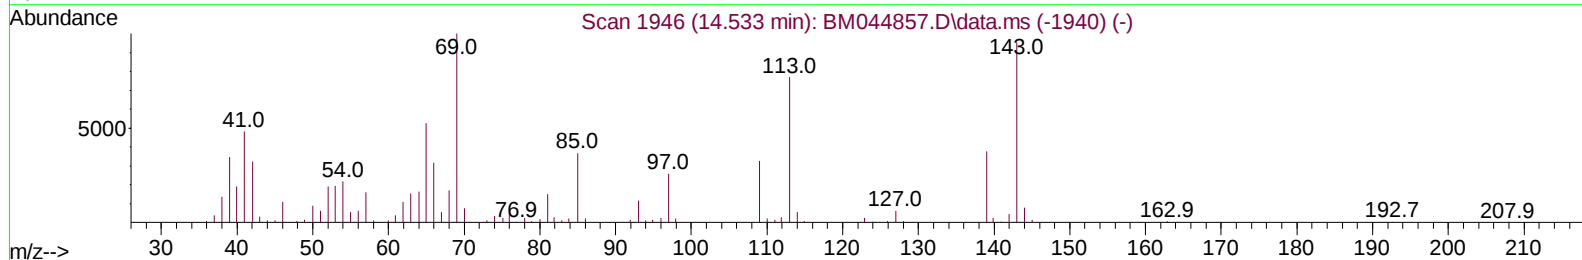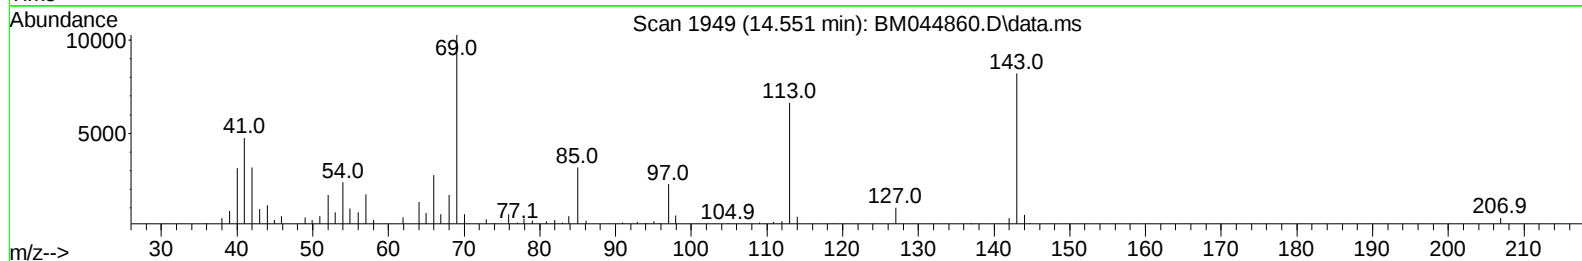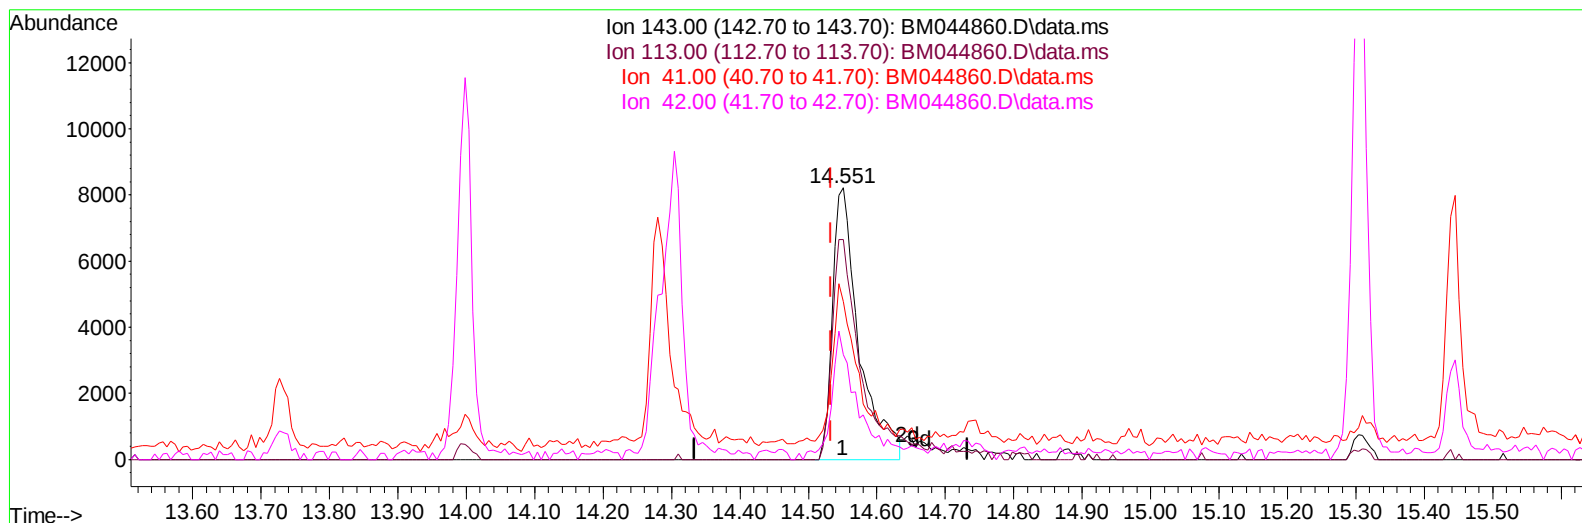

TIC: BM044860.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.018) 6.27 ng/ul m

response 21896

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	80.96#
41.00	38.40	58.08#
42.00	26.60	38.62#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
 Data File : BM044860.D
 Acq On : 01 Apr 2024 11:56
 Operator : MA/JU
 Sample : P1925-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PMW-4(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 23:17:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 13:54:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.657	152	94509	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.433	136	379351	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.304	164	214600	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.062	188	401666	20.000	ng/ul	0.00
79) Chrysene-d12	21.262	240	349227	20.000	ng/ul	0.00
88) Perylene-d12	23.491	264	421697	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	13728	4.927	ng/uL	0.00
4) Pyridine-d5	3.634	84	97619	11.903	ng/ul	0.00
7) Phenol-d5	6.839	99	85721	8.822	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.010	67	209624	34.927	ng/ul	0.00
11) 2-Chlorophenol-d4	7.192	132	206548	28.927	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	143814	18.846	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	123521	38.668	ng/ul	0.00
24) 2-Nitrophenol-d4	9.533	143	133286	38.705	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	216311	36.908	ng/ul	0.00
31) 4-Chloroaniline-d4	10.592	131	213673	21.952	ng/ul	0.00
46) Dimethylphthalate-d6	13.733	166	647857	38.485	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	761131	39.534	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	21896m	6.272	ng/ul	0.02
60) Fluorene-d10	15.304	176	553821	39.149	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.445	200	88413	33.910	ng/ul	0.00
73) Anthracene-d10	17.162	188	828915	43.174	ng/ul	0.00
81) Pyrene-d10	19.462	212	937507	43.769	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.356	264	951360	42.922	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044860.D
Acq On : 01 Apr 2024 11:56
Operator : MA/JU
Sample : P1925-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PMW-4(20240326)

Manual IntegrationsAPPROVED

Quant Time: Apr 01 23:17:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

