




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044862.D
Acq On : 01 Apr 2024 13:09
Operator : MA/JU
Sample : P1925-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PMW-10(20240326)

Manual IntegrationsAPPROVED

Quant Time: Apr 01 13:43:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

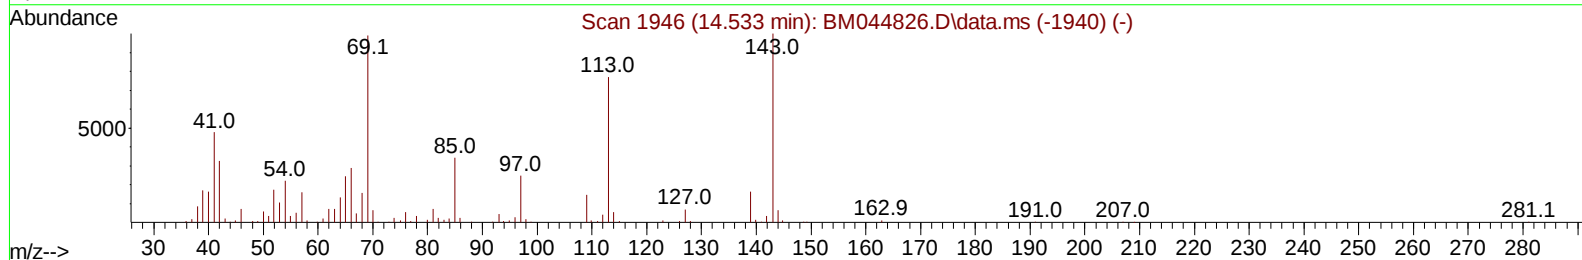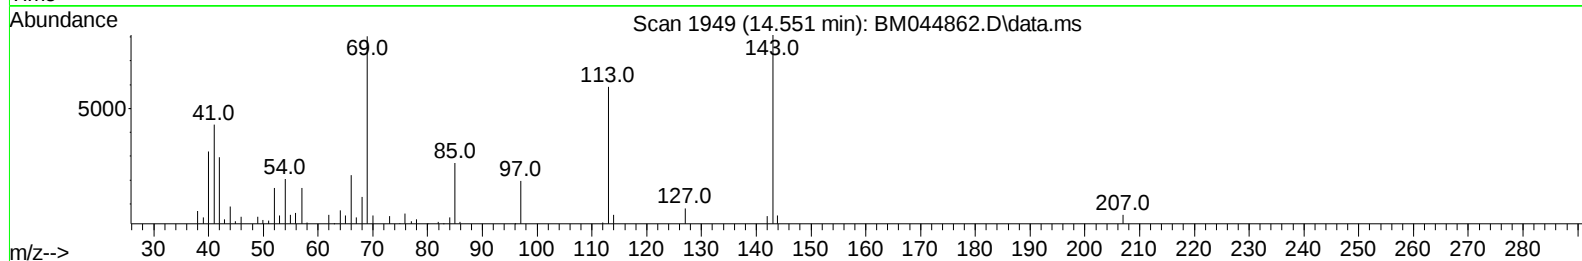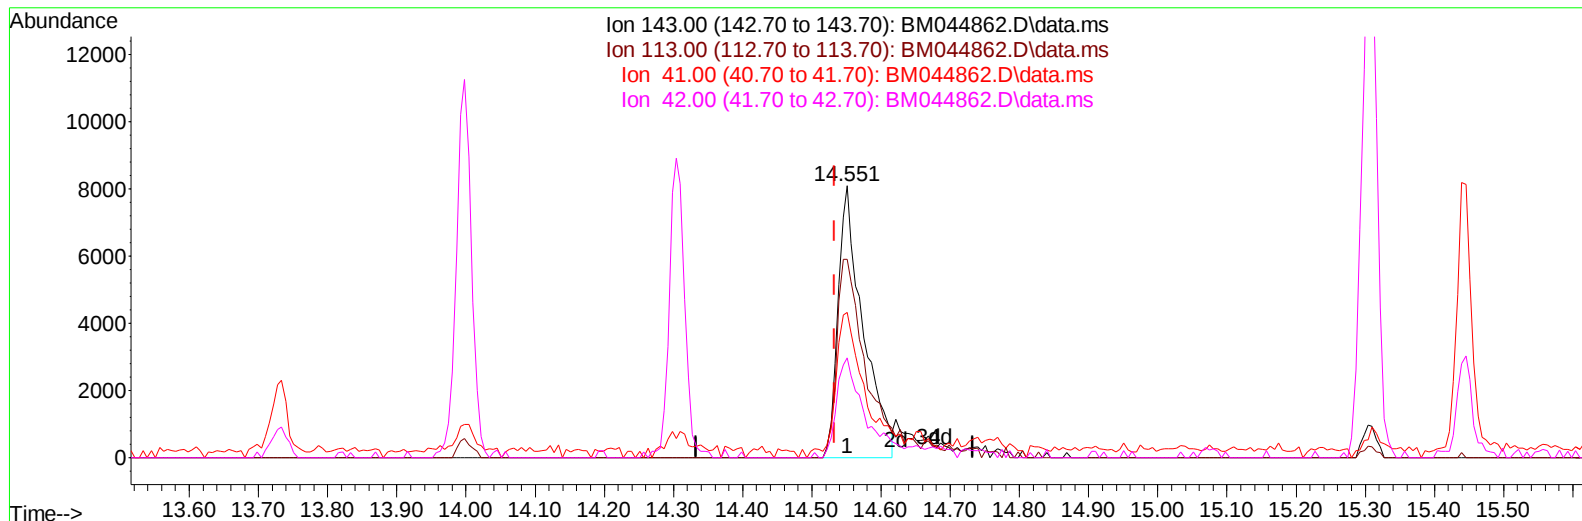

TIC: BM044862.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.018) 5.19 ng/u1

response 20124

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	73.05
41.00	38.40	53.35#
42.00	26.60	36.70#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
 Data File : BM044862.D
 Acq On : 01 Apr 2024 13:09
 Operator : MA/JU
 Sample : P1925-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PMW-10(20240326)

Manual IntegrationsAPPROVED

Quant Time: Apr 01 13:43:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 13:54:26 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
 Supervised By :mohammad ahmed 04/02/2024

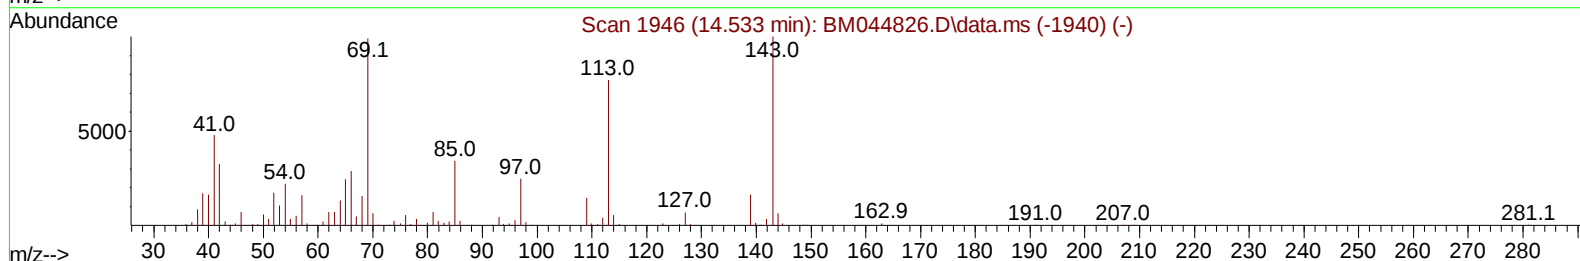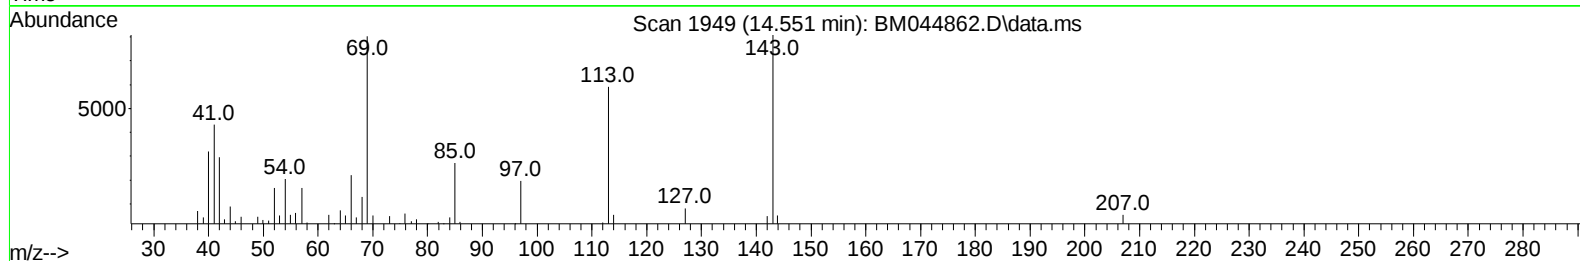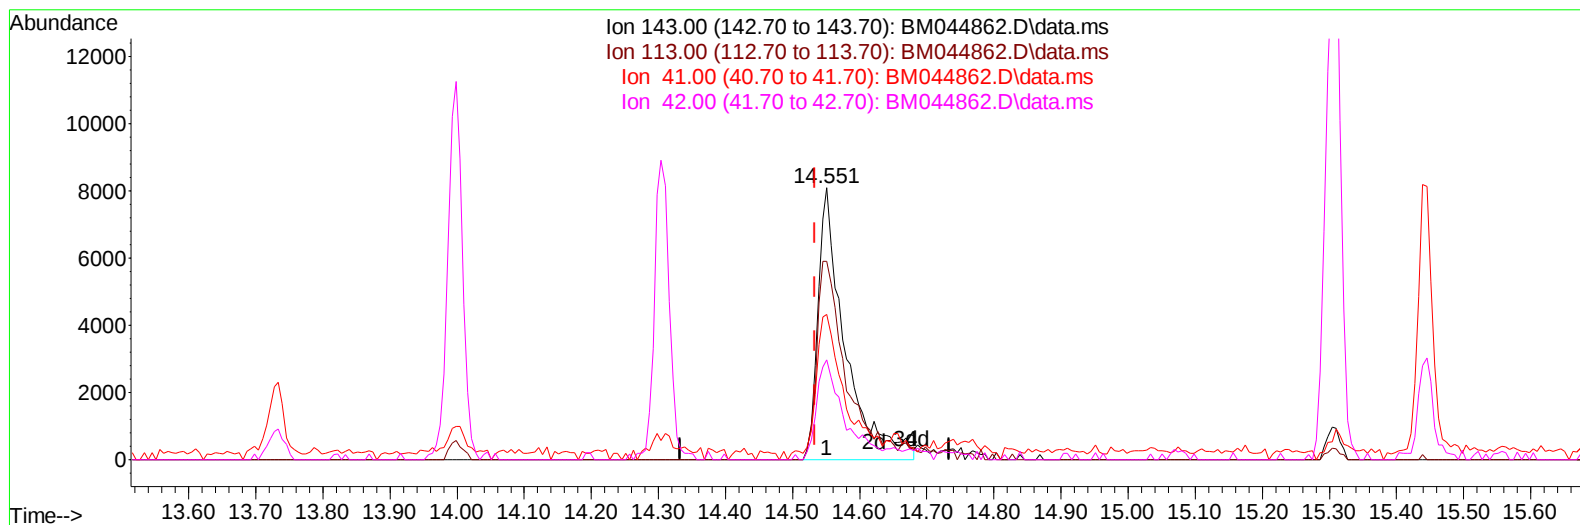

TIC: BM044862.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.018) 5.81 ng/ul m

response 22539

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	73.05
41.00	38.40	53.35#
42.00	26.60	36.70#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
 Data File : BM044862.D
 Acq On : 01 Apr 2024 13:09
 Operator : MA/JU
 Sample : P1925-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PMW-10(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 23:22:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 13:54:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.657	152	94121	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.434	136	402862	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.304	164	238338	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.063	188	443487	20.000	ng/ul	0.00
79) Chrysene-d12	21.262	240	319651	20.000	ng/ul	0.00
88) Perylene-d12	23.492	264	366813	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	12446	4.485	ng/uL	0.00
4) Pyridine-d5	3.634	84	85304	10.444	ng/ul	0.00
7) Phenol-d5	6.840	99	74751	7.725	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.010	67	224749	37.601	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	192240	27.034	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	132844	17.480	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	124922	36.825	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	132974	36.361	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	208120	33.438	ng/ul	0.00
31) 4-Chloroaniline-d4	10.592	131	282014	27.282	ng/ul	0.00
46) Dimethylphthalate-d6	13.733	166	698776	37.375	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	797177	37.283	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	22539m	5.813	ng/ul	0.02
60) Fluorene-d10	15.310	176	596958	37.995	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	98891	34.352	ng/ul	0.00
73) Anthracene-d10	17.163	188	901744	42.538	ng/ul	0.00
81) Pyrene-d10	19.462	212	922420	47.050	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.350	264	839167	43.525	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044862.D
Acq On : 01 Apr 2024 13:09
Operator : MA/JU
Sample : P1925-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PMW-10(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 23:22:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

