




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044863.D
Acq On : 01 Apr 2024 13:46
Operator : MA/JU
Sample : P1925-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 14:47:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

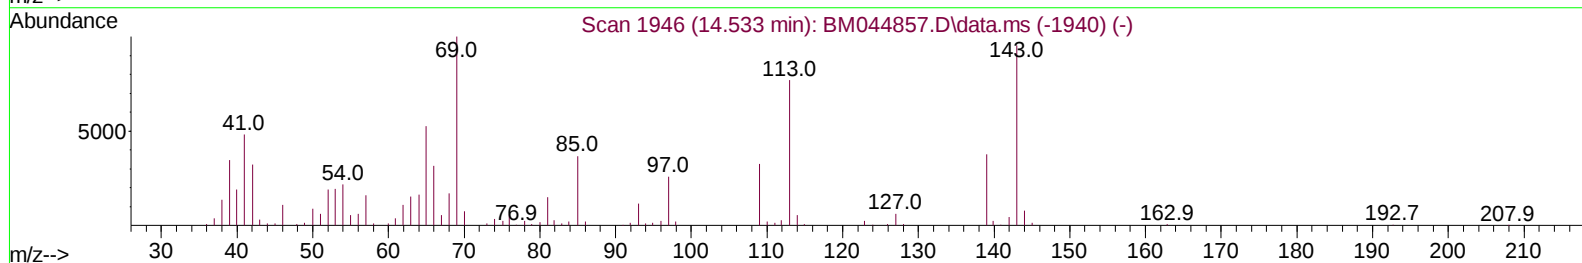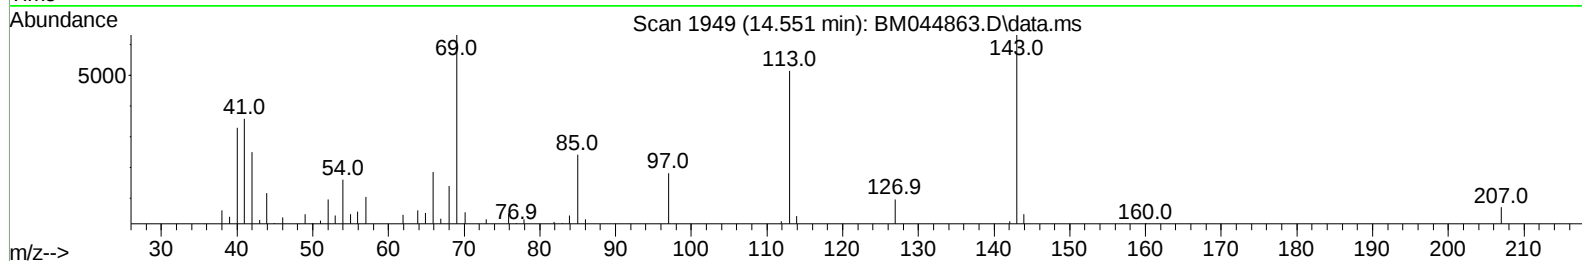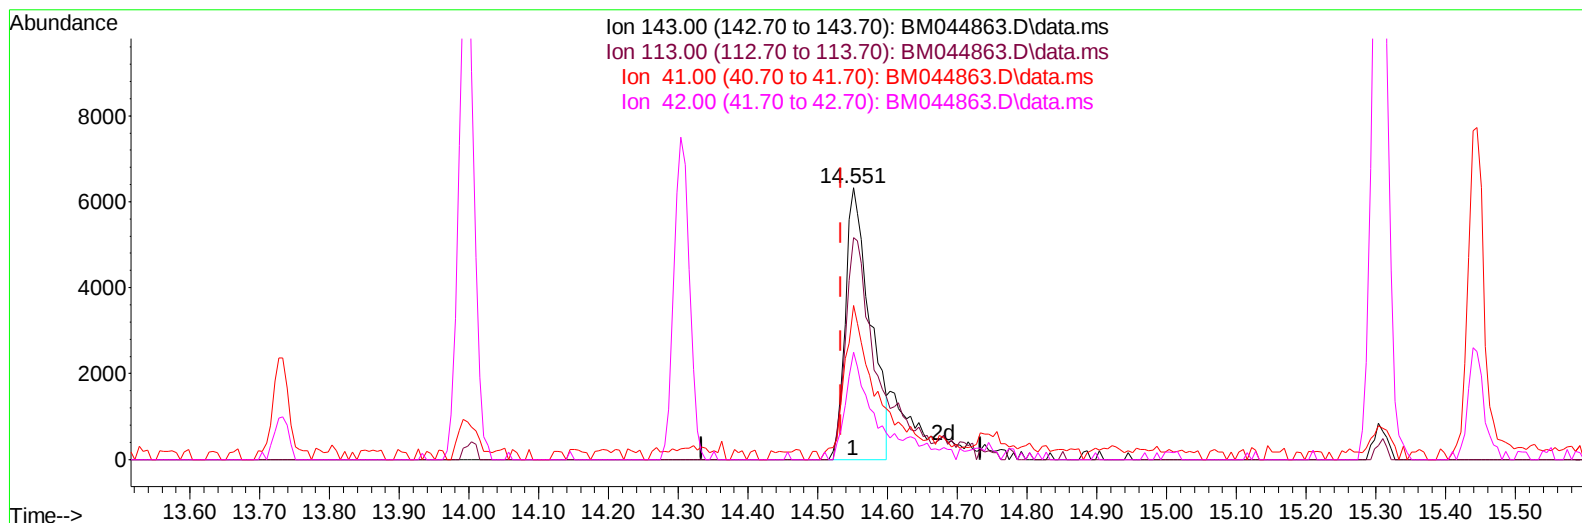

TIC: BM044863.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.018) 4.61 ng/u1

response 15551

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	81.62#
41.00	38.40	56.83#
42.00	26.60	39.60#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044863.D
Acq On : 01 Apr 2024 13:46
Operator : MA/JU
Sample : P1925-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB(20240326)

Manual IntegrationsAPPROVED

Quant Time: Apr 01 14:47:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

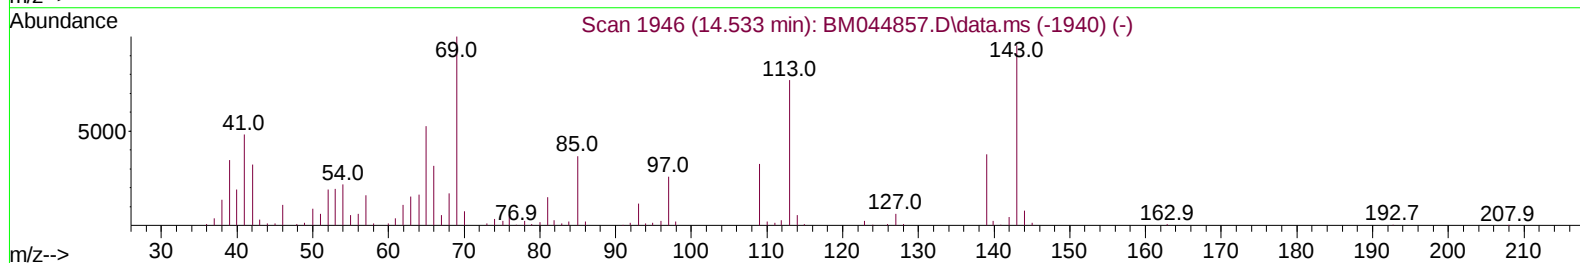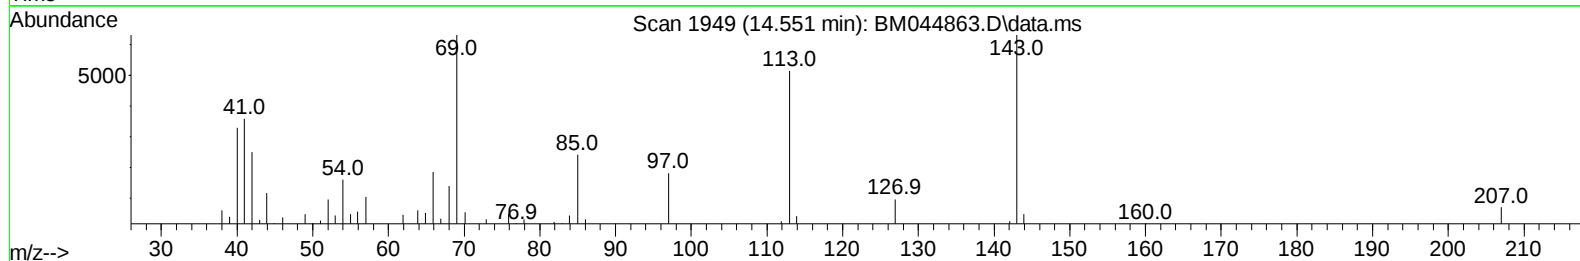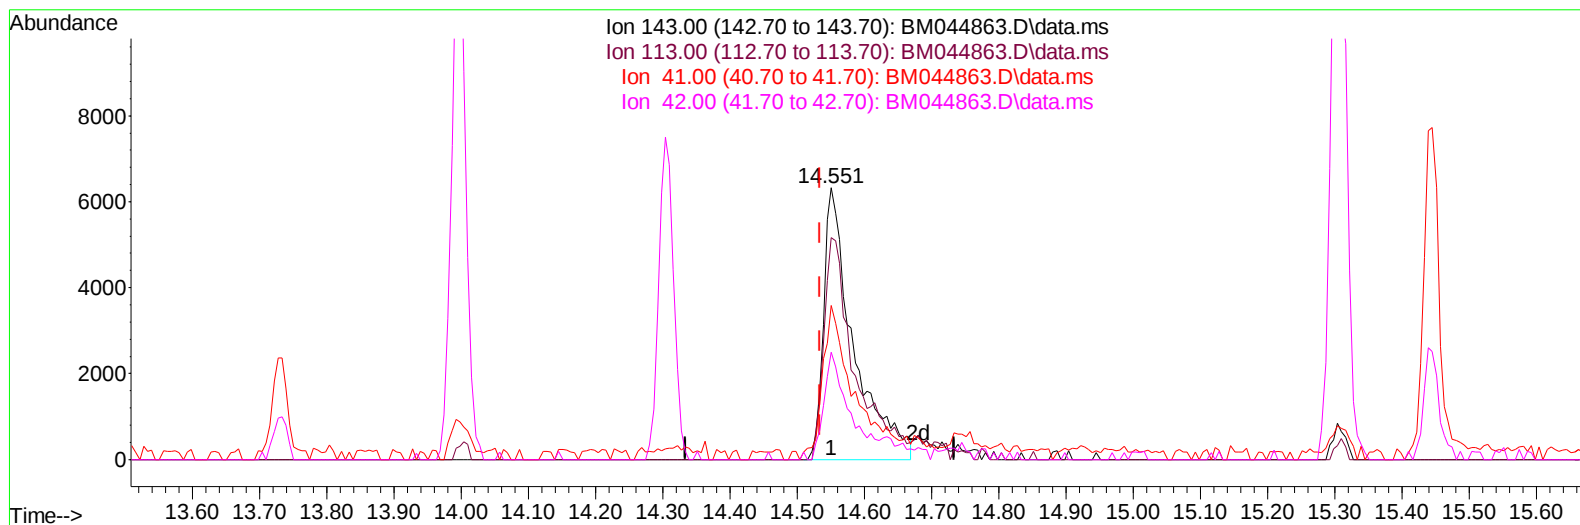

TIC: BM044863.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.018) 5.76 ng/ul m

response 19430

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	81.62#
41.00	38.40	56.83#
42.00	26.60	39.60#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
 Data File : BM044863.D
 Acq On : 01 Apr 2024 13:46
 Operator : MA/JU
 Sample : P1925-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FB(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 14:49:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 13:54:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	87643	20.000	ng/ul	0.00
20) Naphthalene-d8	10.433	136	365084	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.304	164	207300	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.062	188	376734	20.000	ng/ul	0.00
79) Chrysene-d12	21.262	240	291633	20.000	ng/ul	0.00
88) Perylene-d12	23.491	264	340054	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	13442	5.202	ng/uL	0.00
4) Pyridine-d5	3.640	84	40166	5.281	ng/ul	0.00
7) Phenol-d5	6.840	99	73934	8.205	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.010	67	226006	40.606	ng/ul	0.00
11) 2-Chlorophenol-d4	7.192	132	206704	31.216	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	135030	19.081	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	133057	43.281	ng/ul	0.00
24) 2-Nitrophenol-d4	9.533	143	137926	41.618	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	211537	37.504	ng/ul	0.00
31) 4-Chloroaniline-d4	10.592	131	203533	21.727	ng/ul	0.00
46) Dimethylphthalate-d6	13.733	166	722109	44.406	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	826848	44.460	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	19430m	5.762	ng/ul	0.02
60) Fluorene-d10	15.310	176	608520	44.530	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	94996	38.846	ng/ul	0.00
73) Anthracene-d10	17.162	188	894839	49.692	ng/ul	0.00
81) Pyrene-d10	19.462	212	929053	51.941	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.356	264	899682	50.336	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044863.D
Acq On : 01 Apr 2024 13:46
Operator : MA/JU
Sample : P1925-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB(20240326)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 01 14:49:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 13:54:26 2024
Response via : Initial Calibration

