

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
 Data File : BM044858.D
 Acq On : 01 Apr 2024 10:43
 Operator : MA/JU
 Sample : PB159895BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK895

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	31	rVB	33775	46723	2.07%	0.166%
2	3.628	89	92	122	rBV	459251	822089	36.49%	2.924%
3	3.928	141	143	149	rVB4	6999	9435	0.42%	0.034%
4	4.081	168	169	171	rBV2	3613	2921	0.13%	0.010%
5	6.075	506	508	512	rVV4	2160	2263	0.10%	0.008%
6	6.116	512	515	518	rVV4	1810	2427	0.11%	0.009%
7	6.839	631	638	649	rBV	557983	928786	41.22%	3.304%
8	7.016	661	668	677	rBV	442651	712970	31.64%	2.536%
9	7.192	691	698	709	rBV	537768	898419	39.88%	3.196%
10	7.663	769	778	790	rBV	435308	701635	31.14%	2.496%
11	8.369	891	898	910	rBV	644854	1090913	48.42%	3.880%
12	8.822	968	975	983	rBV	548960	913372	40.54%	3.249%
13	9.533	1089	1096	1105	rBV	483102	793759	35.23%	2.823%
14	9.616	1108	1110	1114	rVB5	2687	3836	0.17%	0.014%
15	10.063	1179	1186	1205	rBV	584434	1082357	48.04%	3.850%
16	10.286	1222	1224	1229	rVB6	1810	2381	0.11%	0.008%
17	10.439	1241	1250	1260	rVB	611325	1001919	44.47%	3.564%
18	10.592	1269	1276	1296	rBV	375211	736473	32.69%	2.620%
19	11.639	1451	1454	1457	rBV4	1470	2671	0.12%	0.010%
20	12.045	1517	1523	1533	rBV3	6899	14048	0.62%	0.050%
21	13.204	1713	1720	1726	rBV4	8786	14780	0.66%	0.053%
22	13.733	1803	1810	1820	rBV	1005345	1459742	64.79%	5.192%
23	13.998	1848	1855	1866	rBV	1233212	1817547	80.67%	6.465%
24	14.310	1898	1908	1916	rBV	854852	1249733	55.47%	4.445%
25	14.533	1940	1946	1969	rBV	334779	751382	33.35%	2.673%
26	15.309	2071	2078	2091	rBV	1510486	2139621	94.96%	7.611%
27	15.445	2095	2101	2115	rVV	539575	767832	34.08%	2.731%
28	15.545	2117	2118	2124	rVB3	5936	6314	0.28%	0.022%
29	16.092	2208	2211	2215	rVB4	3649	4393	0.19%	0.016%
30	16.580	2291	2294	2297	rVB5	2296	2475	0.11%	0.009%
31	16.851	2337	2340	2343	rBV4	1945	2757	0.12%	0.010%
32	17.021	2364	2369	2370	rBV4	1528	2549	0.11%	0.009%
33	17.062	2370	2376	2386	rBV	980597	1345227	59.71%	4.785%
34	17.162	2386	2393	2402	rBV	1660216	2253075	100.00%	8.014%
35	17.980	2529	2532	2539	rVB8	7511	11101	0.49%	0.039%
36	18.574	2631	2633	2636	rBV4	1900	2316	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044858.D
Acq On : 01 Apr 2024 10:43
Operator : MA/JU
Sample : PB159895BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK895

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	19.027	2706	2710	2714	rBV4	15189	18671	0.83%	0.066%
38	19.097	2718	2722	2728	rBV	13411	22273	0.99%	0.079%
39	19.209	2739	2741	2743	rBV2	3136	2325	0.10%	0.008%
40	19.262	2748	2750	2758	rVB7	6261	12017	0.53%	0.043%
41	19.468	2778	2785	2794	rBV	1627791	2237284	99.30%	7.958%
42	21.262	3085	3090	3098	rBV	814475	1096247	48.66%	3.899%
43	23.356	3439	3446	3453	rBV2	1067503	1976312	87.72%	7.030%
44	23.497	3464	3470	3480	rVB	596743	1147880	50.95%	4.083%




Sum of corrected areas: 28113250

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044858.D
Acq On : 01 Apr 2024 10:43
Operator : MA/JU
Sample : PB159895BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK895

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

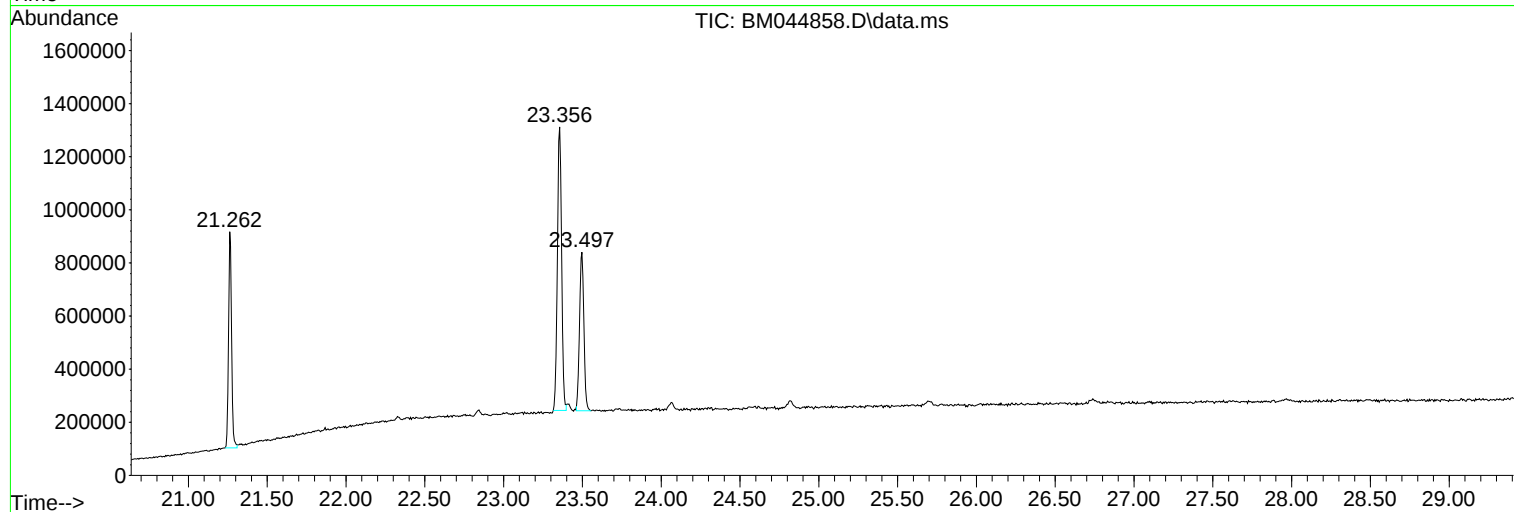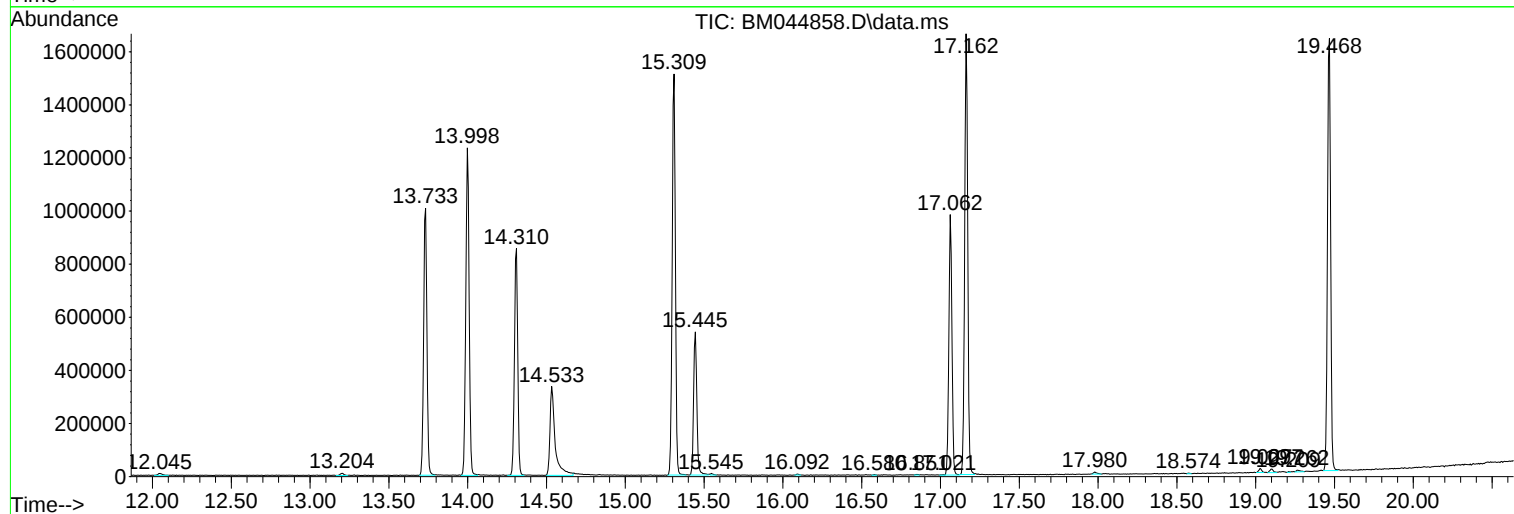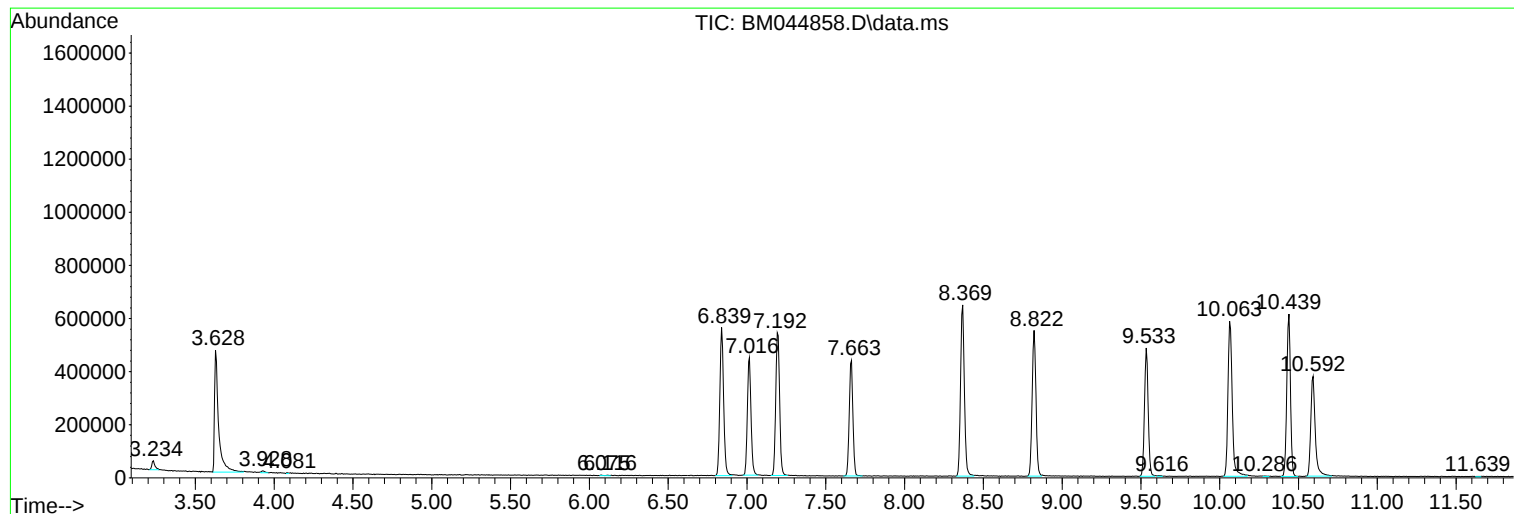

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044858.D
Acq On : 01 Apr 2024 10:43
Operator : MA/JU
Sample : PB159895BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK895

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044858.D
Acq On : 01 Apr 2024 10:43
Operator : MA/JU
Sample : PB159895BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK895

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------