

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
 Data File : BM044867.D
 Acq On : 01 Apr 2024 16:13
 Operator : MA/JU
 Sample : PB159928BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK928

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	37	rVB	35144	59170	3.13%	0.244%
2	3.634	89	93	111	rBV	279424	513055	27.18%	2.114%
3	3.928	140	143	152	rVB3	9097	16606	0.88%	0.068%
4	4.463	232	234	237	rBV4	1955	2627	0.14%	0.011%
5	4.746	280	282	284	rBV3	2977	1889	0.10%	0.008%
6	4.769	284	286	289	rVV4	2028	2333	0.12%	0.010%
7	4.993	322	324	330	rVB5	2648	5088	0.27%	0.021%
8	5.099	340	342	344	rBV3	2036	1959	0.10%	0.008%
9	5.310	376	378	381	rVB4	2186	2073	0.11%	0.009%
10	6.369	556	558	562	rBV3	2327	3421	0.18%	0.014%
11	6.516	581	583	586	rVB3	2538	2675	0.14%	0.011%
12	6.840	631	638	648	rBV	500535	844780	44.75%	3.480%
13	7.010	661	667	678	rBV	395667	645617	34.20%	2.660%
14	7.110	682	684	688	rVB5	2350	1960	0.10%	0.008%
15	7.193	691	698	712	rBV	503435	817965	43.33%	3.370%
16	7.657	771	777	785	rBV	424797	686985	36.39%	2.830%
17	7.798	799	801	805	rVB4	1591	1949	0.10%	0.008%
18	8.287	881	884	889	rBV6	1237	2617	0.14%	0.011%
19	8.369	889	898	912	rBV	566897	988992	52.39%	4.074%
20	8.551	927	929	935	rVB5	1709	2045	0.11%	0.008%
21	8.822	967	975	986	rBV	489385	819917	43.43%	3.378%
22	8.992	999	1004	1008	rVB8	1858	2489	0.13%	0.010%
23	9.534	1087	1096	1105	rBV	412138	696829	36.91%	2.871%
24	9.881	1153	1155	1158	rVB4	1995	2256	0.12%	0.009%
25	9.916	1158	1161	1164	rBV3	1483	1984	0.11%	0.008%
26	10.063	1179	1186	1211	rBV	458594	960837	50.90%	3.958%
27	10.434	1239	1249	1260	rBV	564795	989177	52.40%	4.075%
28	11.075	1355	1358	1361	rBV4	2093	2735	0.14%	0.011%
29	11.592	1442	1446	1449	rBV4	1135	1963	0.10%	0.008%
30	11.833	1484	1487	1490	rBV2	1652	2268	0.12%	0.009%
31	12.016	1514	1518	1519	rBV3	1919	2550	0.14%	0.011%
32	12.051	1519	1524	1529	rVB3	5281	9886	0.52%	0.041%
33	13.198	1716	1719	1724	rVB5	5281	8605	0.46%	0.035%
34	13.286	1729	1734	1737	rVB5	1588	2470	0.13%	0.010%
35	13.727	1803	1809	1820	rBV	876877	1279555	67.78%	5.271%
36	13.804	1820	1822	1828	rVB7	2117	3853	0.20%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
 Data File : BM044867.D
 Acq On : 01 Apr 2024 16:13
 Operator : MA/JU
 Sample : PB159928BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK928

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

37	13.998	1848	1855	1865	rBV	1041298	1545290	81.86%	6.366%
38	14.304	1900	1907	1914	rBV	831011	1209945	64.09%	4.985%
39	14.533	1940	1946	1969	rBV	245989	611327	32.38%	2.518%
40	15.304	2070	2077	2089	rBV	1269580	1860986	98.58%	7.667%
41	15.439	2094	2100	2112	rVV	405273	627948	33.26%	2.587%
42	15.545	2115	2118	2123	rVV6	4548	8197	0.43%	0.034%
43	15.816	2161	2164	2169	rVV3	7452	10523	0.56%	0.043%
44	15.874	2171	2174	2178	rVV5	1421	2355	0.12%	0.010%
45	16.092	2208	2211	2217	rVB6	4764	6634	0.35%	0.027%
46	16.168	2221	2224	2227	rVV4	2363	2952	0.16%	0.012%
47	16.210	2227	2231	2234	rVB5	2606	3210	0.17%	0.013%
48	16.474	2273	2276	2280	rVB4	1688	1955	0.10%	0.008%
49	16.845	2336	2339	2347	rVB7	1881	2933	0.16%	0.012%
50	17.063	2369	2376	2386	rVV	910097	1294228	68.56%	5.332%
51	17.163	2386	2393	2404	rVV	1349272	1887817	100.00%	7.777%
52	17.380	2428	2430	2433	rBV4	1527	1896	0.10%	0.008%
53	17.468	2443	2445	2448	rBV4	1542	2235	0.12%	0.009%
54	17.751	2487	2493	2497	rBV7	4905	10051	0.53%	0.041%
55	17.874	2510	2514	2517	rBV5	2220	2849	0.15%	0.012%
56	17.915	2517	2521	2523	rVB4	1556	2113	0.11%	0.009%
57	17.980	2529	2532	2539	rVB10	4409	8202	0.43%	0.034%
58	18.121	2553	2556	2560	rBV5	1586	2415	0.13%	0.010%
59	18.186	2565	2567	2568	rBV2	2228	2082	0.11%	0.009%
60	18.268	2579	2581	2584	rBV4	1455	2081	0.11%	0.009%
61	18.515	2621	2623	2625	rBV3	2437	1927	0.10%	0.008%
62	18.598	2632	2637	2639	rBV4	1689	2567	0.14%	0.011%
63	18.633	2641	2643	2645	rBV3	1823	2005	0.11%	0.008%
64	19.027	2706	2710	2714	rVV3	14530	19380	1.03%	0.080%
65	19.062	2714	2716	2719	rVV4	4559	6338	0.34%	0.026%
66	19.104	2719	2723	2728	rVB3	10630	16235	0.86%	0.067%
67	19.168	2732	2734	2737	rBV4	2475	3168	0.17%	0.013%
68	19.268	2746	2751	2754	rBV6	7094	12491	0.66%	0.051%
69	19.415	2773	2776	2777	rBV3	4328	4114	0.22%	0.017%
70	19.462	2778	2784	2793	rVV	1370843	1869630	99.04%	7.702%
71	21.262	3085	3090	3098	rBV	815529	1072316	56.80%	4.418%
72	23.350	3439	3445	3452	rBV	917943	1633329	86.52%	6.729%
73	23.492	3463	3469	3480	rVB3	573069	1128865	59.80%	4.651%




Sum of corrected areas: 24273769

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044867.D
Acq On : 01 Apr 2024 16:13
Operator : MA/JU
Sample : PB159928BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK928

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

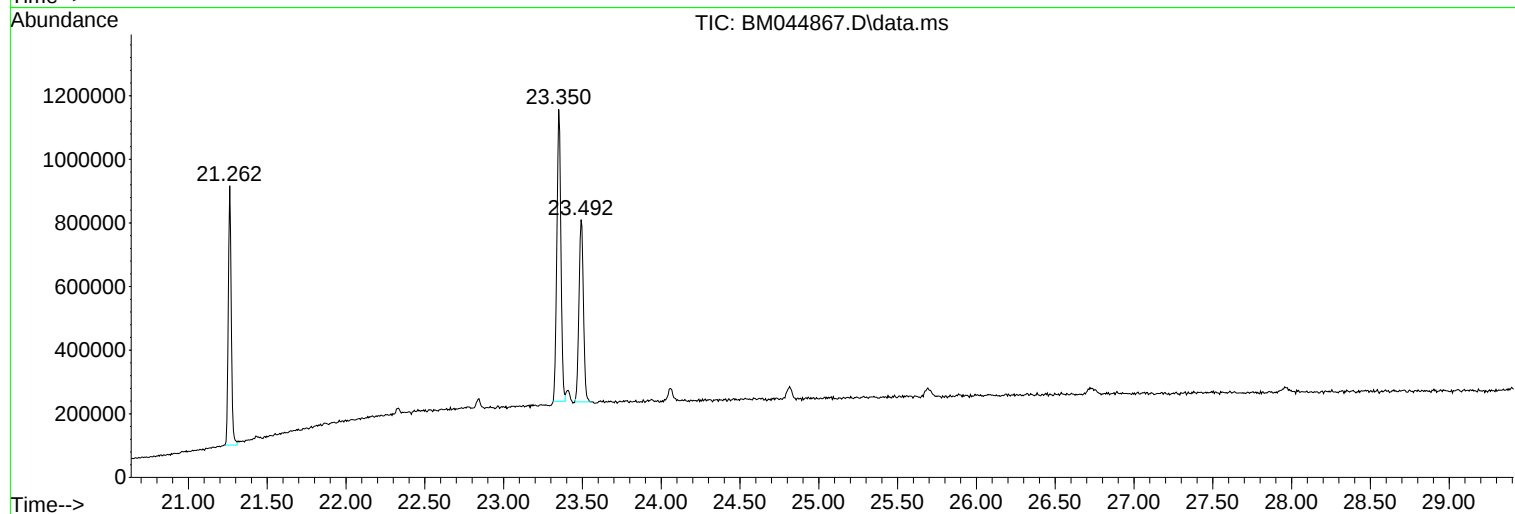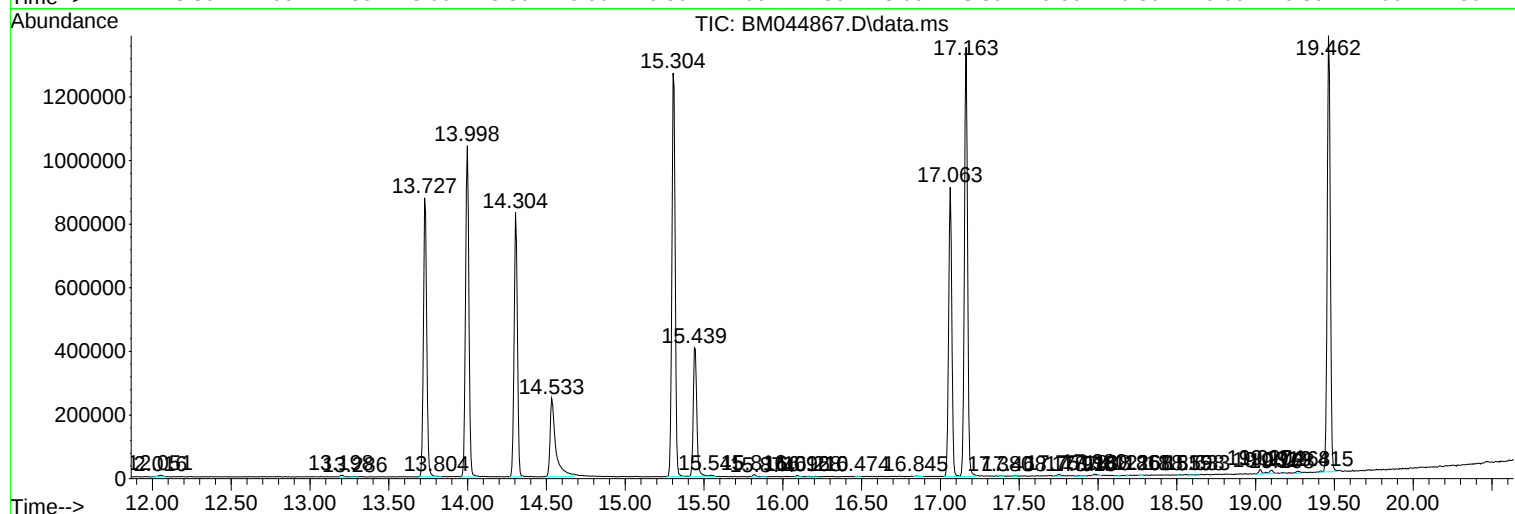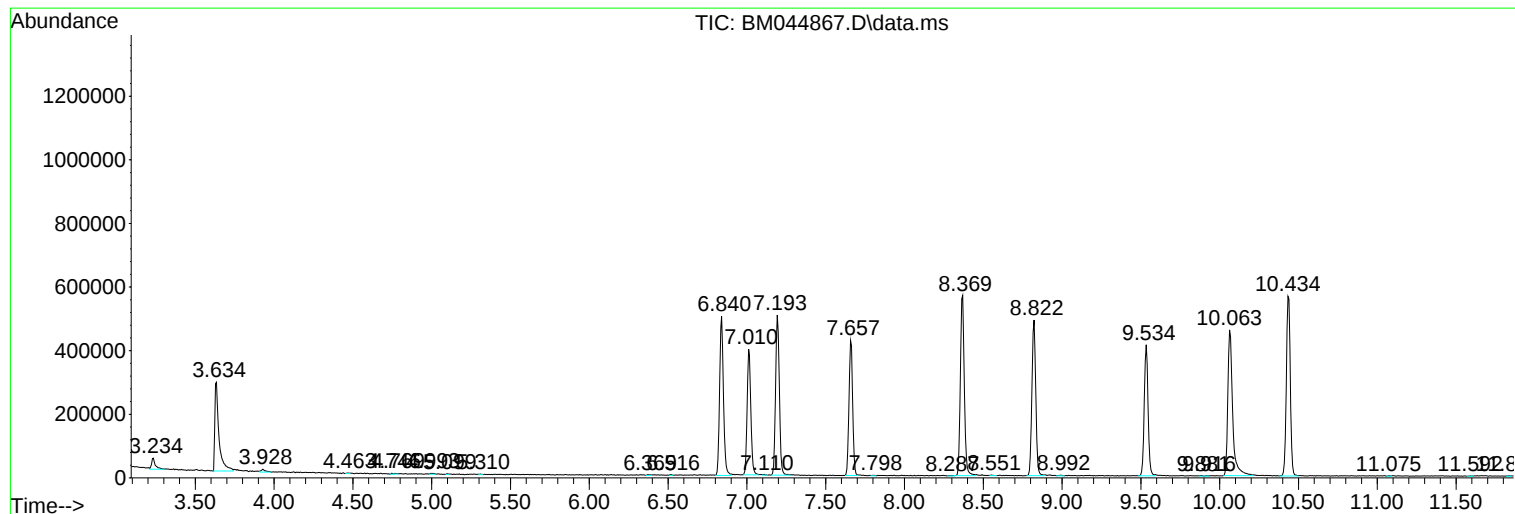

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044867.D
Acq On : 01 Apr 2024 16:13
Operator : MA/JU
Sample : PB159928BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK928

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040124\
Data File : BM044867.D
Acq On : 01 Apr 2024 16:13
Operator : MA/JU
Sample : PB159928BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK928

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc