

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040125\
 Data File : BM049779.D
 Acq On : 01 Apr 2025 18:06
 Operator : RC/JU
 Sample : Q1662-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-6

Quant Time: Apr 01 19:19:37 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 13 14:55:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	310337	20.000	ng	-0.01
21) Naphthalene-d8	10.586	136	1060057	20.000	ng	-0.02
39) Acenaphthene-d10	14.433	164	672580	20.000	ng	-0.01
64) Phenanthrene-d10	17.174	188	1210736	20.000	ng	-0.01
76) Chrysene-d12	21.403	240	835223	20.000	ng	-0.02
86) Perylene-d12	24.409	264	746205	20.000	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.381	112	3592376	195.320	ng	0.00
7) Phenol-d6	6.969	99	4463605	193.386	ng	-0.01
23) Nitrobenzene-d5	8.951	82	2674812	129.549	ng	-0.01
42) 2,4,6-Tribromophenol	15.921	330	1836095	233.787	ng	-0.01
45) 2-Fluorobiphenyl	13.057	172	7058484	131.433	ng	-0.01
79) Terphenyl-d14	19.797	244	8720938	175.951	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040125\
Data File : BM049779.D
Acq On : 01 Apr 2025 18:06
Operator : RC/JU
Sample : Q1662-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-6


Quant Time: Apr 01 19:19:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

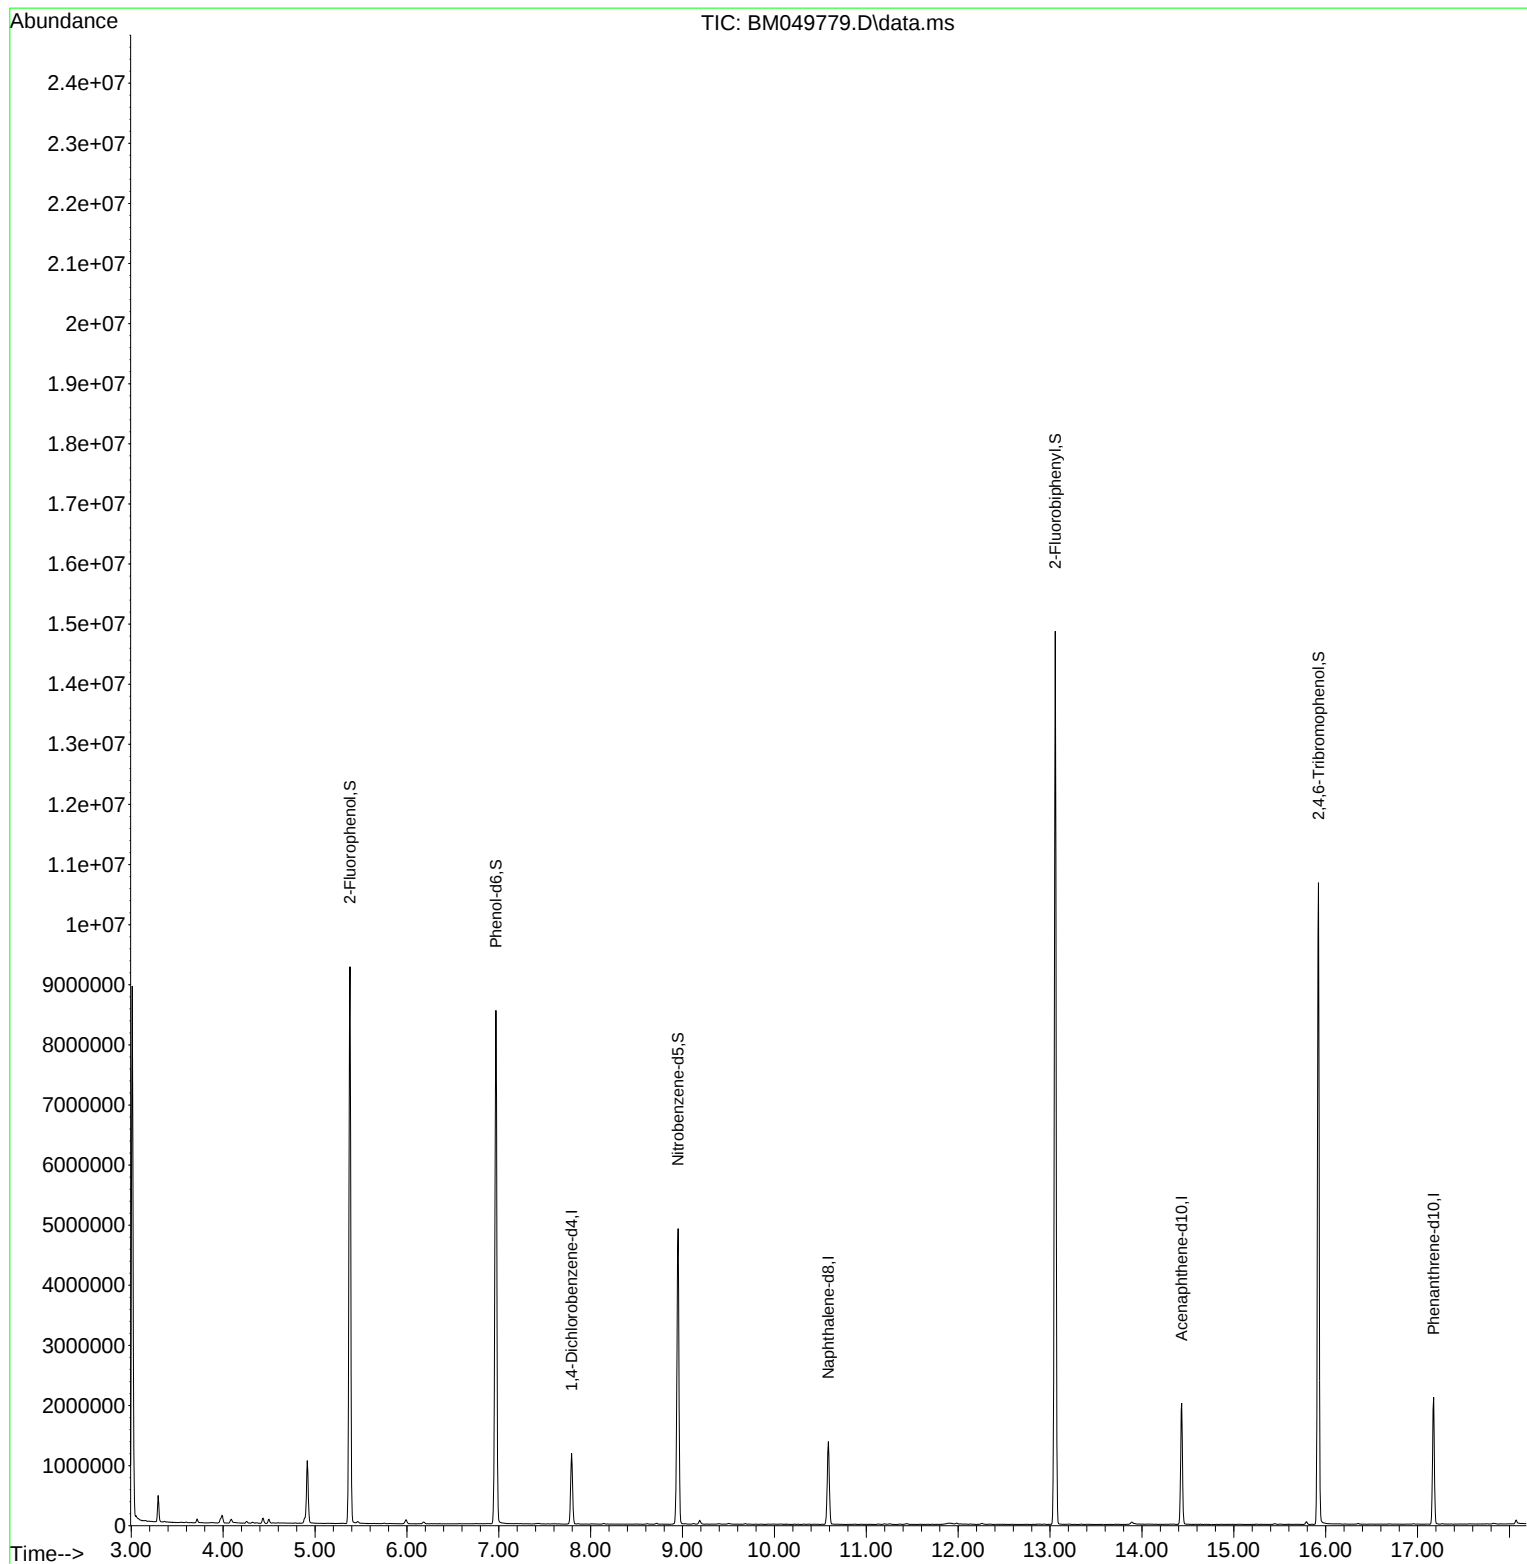


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040125\
Data File : BM049779.D
Acq On : 01 Apr 2025 18:06
Operator : RC/JU
Sample : Q1662-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-6

Quant Time: Apr 01 19:19:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration




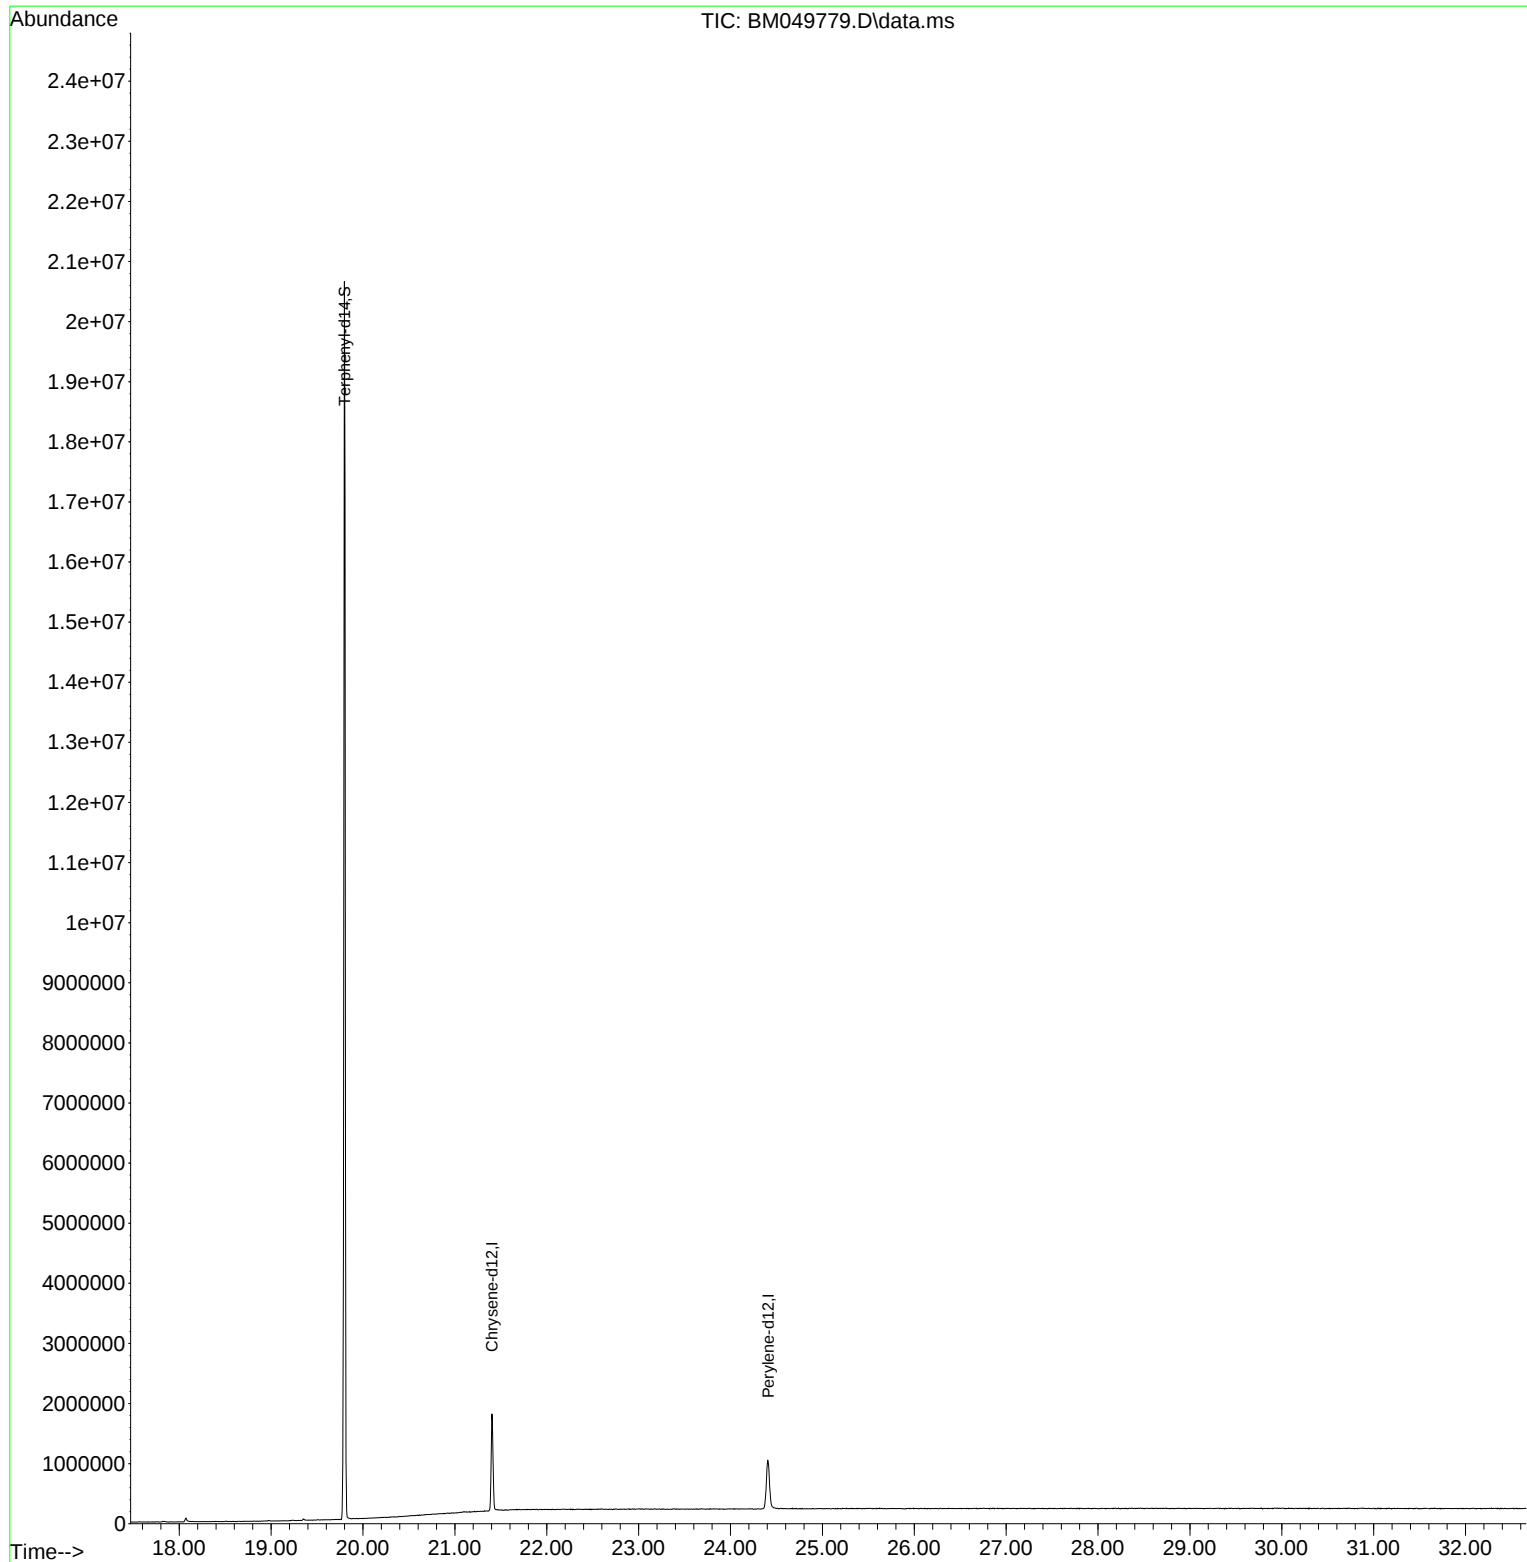


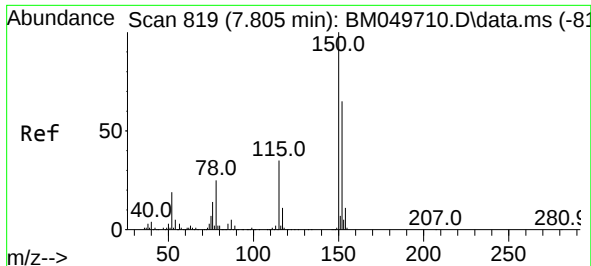

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.792 min Scan# 81
 Delta R.T. -0.013 min
 Lab File: BM049779.D
 Acq: 01 Apr 2025 18:06




Instrument :
 BNA_M
 ClientSampleId :
 TP-6


Tgt Ion:152 Resp: 310337
 Ion Ratio Lower Upper
 152 100
 150 158.3 123.8 185.8
 115 52.5 43.0 64.6

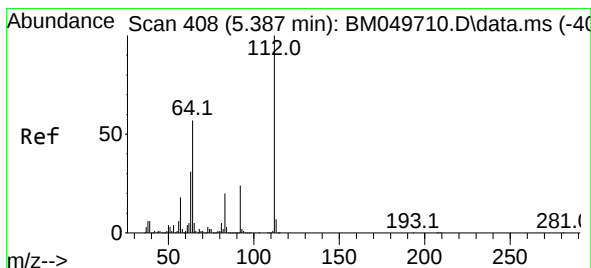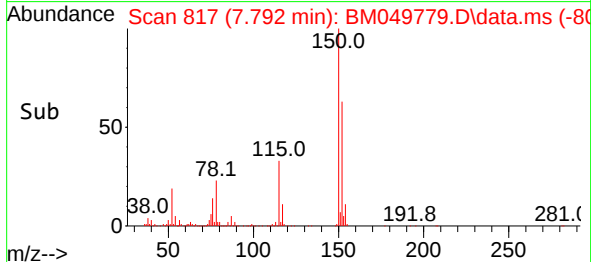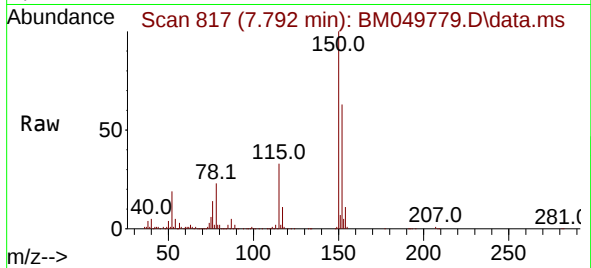

#5
 2-Fluorophenol
 Concen: 195.320 ng
 RT: 5.381 min Scan# 407
 Delta R.T. -0.006 min
 Lab File: BM049779.D
 Acq: 01 Apr 2025 18:06

Tgt Ion:112 Resp: 3592376
 Ion Ratio Lower Upper
 112 100
 64 56.4 45.3 67.9
 63 29.8 24.4 36.6

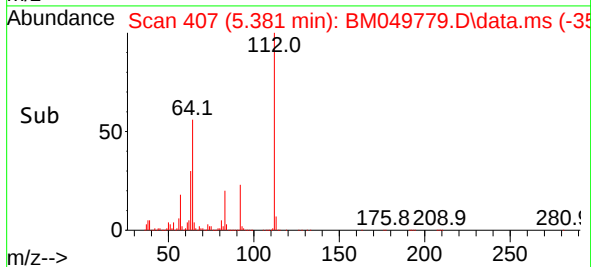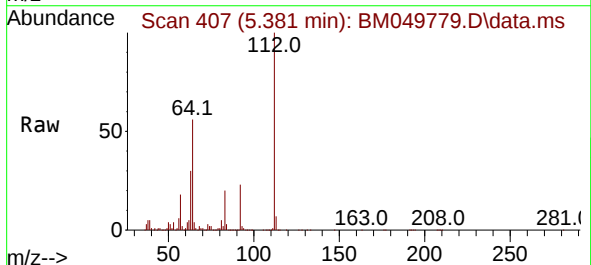




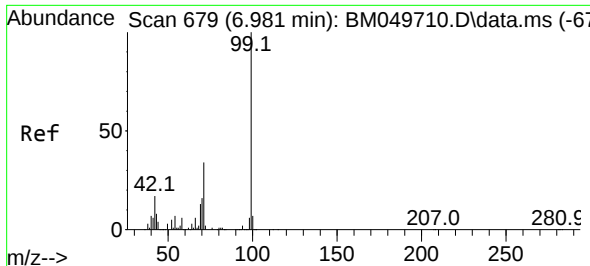


#7
Phenol-d6
Concen: 193.386 ng
RT: 6.969 min Scan# 61
Delta R.T. -0.012 min
Lab File: BM049779.D
Acq: 01 Apr 2025 18:06

Instrument :
BNA_M
ClientSampleId :
TP-6

Tgt Ion: 99 Resp: 4463605




Ion	Ratio	Lower	Upper
99	100		
42	16.8	13.6	20.4
71	32.9	27.0	40.6

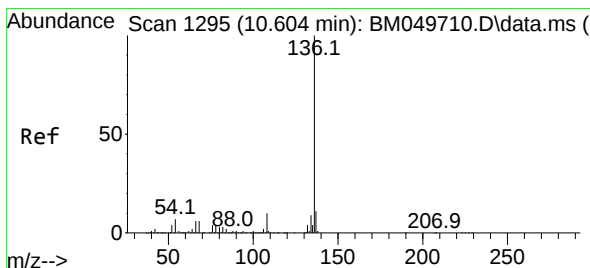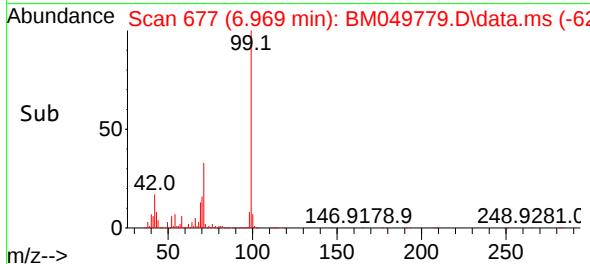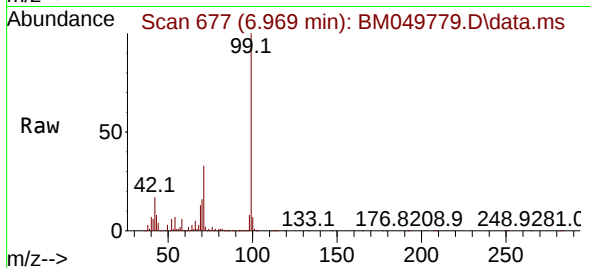


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.586 min Scan# 1292
Delta R.T. -0.018 min
Lab File: BM049779.D
Acq: 01 Apr 2025 18:06

Tgt Ion: 136 Resp: 1060057

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.6	12.8
54	7.5	5.8	8.8
68	6.1	4.5	6.7


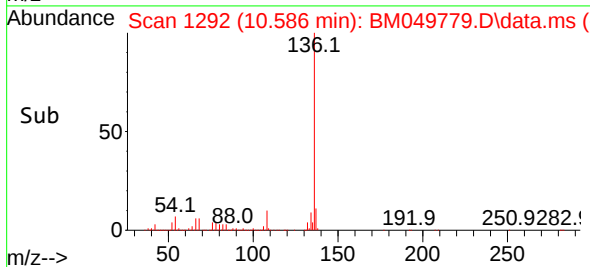

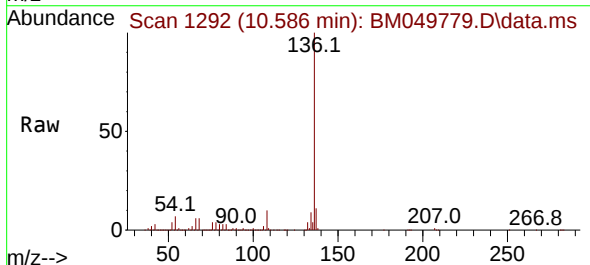


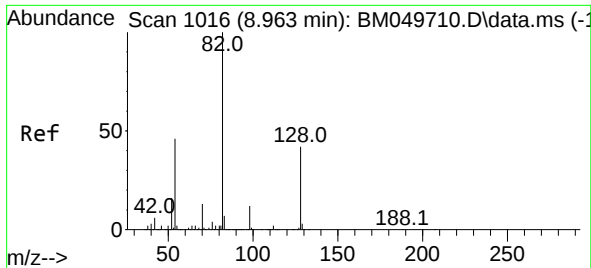

#23
Nitrobenzene-d5
Concen: 129.549 ng
RT: 8.951 min Scan# 1014
Delta R.T. -0.012 min
Lab File: BM049779.D
Acq: 01 Apr 2025 18:06




Instrument :
BNA_M
ClientSampleId :
TP-6


Tgt Ion: 82 Resp: 2674812
Ion Ratio Lower Upper
82 100
128 41.4 33.4 50.0
54 45.2 36.4 54.6

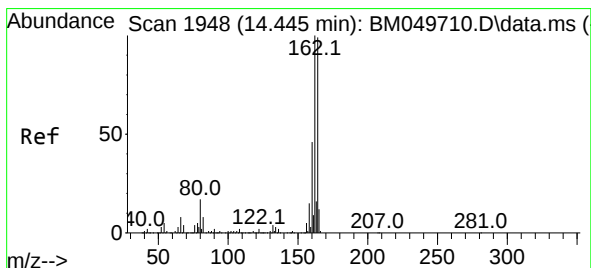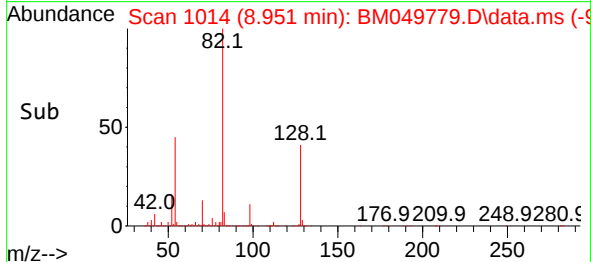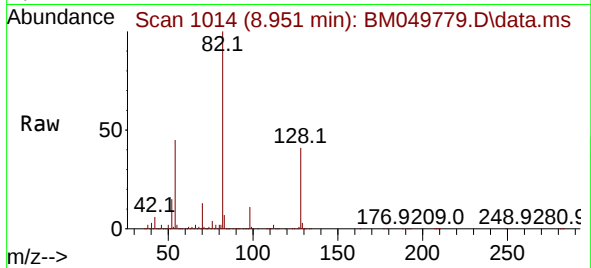

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.433 min Scan# 1946
Delta R.T. -0.012 min
Lab File: BM049779.D
Acq: 01 Apr 2025 18:06

Tgt Ion:164 Resp: 672580
Ion Ratio Lower Upper
164 100
162 101.3 80.5 120.7
160 47.8 36.9 55.3


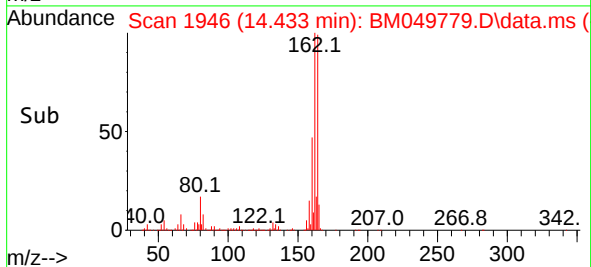

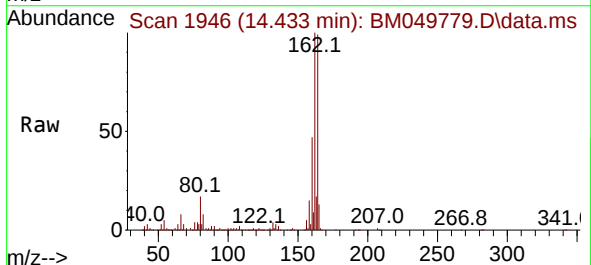


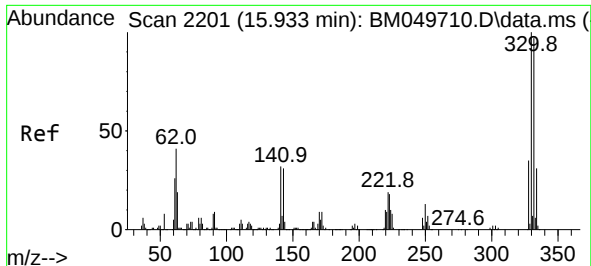

#42
2,4,6-Tribromophenol
Concen: 233.787 ng
RT: 15.921 min Scan# 2199
Delta R.T. -0.012 min
Lab File: BM049779.D
Acq: 01 Apr 2025 18:06




Instrument :
BNA_M
ClientSampleId :
TP-6


Tgt Ion:330 Resp: 1836095
Ion Ratio Lower Upper
330 100
332 95.8 77.0 115.4
141 31.4 27.8 41.6

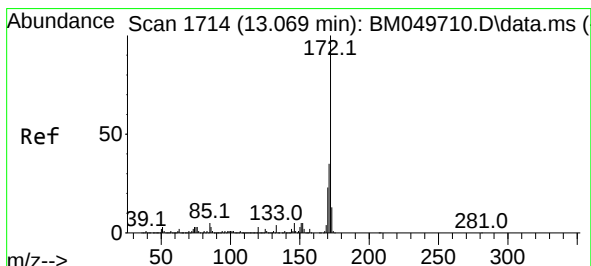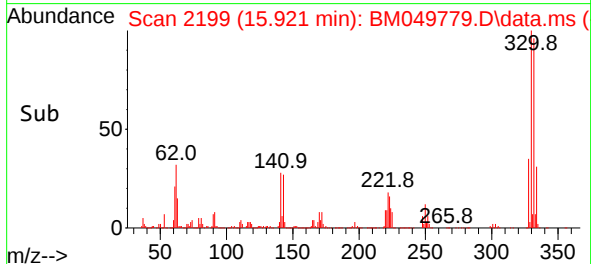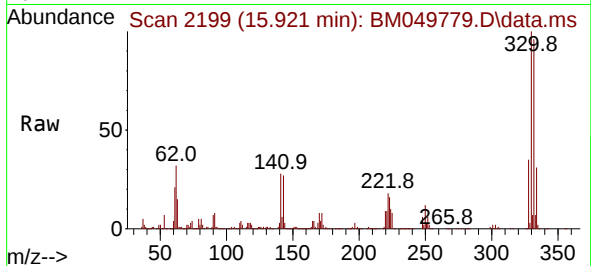

#45
2-Fluorobiphenyl
Concen: 131.433 ng
RT: 13.057 min Scan# 1712
Delta R.T. -0.012 min
Lab File: BM049779.D
Acq: 01 Apr 2025 18:06

Tgt Ion:172 Resp: 7058484
Ion Ratio Lower Upper
172 100
171 35.4 27.9 41.9
170 23.7 18.6 28.0

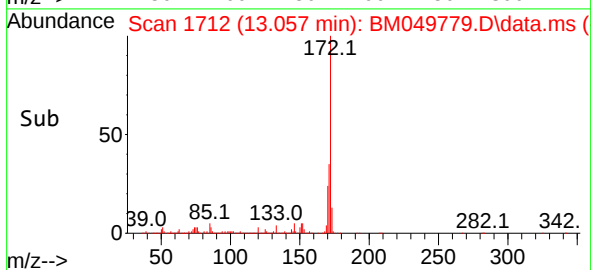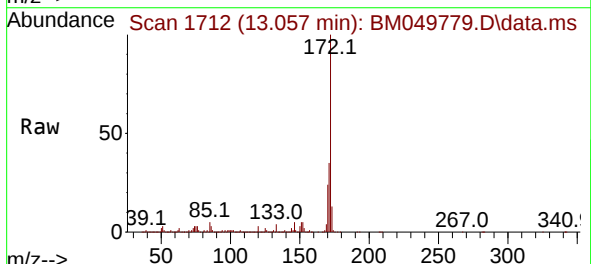

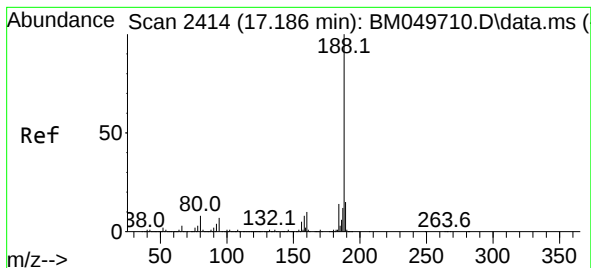

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.174 min Scan# 2414

Delta R.T. -0.012 min

Lab File: BM049779.D

Acq: 01 Apr 2025 18:06

Instrument :

BNA_M

ClientSampleId :

TP-6





Tgt Ion:188 Resp: 1210736

Ion Ratio Lower Upper

188 100

94 7.3 5.8 8.6

80 7.6 6.3 9.5

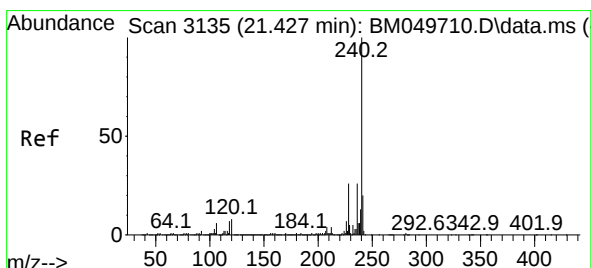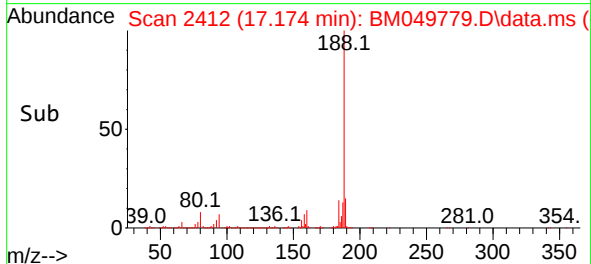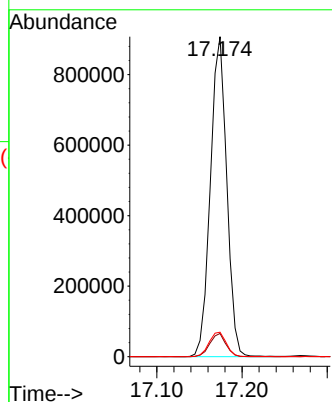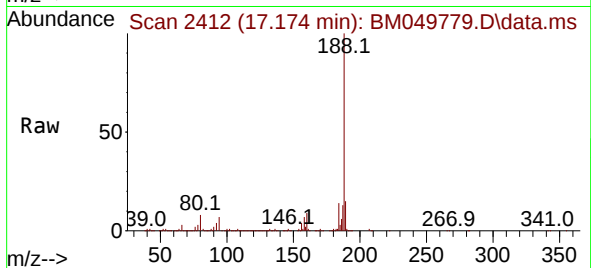

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.403 min Scan# 3131

Delta R.T. -0.024 min

Lab File: BM049779.D

Acq: 01 Apr 2025 18:06




Tgt Ion:240 Resp: 835223


Ion Ratio Lower Upper

240 100

120 8.8 6.5 9.7

236 26.0 20.7 31.1


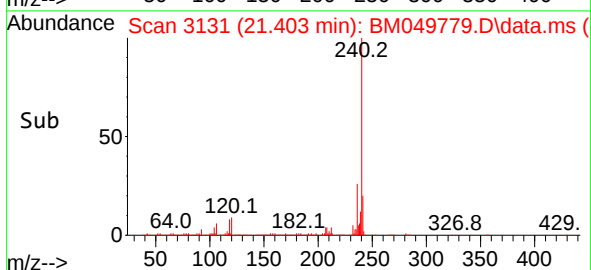

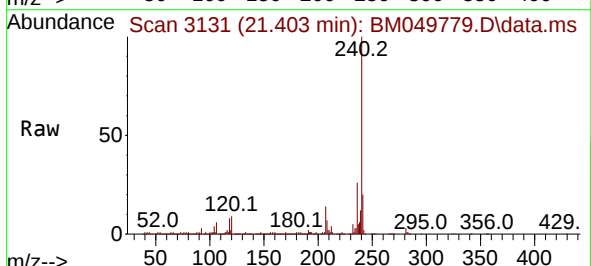


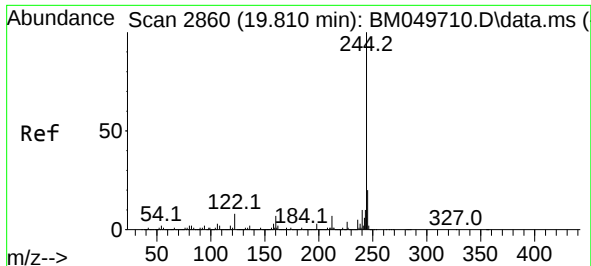

#79
 Terphenyl-d14
 Concen: 175.951 ng
 RT: 19.797 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BM049779.D
 Acq: 01 Apr 2025 18:06

Instrument :
 BNA_M
 ClientSampleId :
 TP-6

Tgt Ion:244 Resp: 8720938
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.6
 122 7.8 6.0 9.0

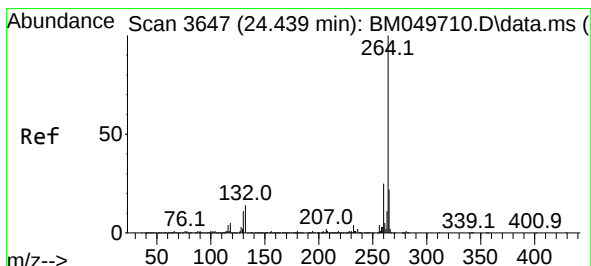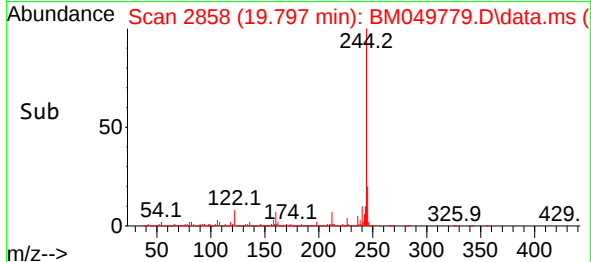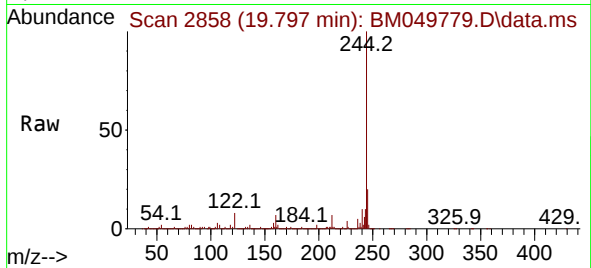

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.409 min Scan# 3642
 Delta R.T. -0.030 min
 Lab File: BM049779.D
 Acq: 01 Apr 2025 18:06

Tgt Ion:264 Resp: 746205
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.6 29.4
 265 21.5 18.2 27.2

