

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040125\  
 Data File : BM049770.D  
 Acq On : 01 Apr 2025 12:15  
 Operator : RC/JU  
 Sample : Q1672-04  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 TP-8

Quant Time: Apr 01 12:57:54 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031325.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Mar 13 14:55:34 2025  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-----------------------------|--------|------|----------|---------|-------|----------|
| -----                       |        |      |          |         |       |          |
| Internal Standards          |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.792  | 152  | 322537   | 20.000  | ng    | -0.01    |
| 21) Naphthalene-d8          | 10.586 | 136  | 1098091  | 20.000  | ng    | -0.02    |
| 39) Acenaphthene-d10        | 14.433 | 164  | 667617   | 20.000  | ng    | -0.01    |
| 64) Phenanthrene-d10        | 17.174 | 188  | 1169902  | 20.000  | ng    | -0.01    |
| 76) Chrysene-d12            | 21.409 | 240  | 839213   | 20.000  | ng    | -0.02    |
| 86) Perylene-d12            | 24.409 | 264  | 776759   | 20.000  | ng    | -0.03    |
|                             |        |      |          |         |       |          |
| System Monitoring Compounds |        |      |          |         |       |          |
| 5) 2-Fluorophenol           | 5.381  | 112  | 3052572  | 159.693 | ng    | 0.00     |
| 7) Phenol-d6                | 6.969  | 99   | 3678927  | 153.361 | ng    | -0.01    |
| 23) Nitrobenzene-d5         | 8.951  | 82   | 2312863  | 108.139 | ng    | -0.01    |
| 42) 2,4,6-Tribromophenol    | 15.921 | 330  | 1407034  | 180.487 | ng    | -0.01    |
| 45) 2-Fluorobiphenyl        | 13.057 | 172  | 5618873  | 105.404 | ng    | -0.01    |
| 79) Terphenyl-d14           | 19.797 | 244  | 7170132  | 143.975 | ng    | -0.01    |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040125\  
Data File : BM049770.D  
Acq On : 01 Apr 2025 12:15  
Operator : RC/JU  
Sample : Q1672-04  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
TP-8

Quant Time: Apr 01 12:57:54 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 13 14:55:34 2025  
Response via : Initial Calibration

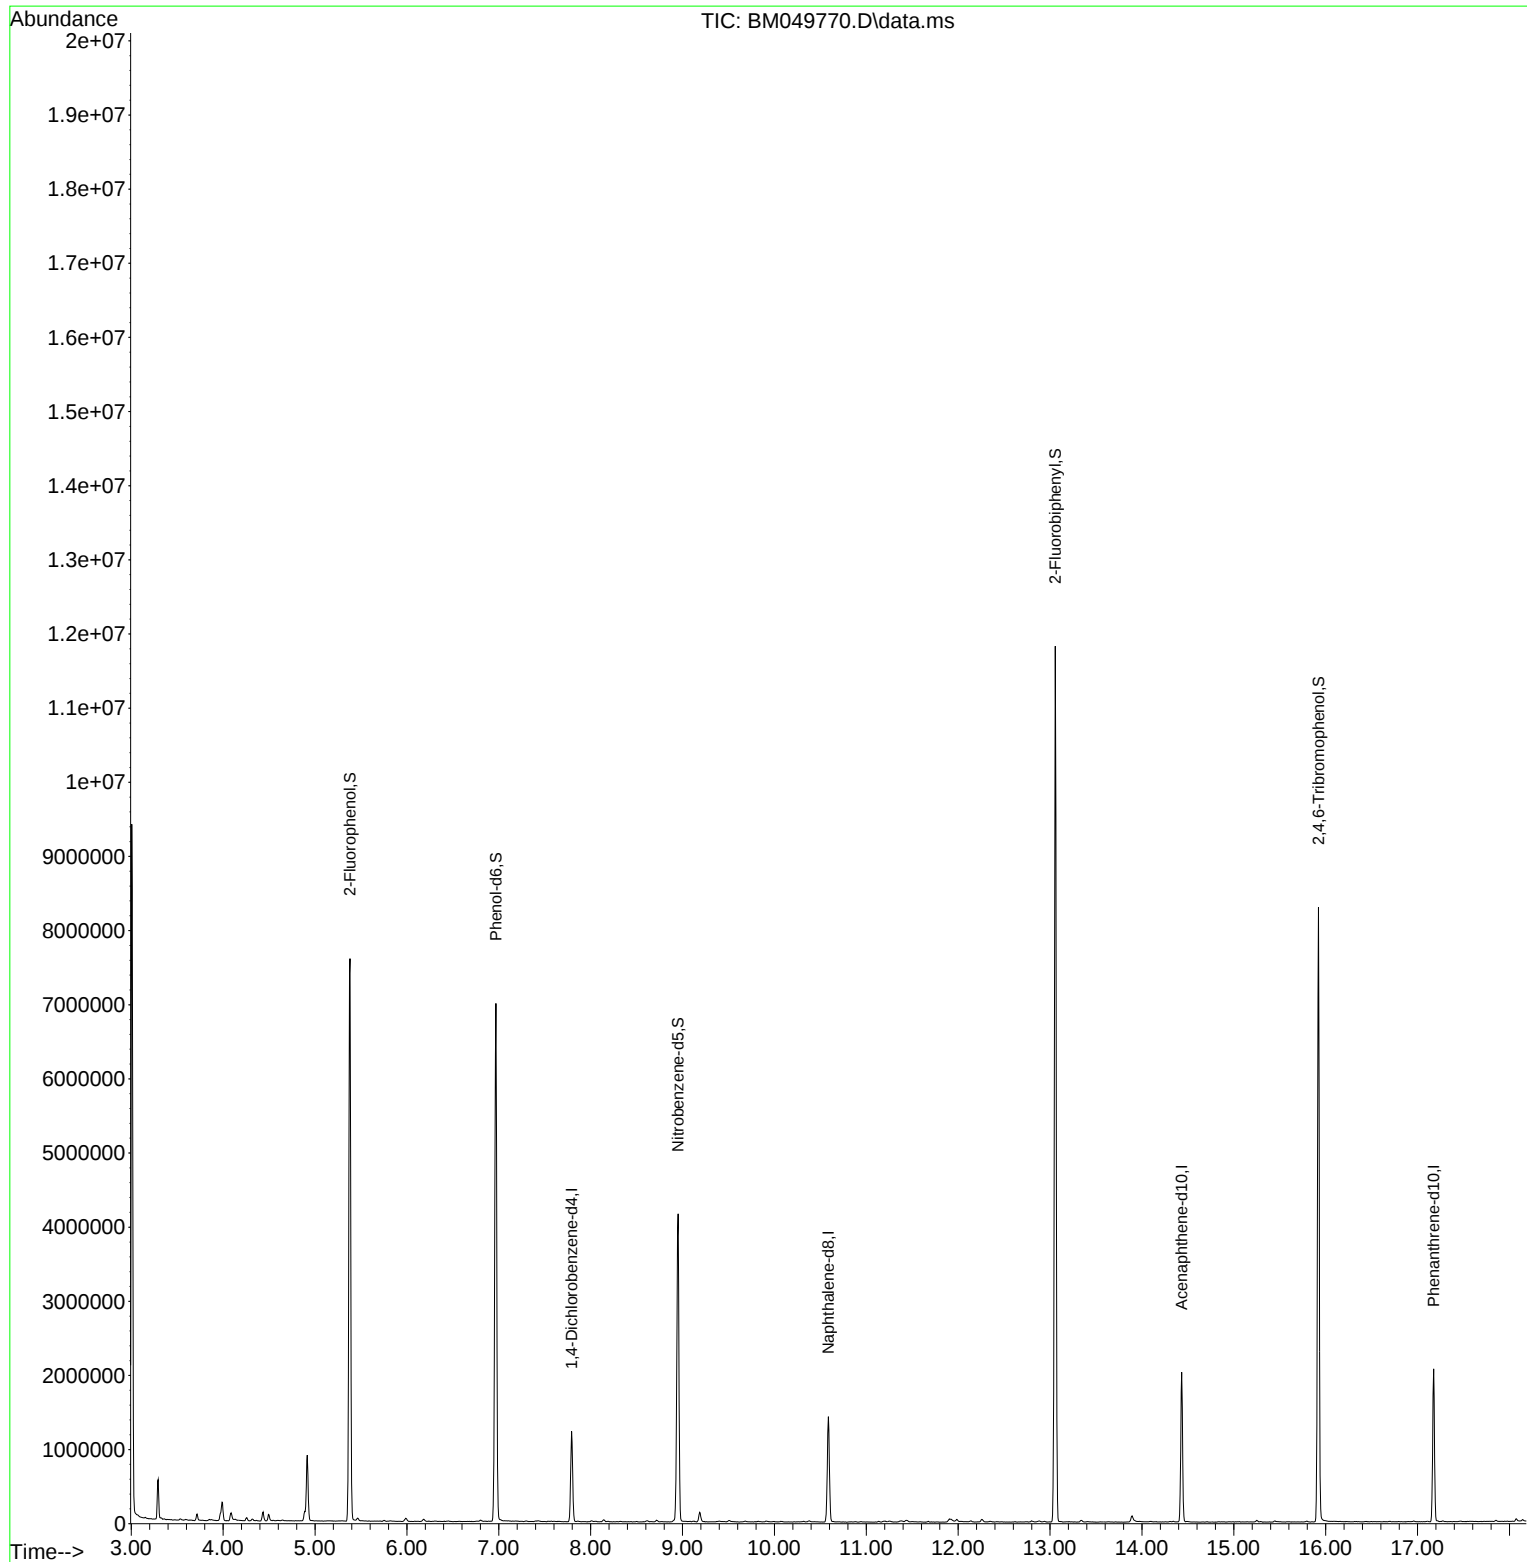

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040125\  
Data File : BM049770.D  
Acq On : 01 Apr 2025 12:15  
Operator : RC/JU  
Sample : Q1672-04  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
TP-8

Quant Time: Apr 01 12:57:54 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 13 14:55:34 2025  
Response via : Initial Calibration

