

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040125\
 Data File : BM049771.D
 Acq On : 01 Apr 2025 12:54
 Operator : RC/JU
 Sample : Q1597-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 1-CONCRETE-SLAB

Quant Time: Apr 01 13:42:59 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 13 14:55:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	314201	20.000	ng	-0.01
21) Naphthalene-d8	10.586	136	1089882	20.000	ng	-0.02
39) Acenaphthene-d10	14.433	164	721540	20.000	ng	-0.01
64) Phenanthrene-d10	17.174	188	1329740	20.000	ng	-0.01
76) Chrysene-d12	21.409	240	950939	20.000	ng	-0.02
86) Perylene-d12	24.409	264	831342	20.000	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.375	112	1003399	53.885	ng	-0.01
7) Phenol-d6	6.963	99	1534579	65.668	ng	-0.02
23) Nitrobenzene-d5	8.945	82	1097966	51.723	ng	-0.02
42) 2,4,6-Tribromophenol	15.915	330	352116	41.792	ng	-0.02
45) 2-Fluorobiphenyl	13.057	172	3001300	52.094	ng	-0.01
79) Terphenyl-d14	19.798	244	3963178	70.230	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040125\
Data File : BM049771.D
Acq On : 01 Apr 2025 12:54
Operator : RC/JU
Sample : Q1597-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
1-CONCRETE-SLAB


Quant Time: Apr 01 13:42:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

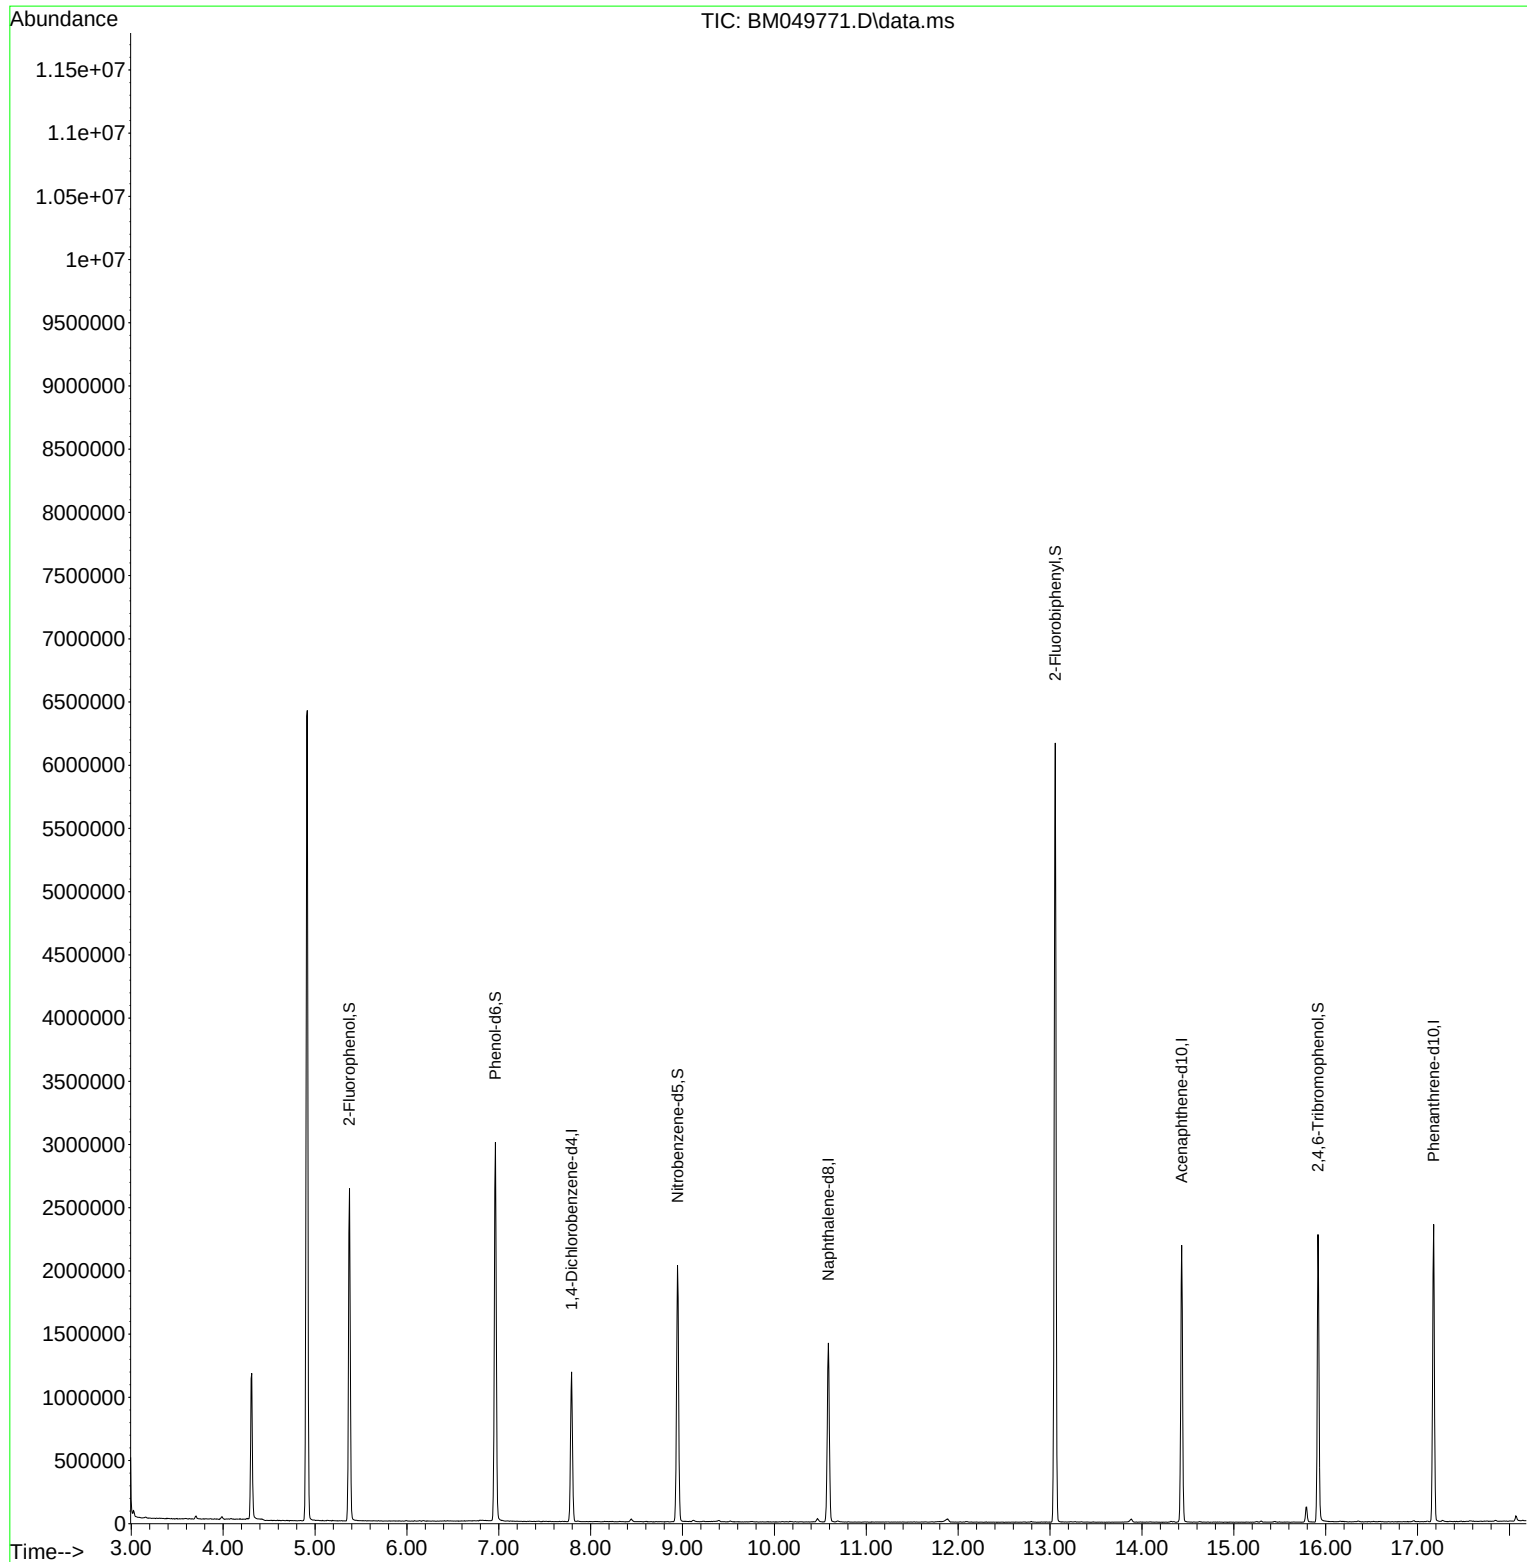


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040125\
Data File : BM049771.D
Acq On : 01 Apr 2025 12:54
Operator : RC/JU
Sample : Q1597-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
1-CONCRETE-SLAB

Quant Time: Apr 01 13:42:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration




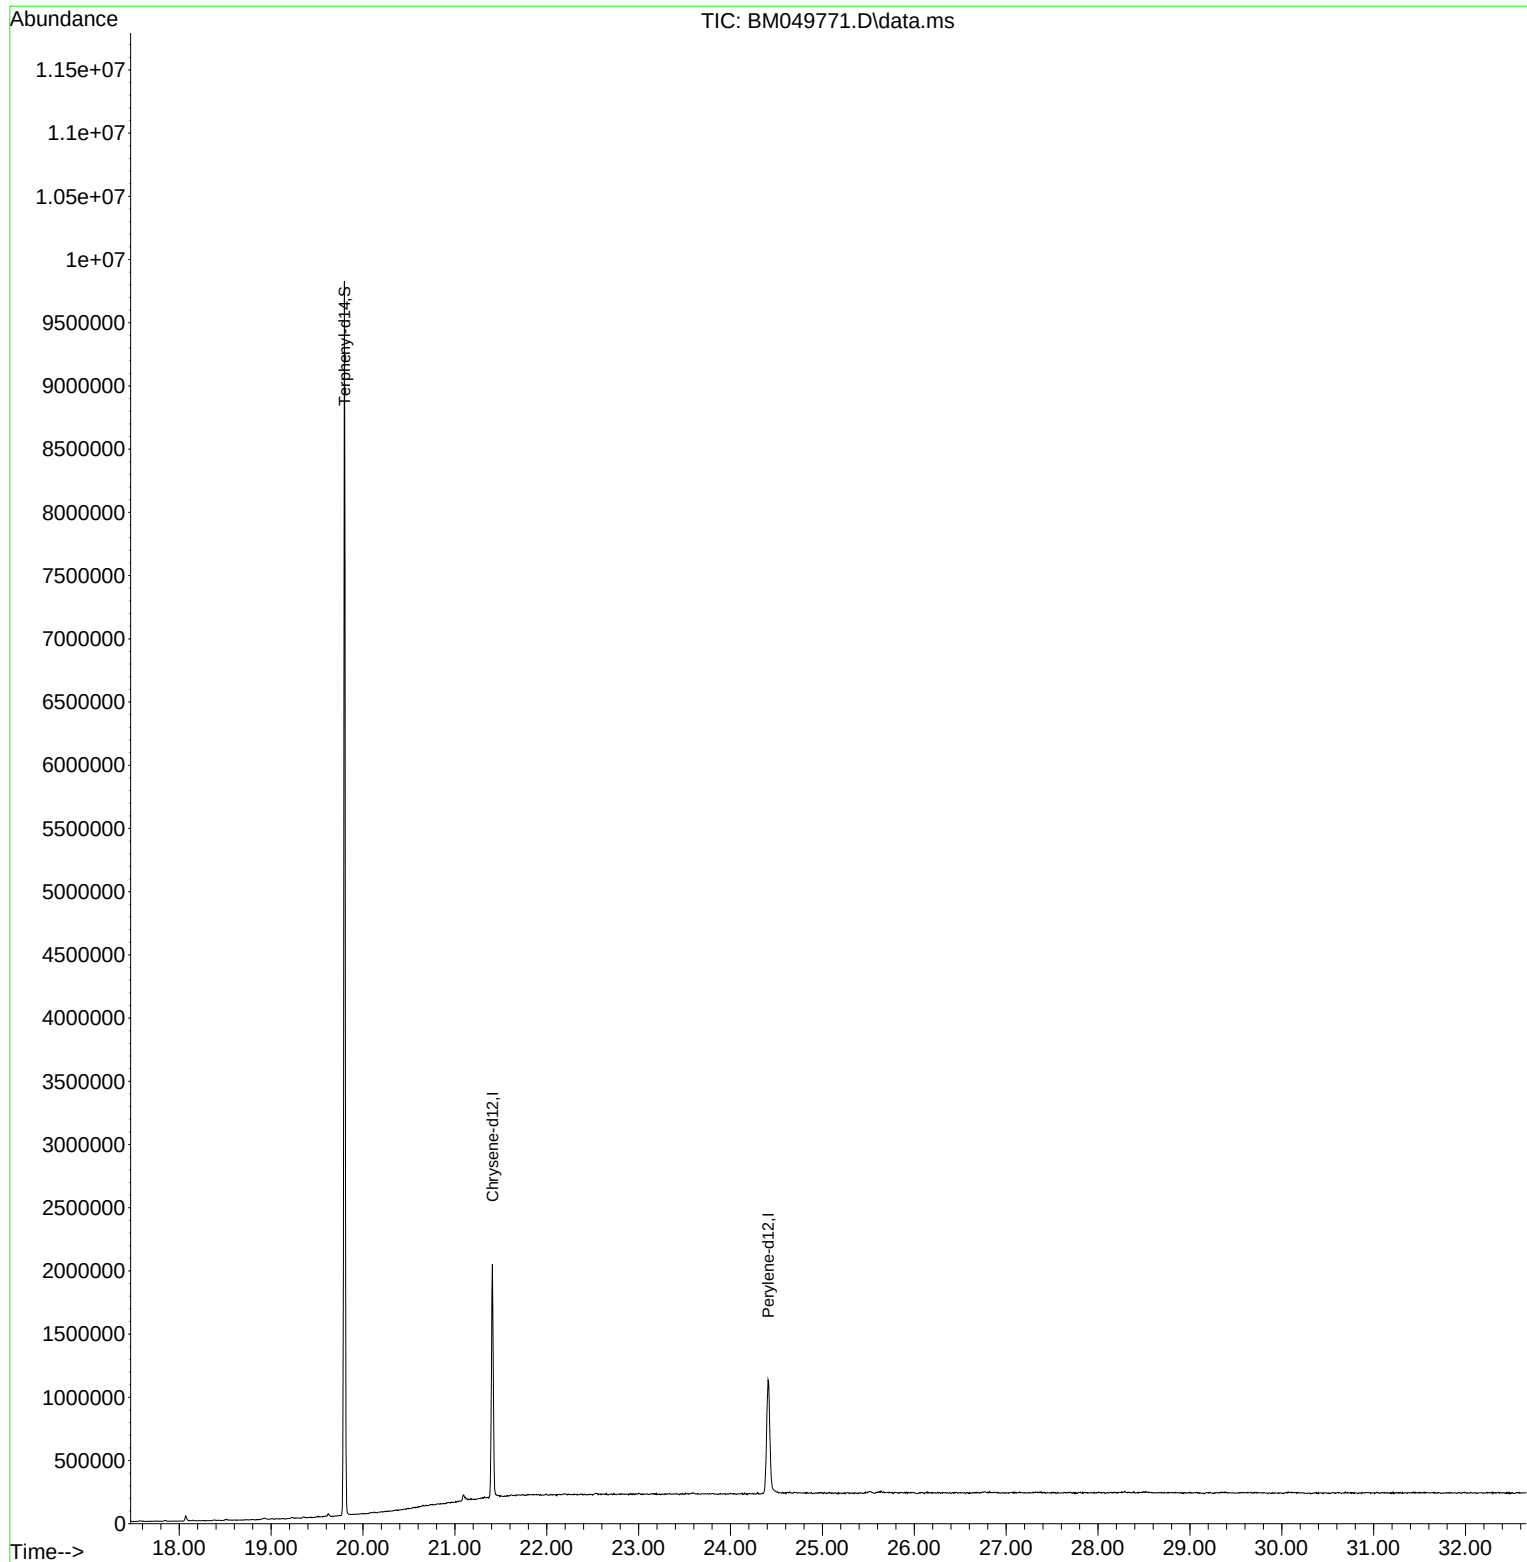


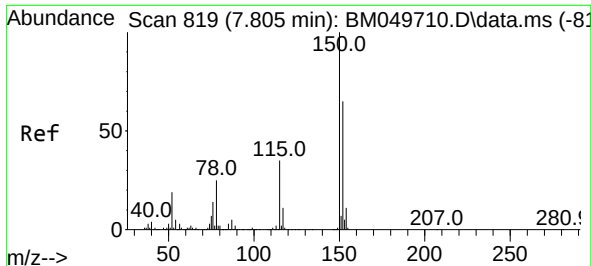

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.792 min Scan# 819
Delta R.T. -0.013 min
Lab File: BM049771.D
Acq: 01 Apr 2025 12:54




Instrument :
BNA_M
ClientSampleId :
1-CONCRETE-SLAB


Tgt Ion:152 Resp: 314201
Ion Ratio Lower Upper
152 100
150 154.1 123.8 185.8
115 52.3 43.0 64.6

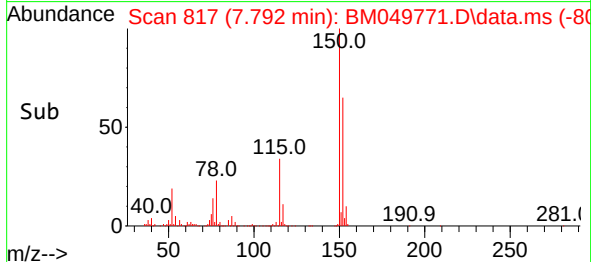

#5
2-Fluorophenol
Concen: 53.885 ng
RT: 5.375 min Scan# 406
Delta R.T. -0.012 min
Lab File: BM049771.D
Acq: 01 Apr 2025 12:54

Tgt Ion:112 Resp: 1003399
Ion Ratio Lower Upper
112 100
64 56.6 45.3 67.9
63 30.3 24.4 36.6


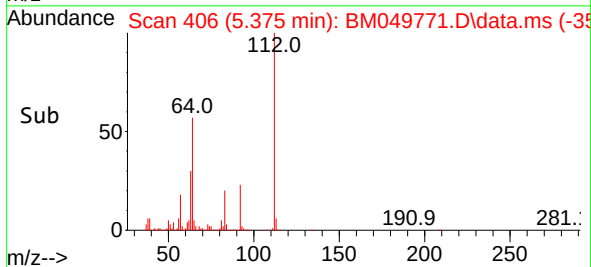

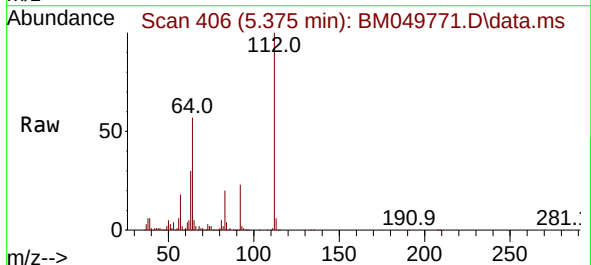


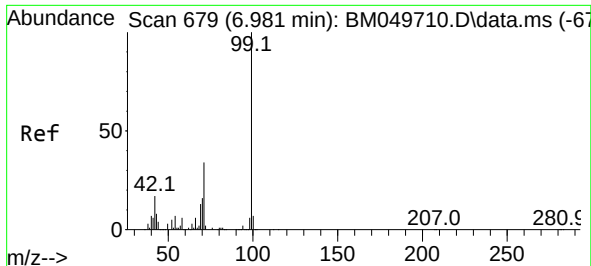

#7
Phenol-d6
Concen: 65.668 ng
RT: 6.963 min Scan# 61
Delta R.T. -0.018 min
Lab File: BM049771.D
Acq: 01 Apr 2025 12:54




Instrument :
BNA_M
ClientSampleId :
1-CONCRETE-SLAB


Tgt Ion: 99 Resp: 1534579
Ion Ratio Lower Upper
99 100
42 18.0 13.6 20.4
71 33.6 27.0 40.6

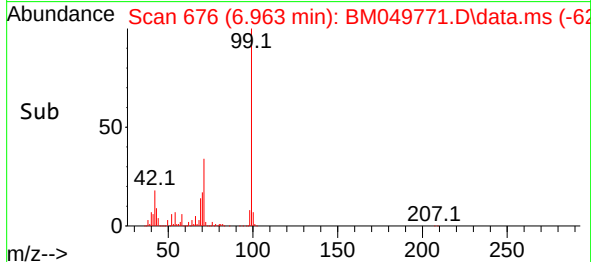

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.586 min Scan# 1292
Delta R.T. -0.018 min
Lab File: BM049771.D
Acq: 01 Apr 2025 12:54

Tgt Ion: 136 Resp: 1089882
Ion Ratio Lower Upper
136 100
137 10.7 8.6 12.8
54 7.5 5.8 8.8
68 5.8 4.5 6.7

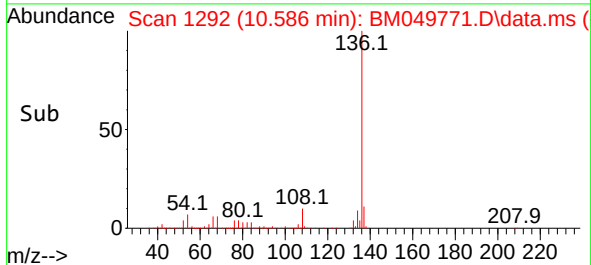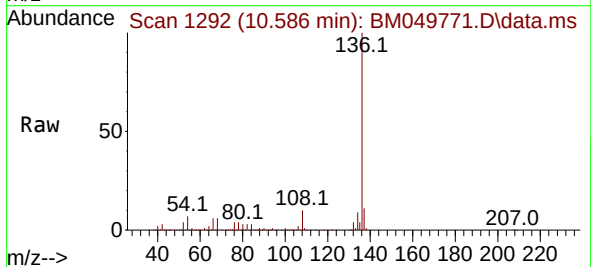



#23

Nitrobenzene-d5

Concen: 51.723 ng

RT: 8.945 min Scan# 1013

Delta R.T. -0.018 min

Lab File: BM049771.D

Acq: 01 Apr 2025 12:54

Instrument :

BNA_M

ClientSampleId :

1-CONCRETE-SLAB





Tgt Ion: 82 Resp: 1097966

Ion Ratio Lower Upper

82 100

128 40.5 33.4 50.0

54 46.8 36.4 54.6

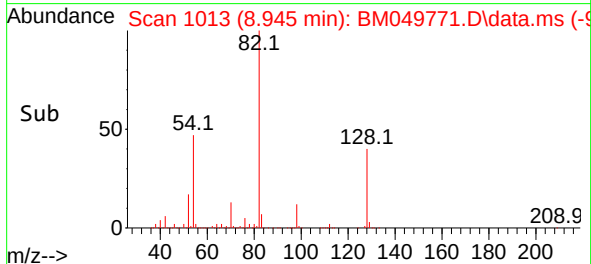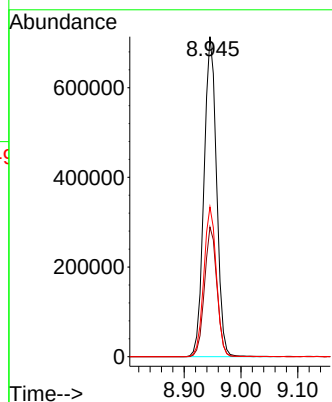

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.433 min Scan# 1946

Delta R.T. -0.012 min

Lab File: BM049771.D

Acq: 01 Apr 2025 12:54




Tgt Ion:164 Resp: 721540


Ion Ratio Lower Upper

164 100

162 99.4 80.5 120.7

160 45.6 36.9 55.3




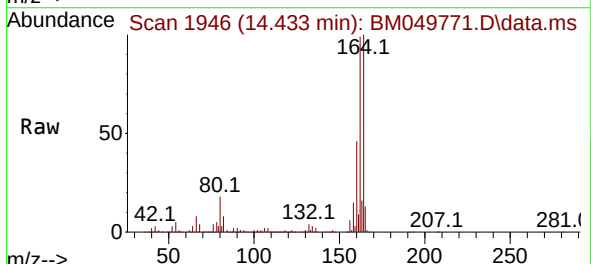




#42
 2,4,6-Tribromophenol
 Concen: 41.792 ng
 RT: 15.915 min Scan# 211
 Delta R.T. -0.018 min
 Lab File: BM049771.D
 Acq: 01 Apr 2025 12:54




Instrument :
 BNA_M
 ClientSampleId :
 1-CONCRETE-SLAB


Tgt Ion:330 Resp: 352116
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.0 115.4
 141 36.9 27.8 41.6

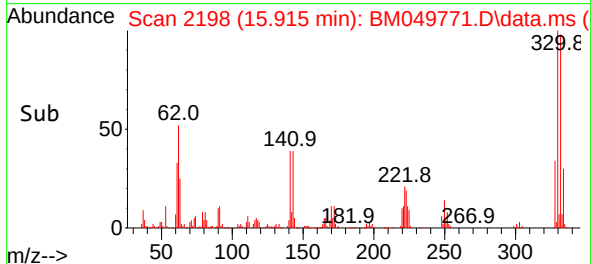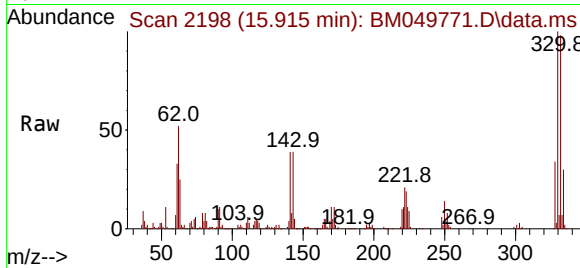

#45
 2-Fluorobiphenyl
 Concen: 52.094 ng
 RT: 13.057 min Scan# 1712
 Delta R.T. -0.012 min
 Lab File: BM049771.D
 Acq: 01 Apr 2025 12:54

Tgt Ion:172 Resp: 3001300
 Ion Ratio Lower Upper
 172 100
 171 34.8 27.9 41.9
 170 23.5 18.6 28.0


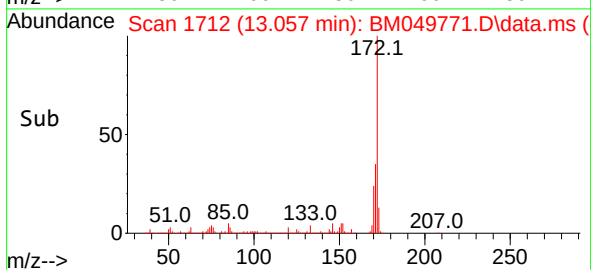

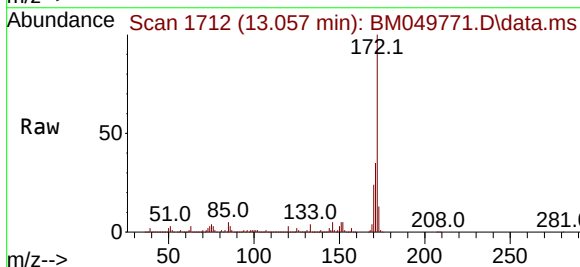


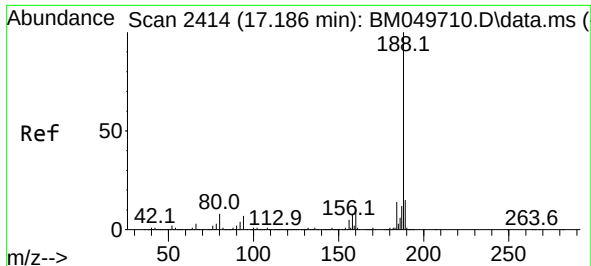

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.174 min Scan# 2414
Delta R.T. -0.012 min
Lab File: BM049771.D
Acq: 01 Apr 2025 12:54




Instrument :
BNA_M
ClientSampleId :
1-CONCRETE-SLAB


Tgt Ion:188 Resp: 1329740
Ion Ratio Lower Upper
188 100
94 7.0 5.8 8.6
80 8.0 6.3 9.5

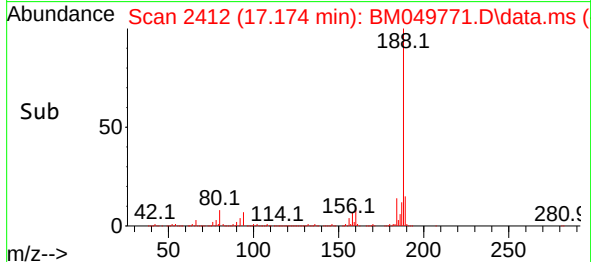

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.409 min Scan# 3132
Delta R.T. -0.018 min
Lab File: BM049771.D
Acq: 01 Apr 2025 12:54

Tgt Ion:240 Resp: 950939
Ion Ratio Lower Upper
240 100
120 8.4 6.5 9.7
236 25.9 20.7 31.1


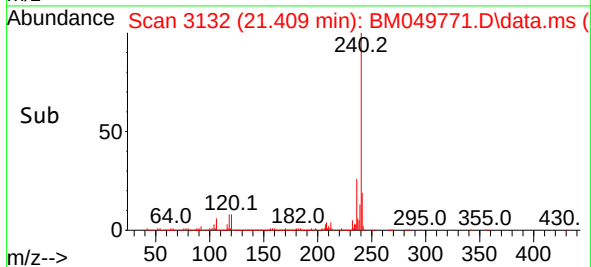

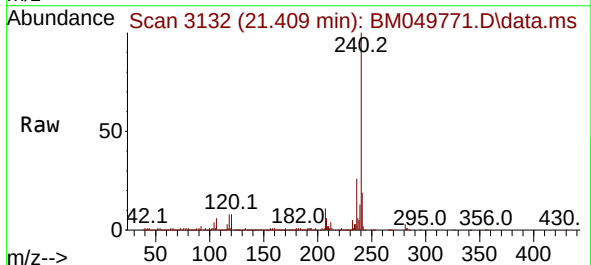


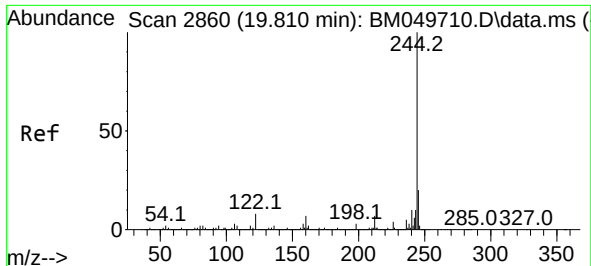

#79
 Terphenyl-d14
 Concen: 70.230 ng
 RT: 19.798 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BM049771.D
 Acq: 01 Apr 2025 12:54

Instrument :
 BNA_M
 ClientSampleId :
 1-CONCRETE-SLAB

Tgt Ion:244 Resp: 3963178
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.6
 122 7.9 6.0 9.0

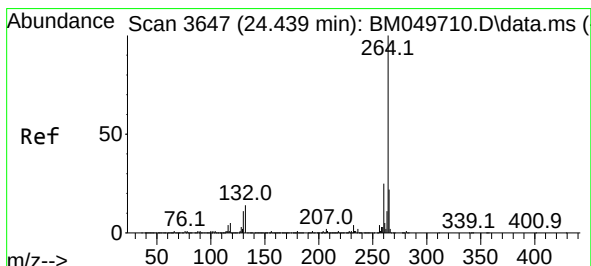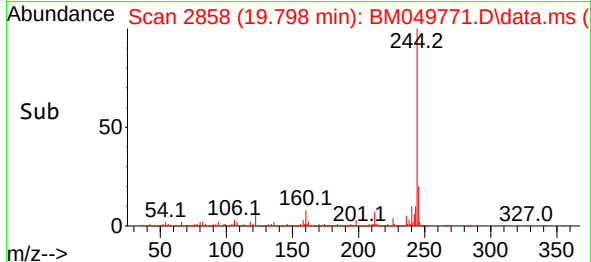

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.409 min Scan# 3642
 Delta R.T. -0.030 min
 Lab File: BM049771.D
 Acq: 01 Apr 2025 12:54

Tgt Ion:264 Resp: 831342
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.6 29.4
 265 22.0 18.2 27.2

