


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040125\
Data File : BM049766.D
Acq On : 01 Apr 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 14:55:34 2025

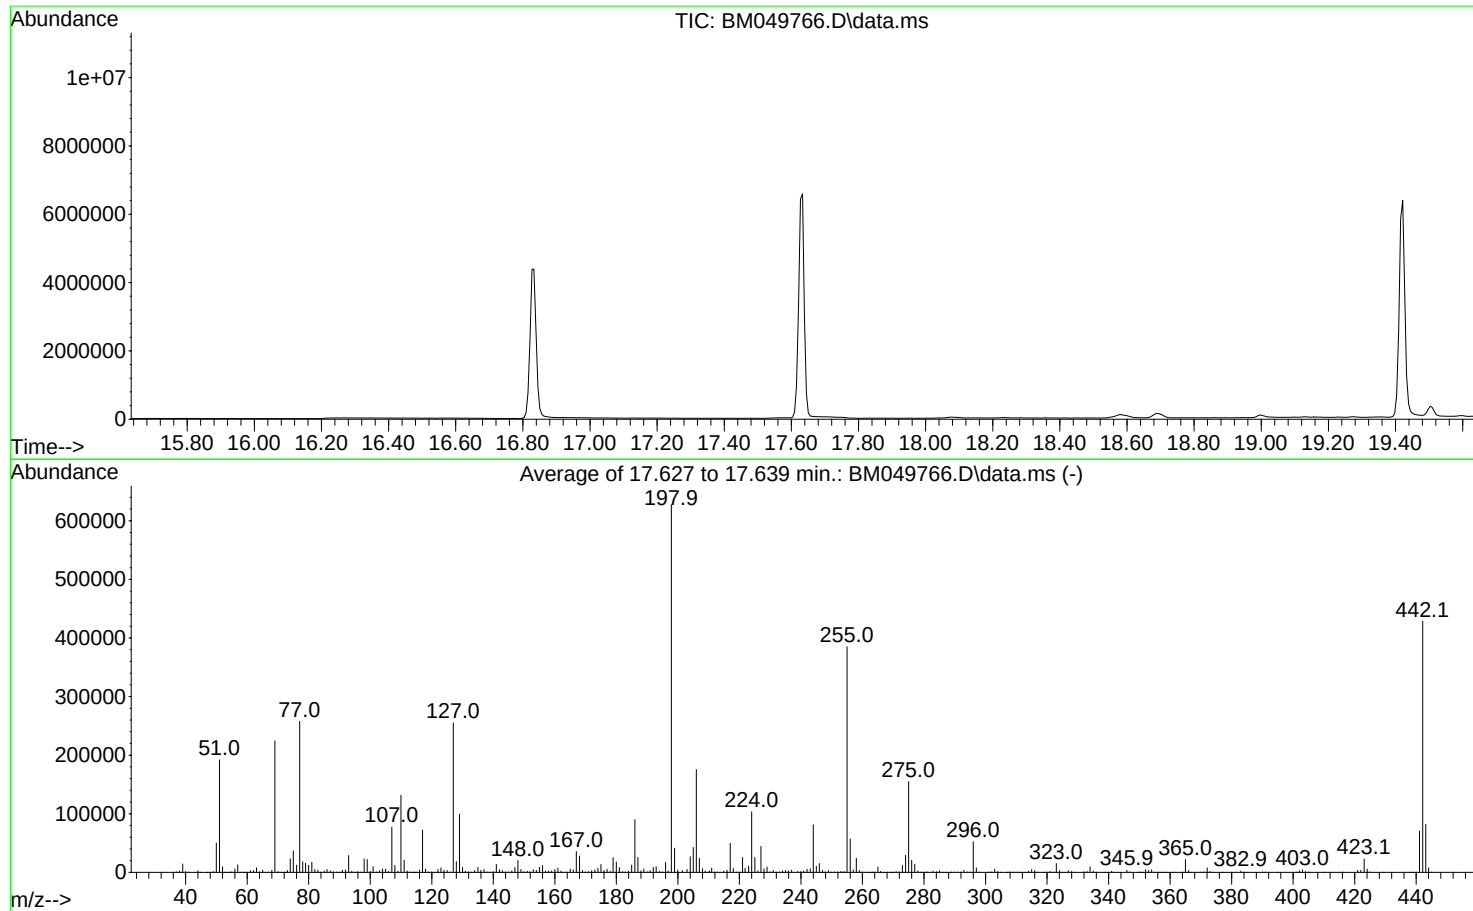

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	192060	PASS
68	69	0.00	2	1.6	3682	PASS
69	198	0.00	100	35.8	224568	PASS
70	69	0.00	2	0.6	1260	PASS
127	198	10	80	40.6	254925	PASS
197	198	0.00	2	0.4	2614	PASS
198	198	100	100	100.0	627797	PASS
199	198	5	9	6.6	41243	PASS
275	198	10	60	24.7	154787	PASS
365	198	1	100	3.5	21849	PASS
441	198	0.01	100	11.2	70507	PASS
442	442	50	100	100.0	428352	PASS
443	442	15	24	19.1	81939	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/1/2025	BNA_M	<u>BM049766.D</u>
Compound Name	Response	Retention Time
DDT	2298205	20.662
DDD	16804	20.274
DDE	1592	19.715
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18396	2316601	0.79

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040125\
Data File : BM049766.D
Acq On : 01 Apr 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 01 11:43:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

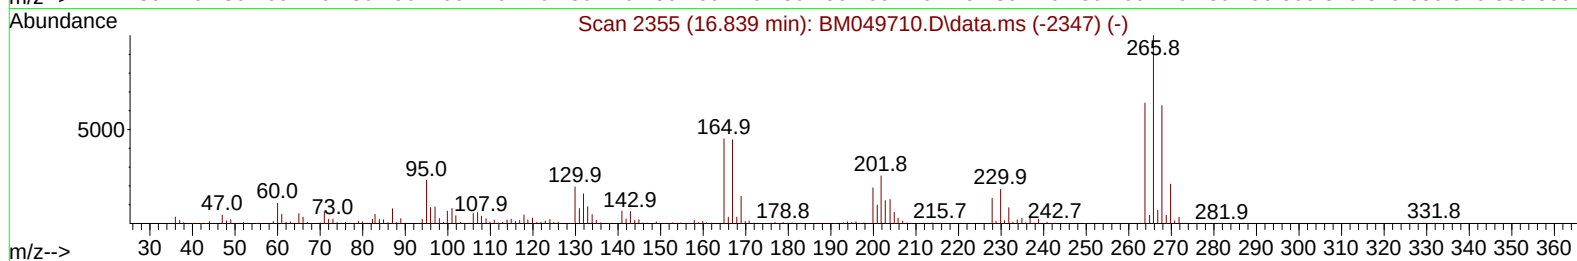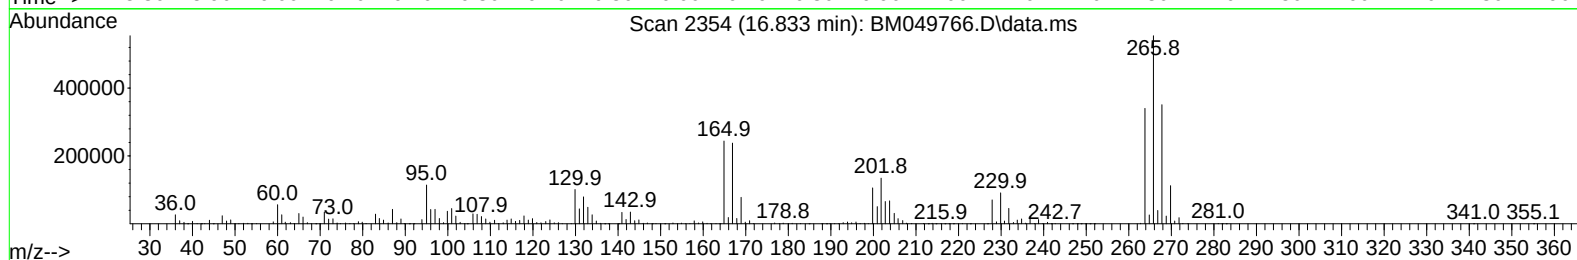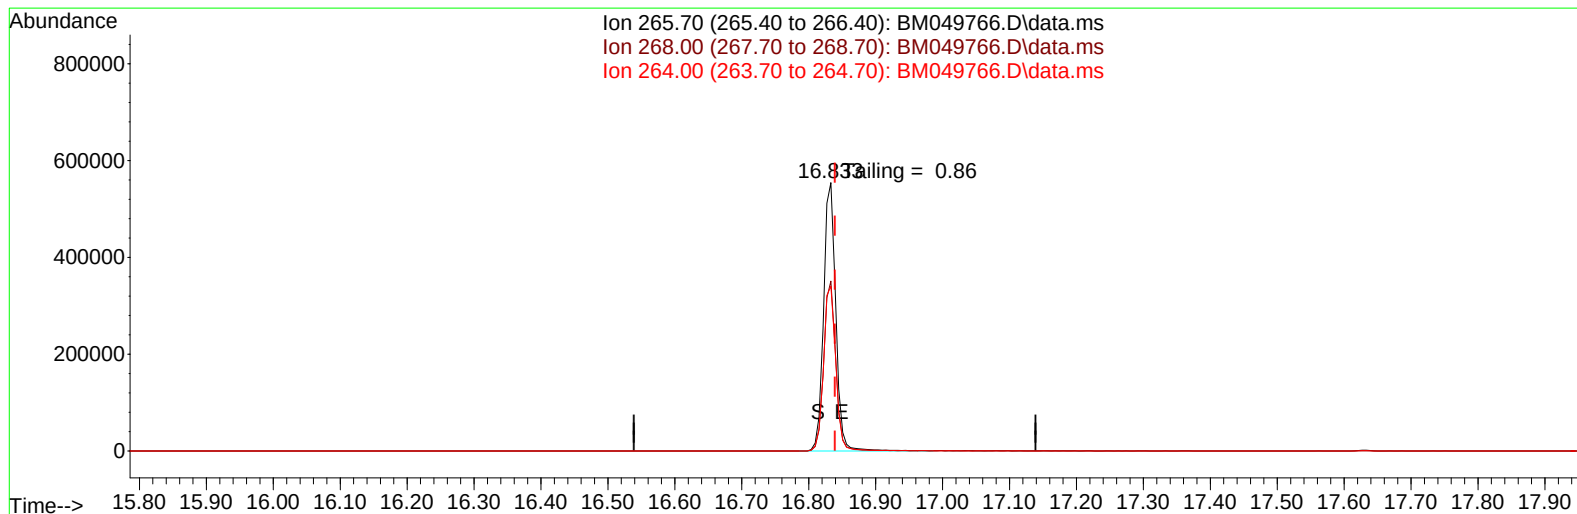

TIC: BM049766.D\data.ms

(70) Pentachlorophenol (C)

16.833min (-0.006) 85476.14 ng




response 700196

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.34
264.00	64.10	61.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040125\
Data File : BM049766.D
Acq On : 01 Apr 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 01 11:43:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

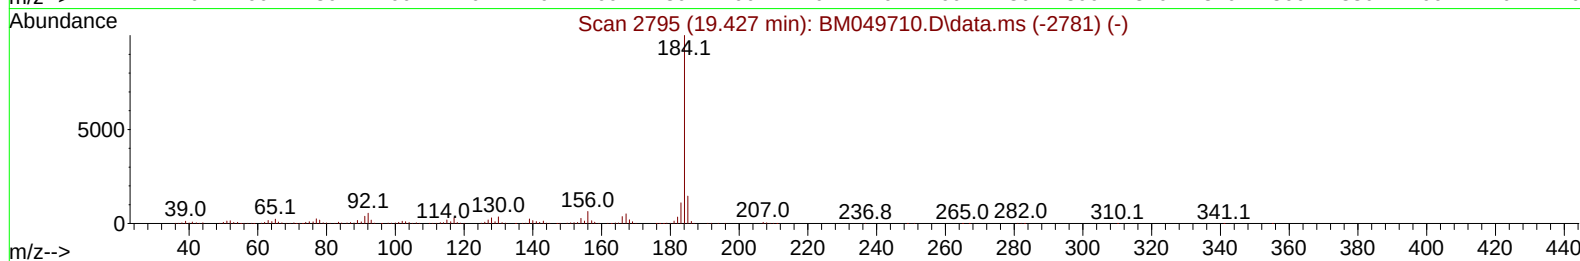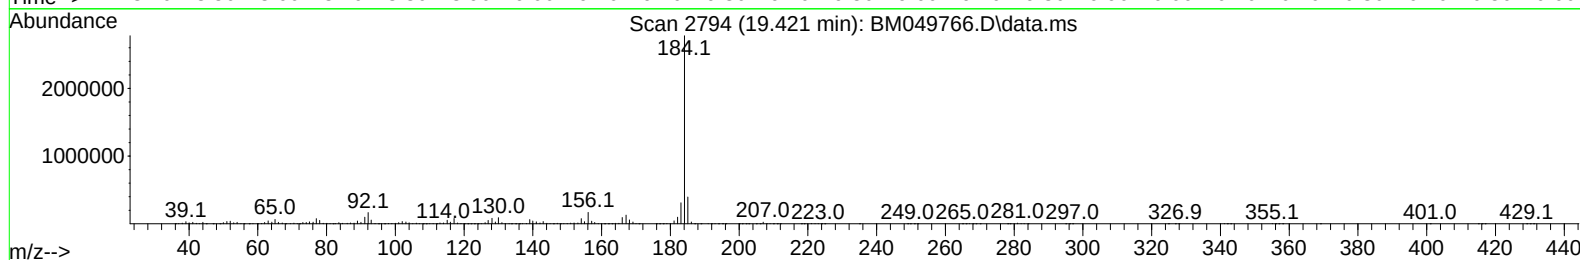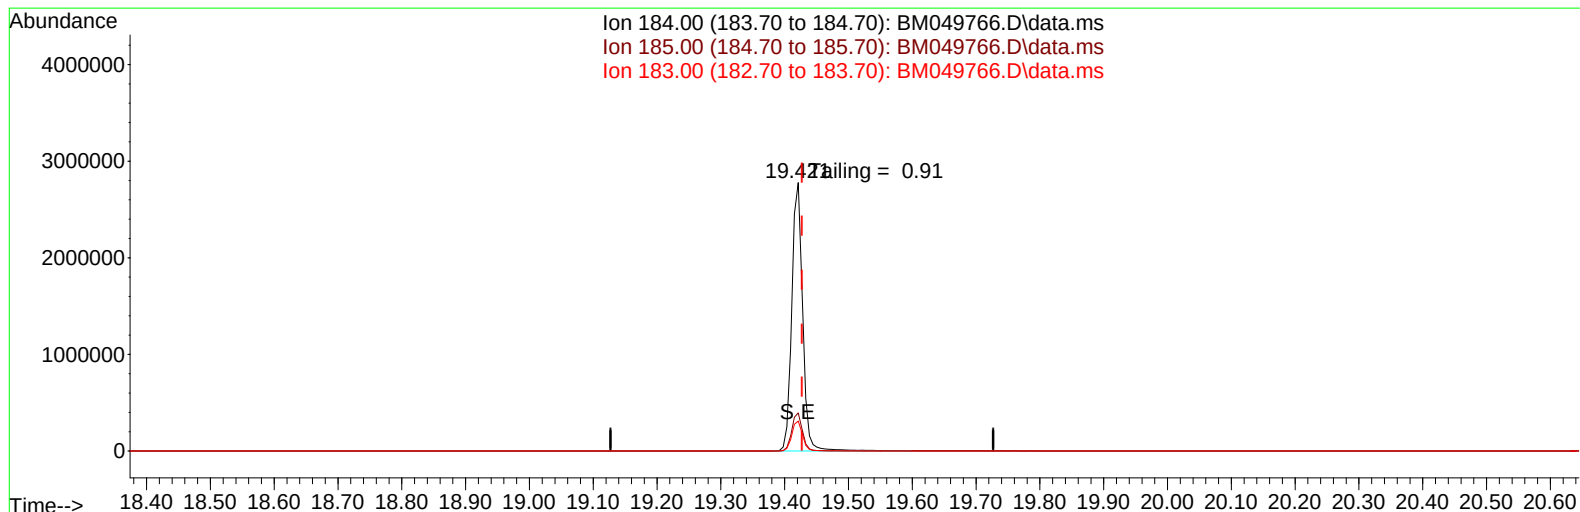

TIC: BM049766.D\data.ms

(77) Benzidine

19.421min (-0.006) 26283.94 ng

response 3296061

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.22
183.00	11.00	11.17
0.00	0.00	0.00