


Data Path : Z:\HPCHEM1\BNA_M\Data\BM040215\
 Data File : BM000805.D
 Acq On : 02 Apr 2015 09:36
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

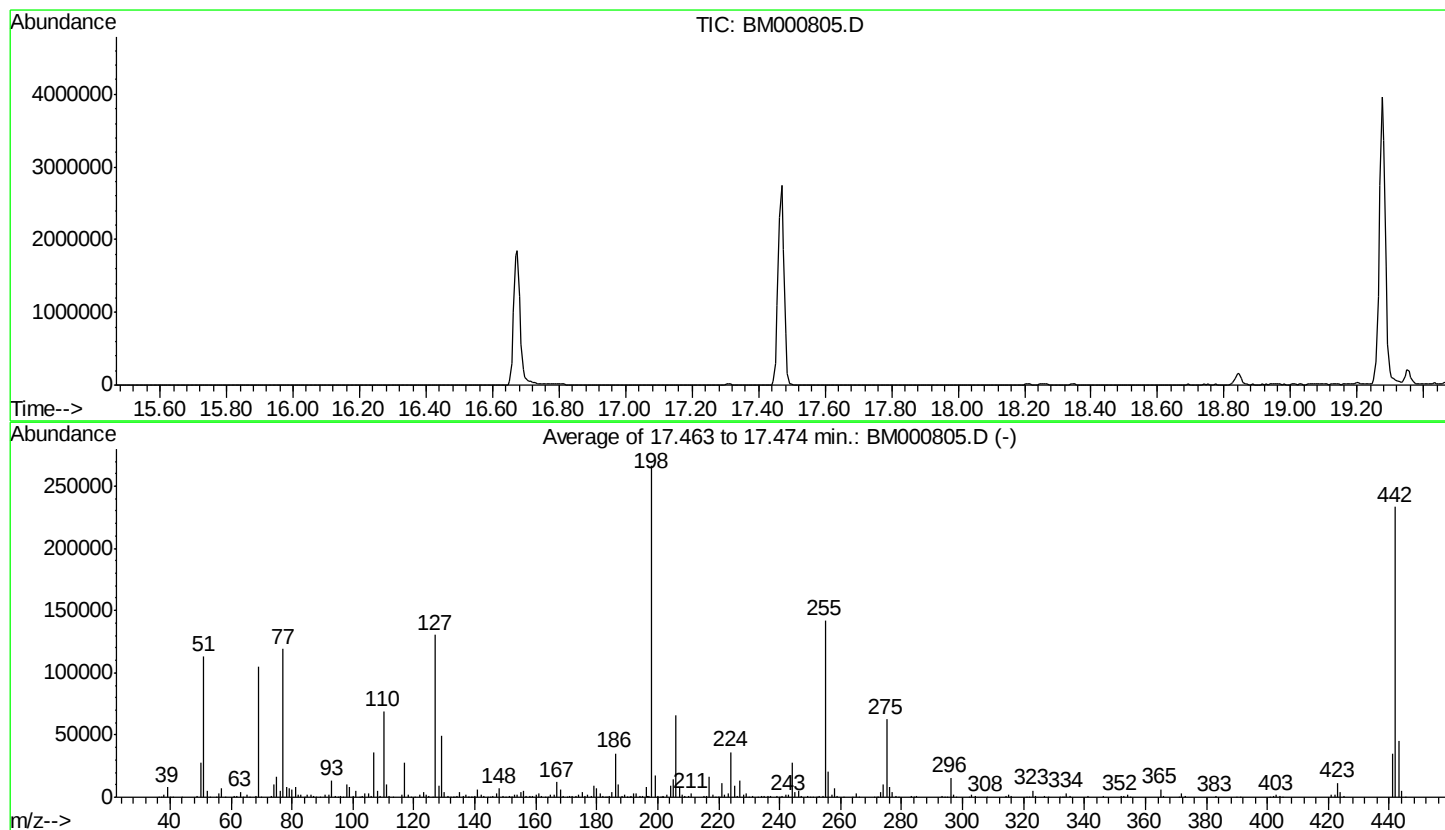

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	113074	PASS
68	69	0.00	2	1.4	1493	PASS
69	198	0.00	100	39.5	105218	PASS
70	69	0.00	2	0.5	494	PASS
127	198	10	80	48.9	130405	PASS
197	198	0.00	2	0.3	840	PASS
198	198	100	100	100.0	266496	PASS
199	198	5	9	6.5	17400	PASS
275	198	10	60	23.4	62488	PASS
365	198	1	100	2.5	6598	PASS
441	442	0.01	24	15.2	35480	PASS
442	198	50	100	87.5	233237	PASS
443	442	15	24	19.3	44933	PASS