
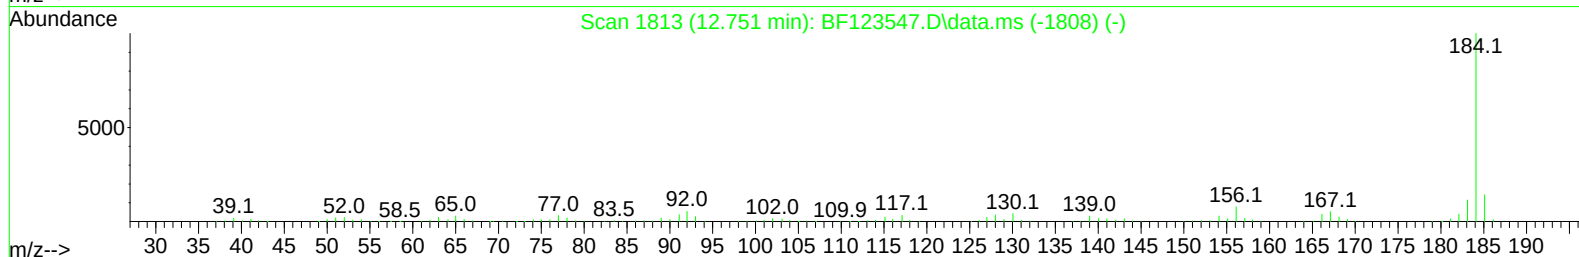
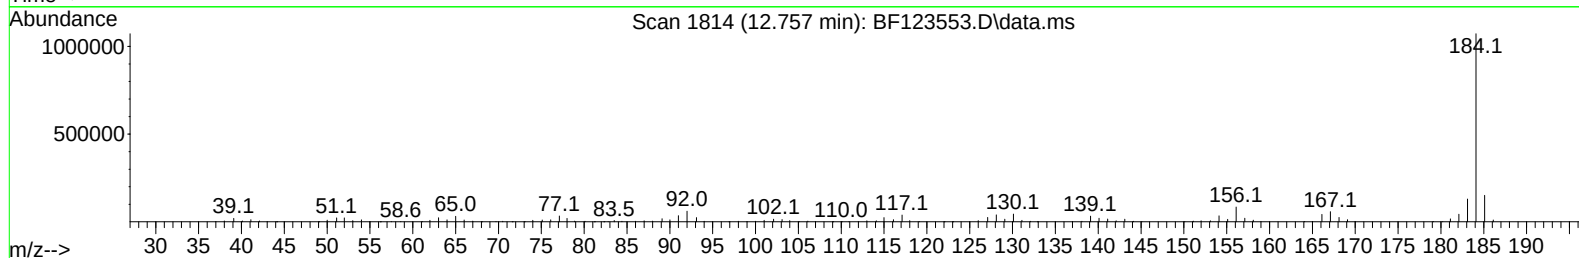


Quant Time: Apr 02 12:22:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 12:11:51 2021
Response via : Initial Calibration

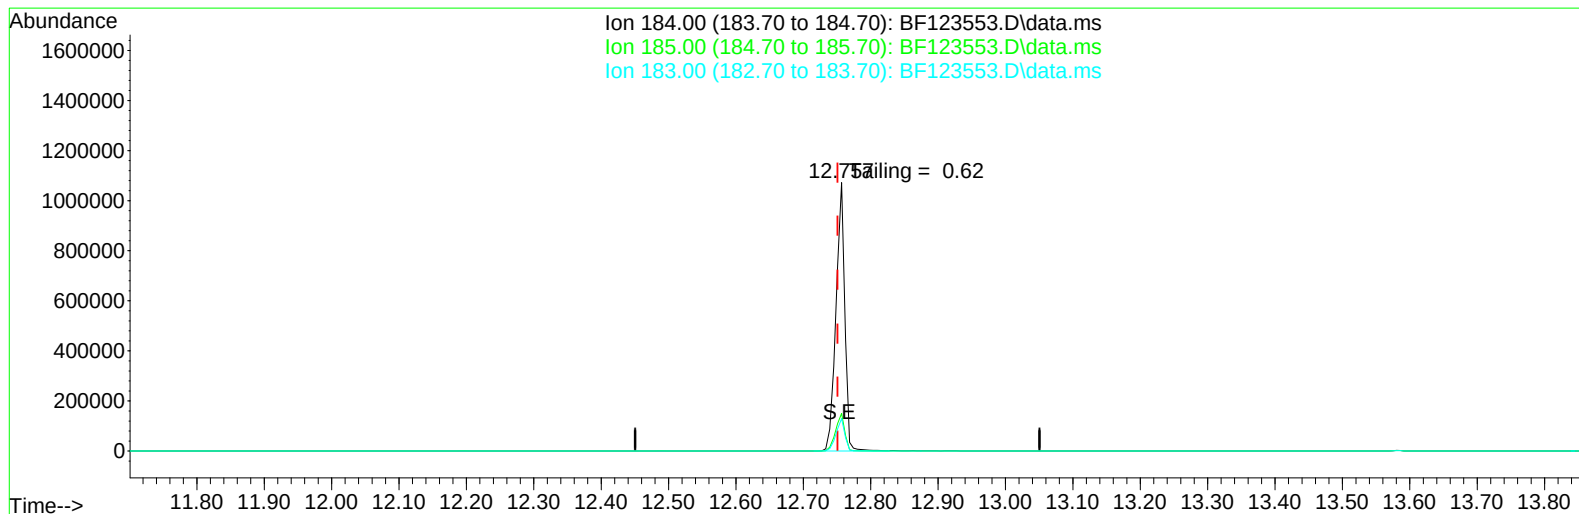

TIC: BF123553.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response **978214**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.03
183.00	12.10	12.11
0.00	0.00	0.00