
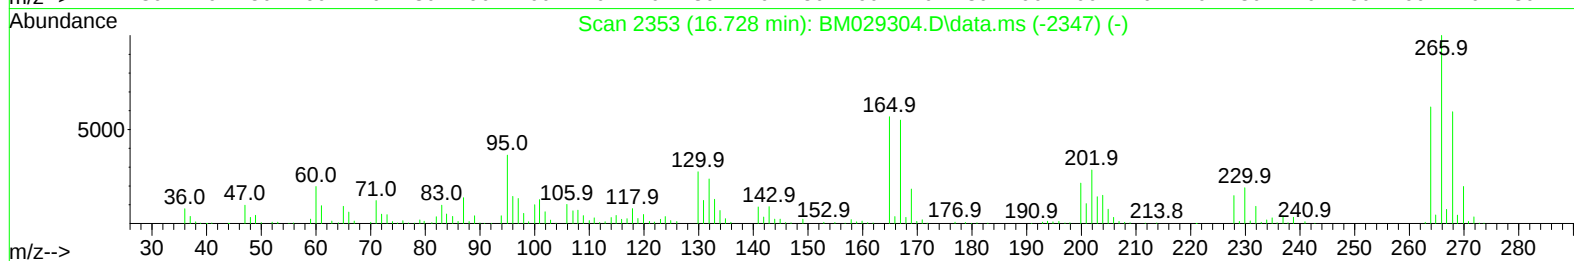
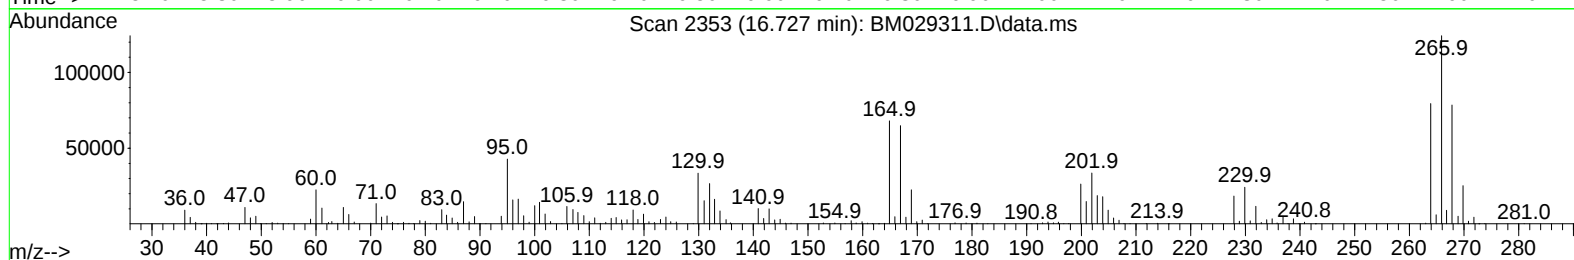


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040221\
Data File : BM029311.D
Acq On : 02 Apr 2021 08:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 11:22:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 16:52:48 2021
Response via : Initial Calibration

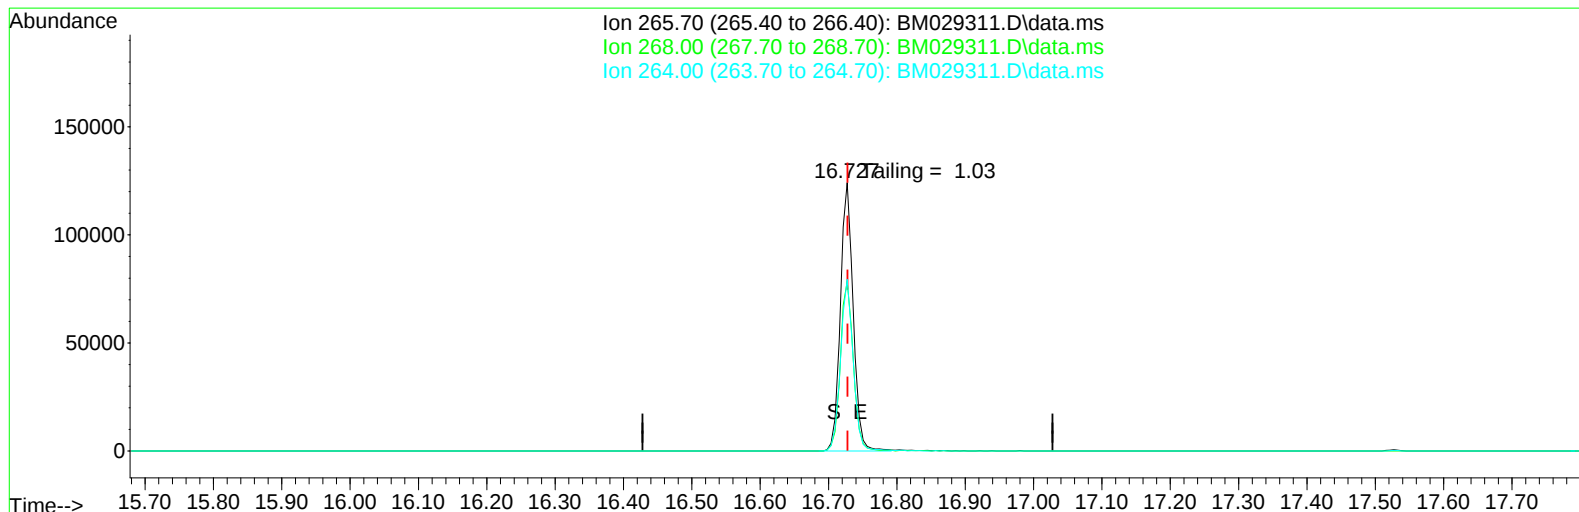

TIC: BM029311.D\data.ms

(70) Pentachlorophenol (C)




16.727min (-0.001) 446629.35 ng

response 161839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	63.22
264.00	63.60	63.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040221\
 Data File : BM029311.D
 Acq On : 02 Apr 2021 08:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 11:22:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 16:52:48 2021
 Response via : Initial Calibration

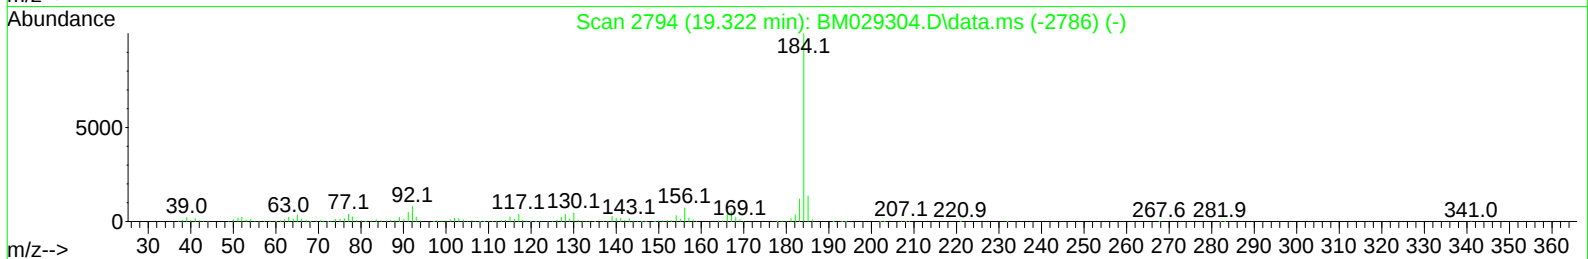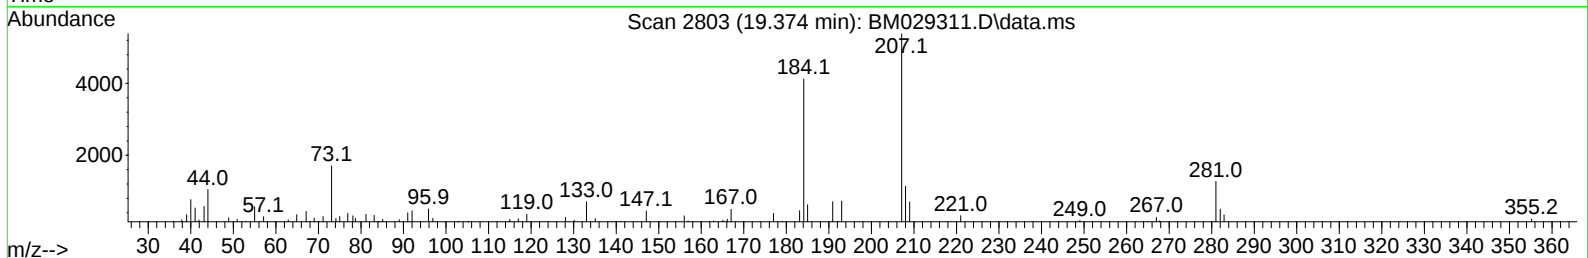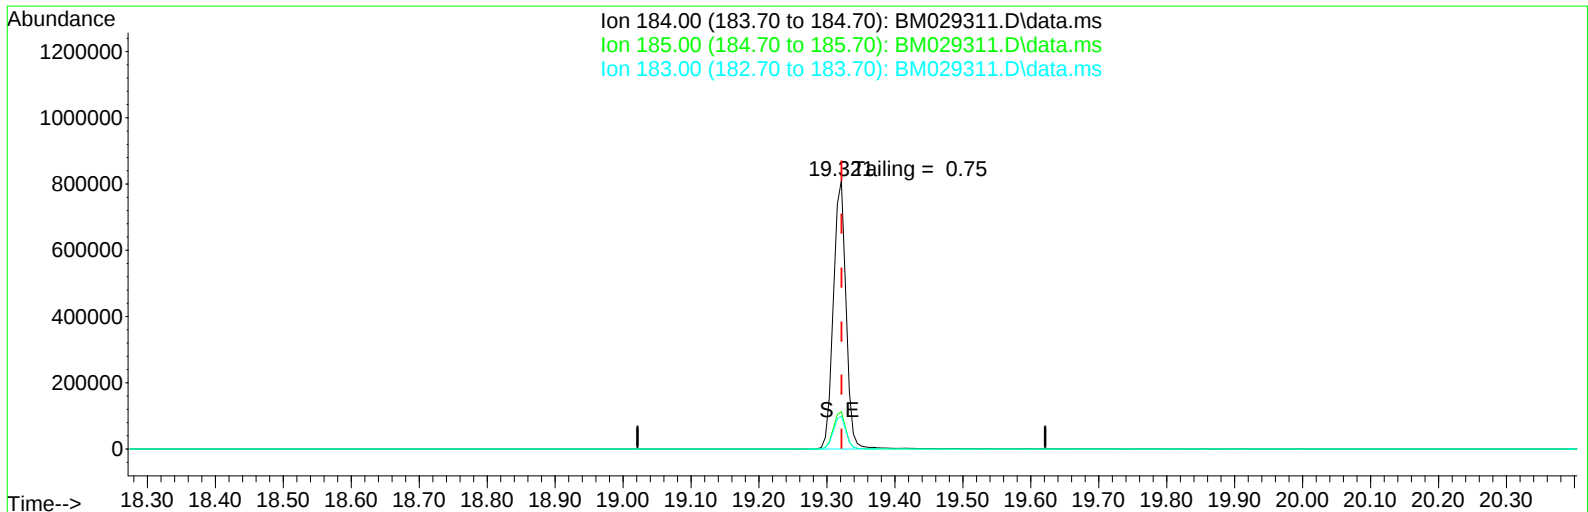

TIC: BM029311.D\data.ms

(77) Benzidine**19.321min (-0.000) 12237.65 ng****response 1049825**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.92
183.00	12.20	12.31
0.00	0.00	0.00