
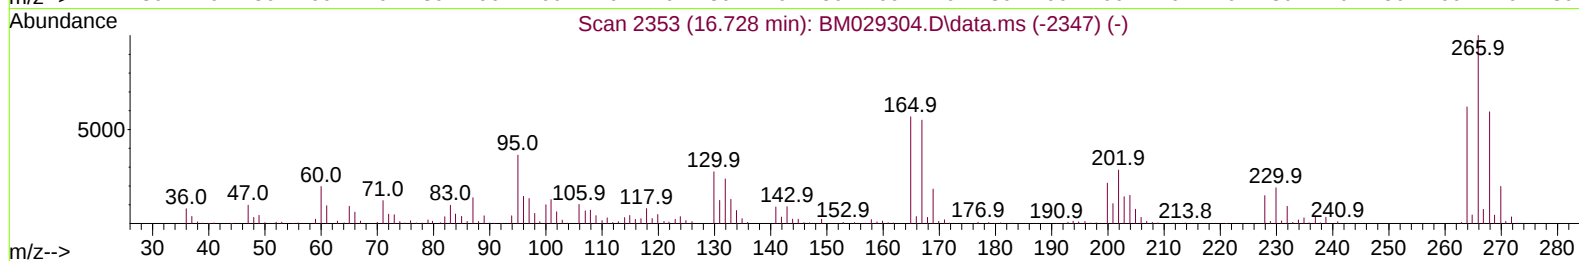
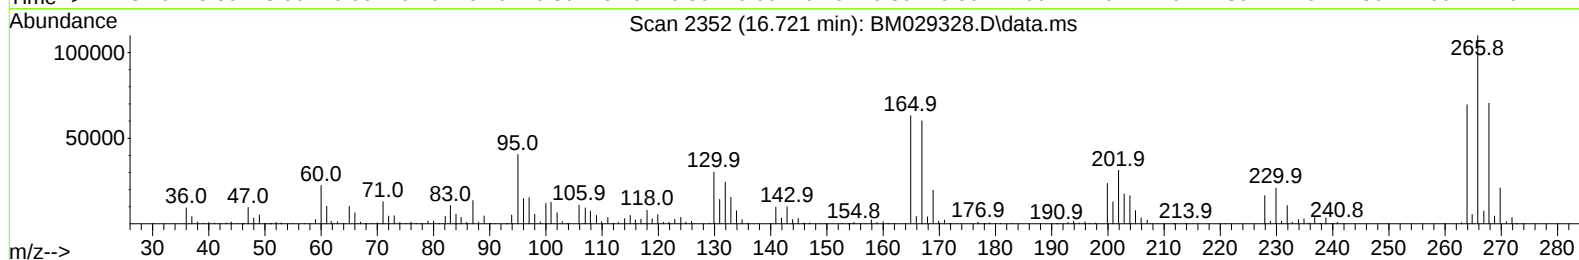


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040221\
Data File : BM029328.D
Acq On : 02 Apr 2021 20:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 01:22:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 16:52:48 2021
Response via : Initial Calibration

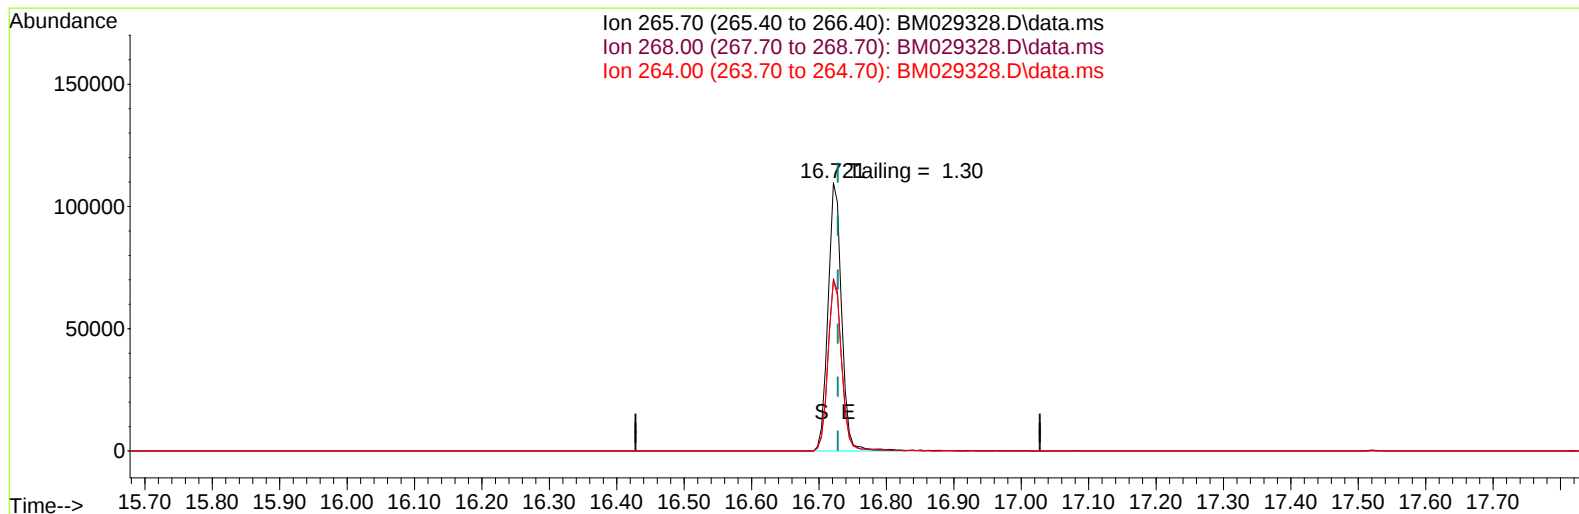

TIC: BM029328.D\data.ms

(70) Pentachlorophenol (C)




16.721min (-0.007) 91485.18 ng

response 153689

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	64.15
264.00	63.60	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040221\
 Data File : BM029328.D
 Acq On : 02 Apr 2021 20:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 01:22:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 16:52:48 2021
 Response via : Initial Calibration

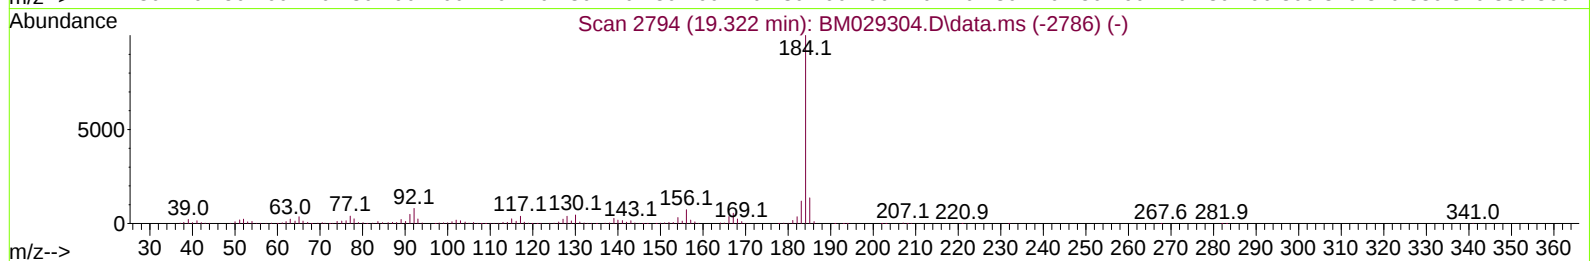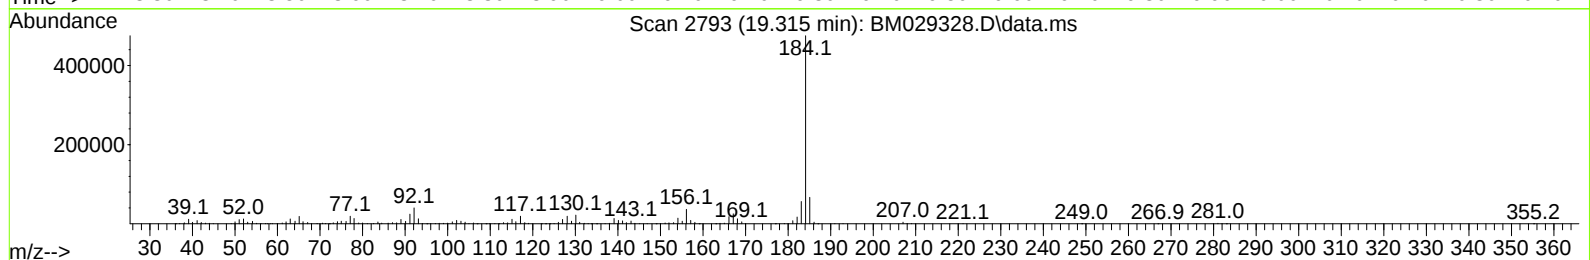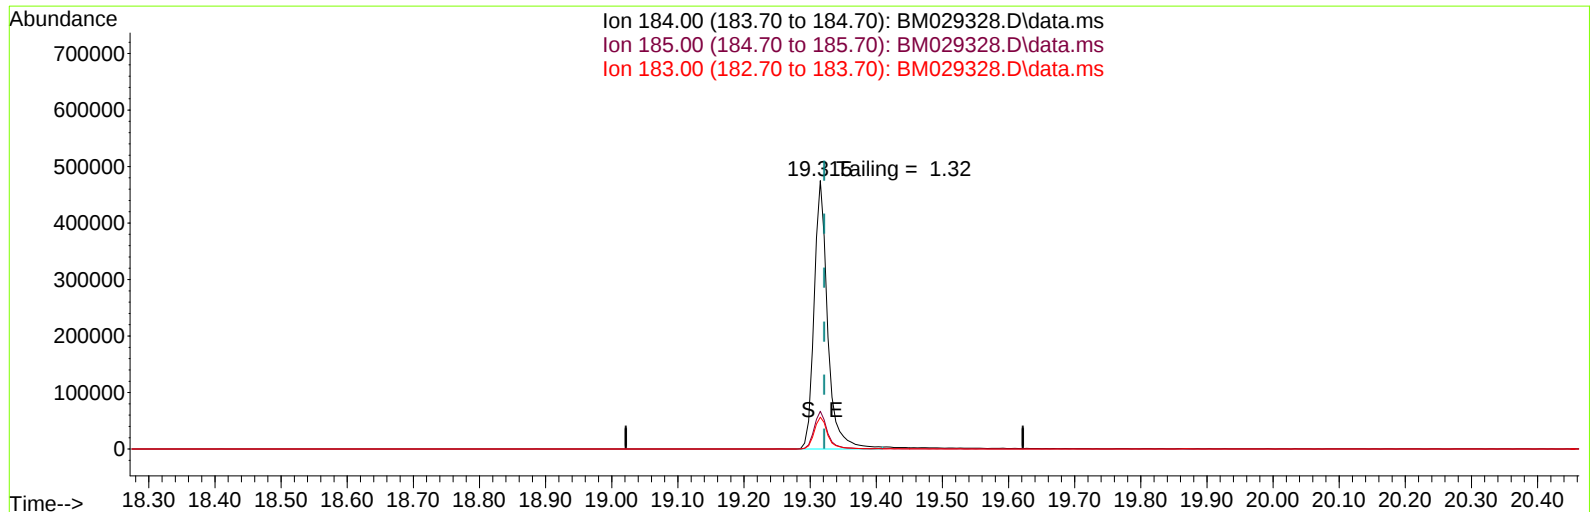

TIC: BM029328.D\data.ms

(77) Benzidine**19.315min (-0.006) 38144.40 ng****response 687858**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	12.20	11.88
0.00	0.00	0.00