
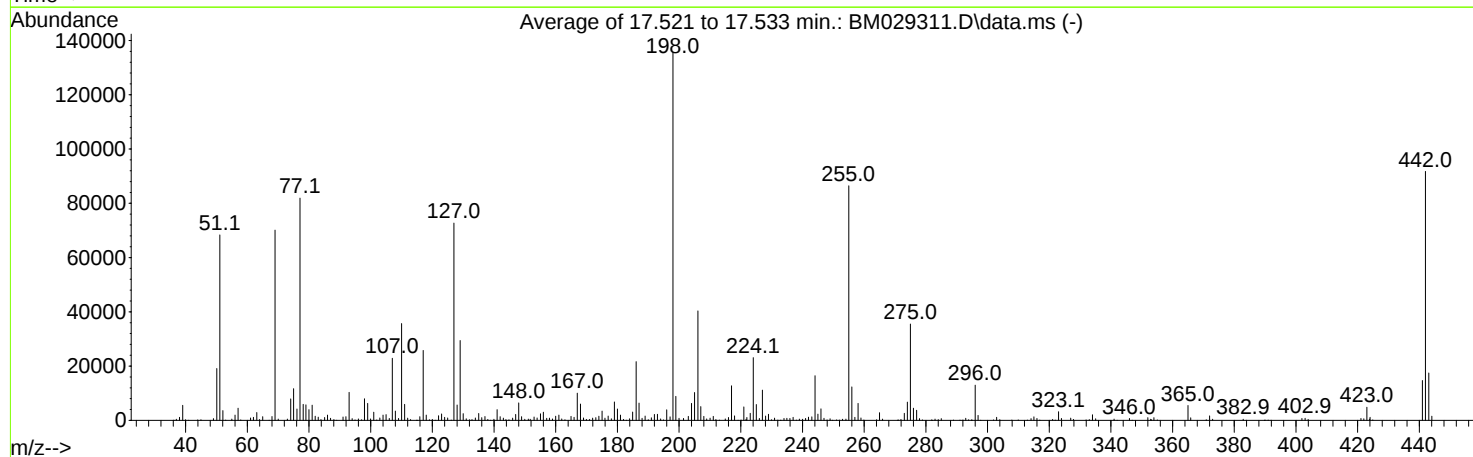


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040221\  
 Data File : BM029311.D  
 Acq On : 02 Apr 2021 08:17  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM040121.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Apr 01 16:52:48 2021

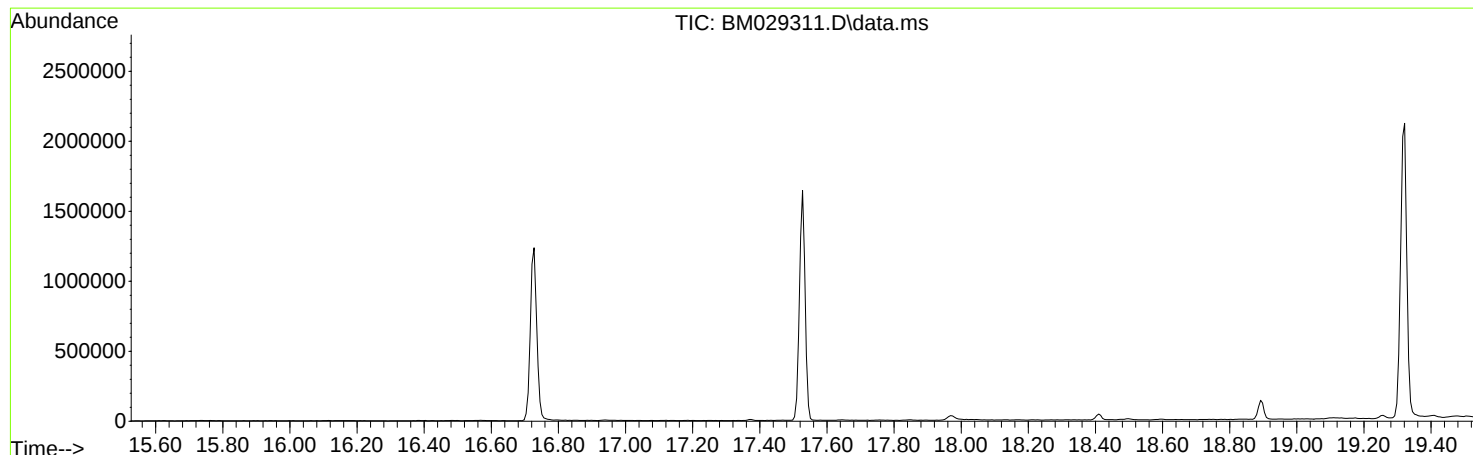

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 50.4         | 68371      | PASS                |
| 68             | 69              | 0.00            | 2               | 2.0          | 1399       | PASS                |
| 69             | 198             | 0.00            | 100             | 51.7         | 70104      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 492        | PASS                |
| 127            | 198             | 10              | 80              | 53.6         | 72701      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.9          | 1273       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 135576     | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 8870       | PASS                |
| 275            | 198             | 10              | 60              | 26.2         | 35533      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 5517       | PASS                |
| 441            | 198             | 0.01            | 100             | 10.8         | 14683      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 91744      | PASS                |
| 443            | 442             | 15              | 24              | 19.0         | 17451      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/2/2021      | BNA_M            | <u>BM029311.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 528783           | 20.55              |
| DDD           | 2491             | 20.11              |
| DDE           | 579              | 19.6               |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3070          | 531853           | 0.58               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040221\  
Data File : BM029311.D  
Acq On : 02 Apr 2021 08:17  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Apr 02 11:22:13 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM040121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 01 16:52:48 2021  
Response via : Initial Calibration

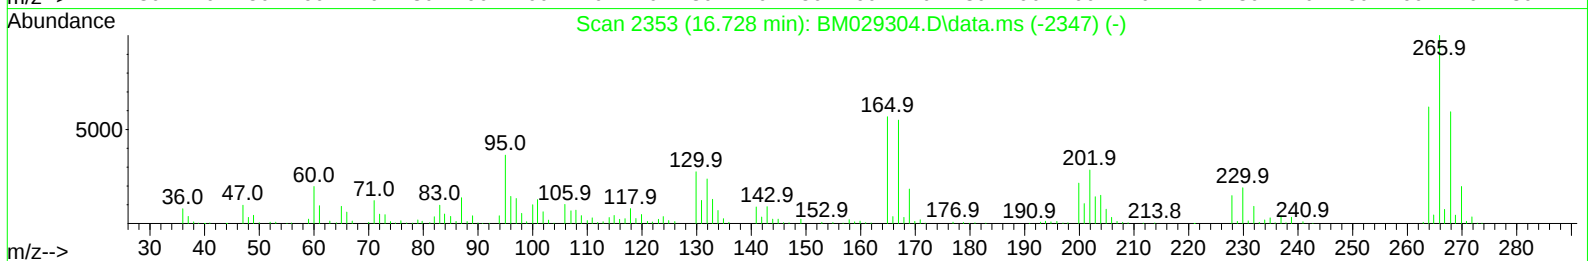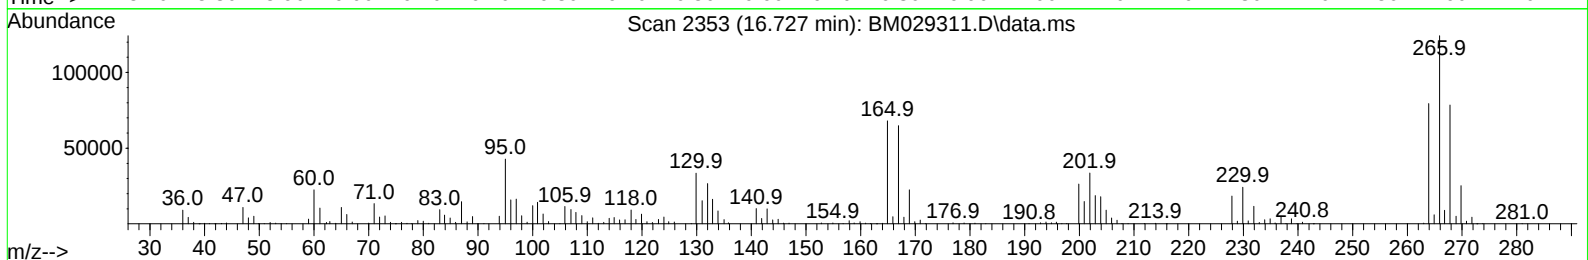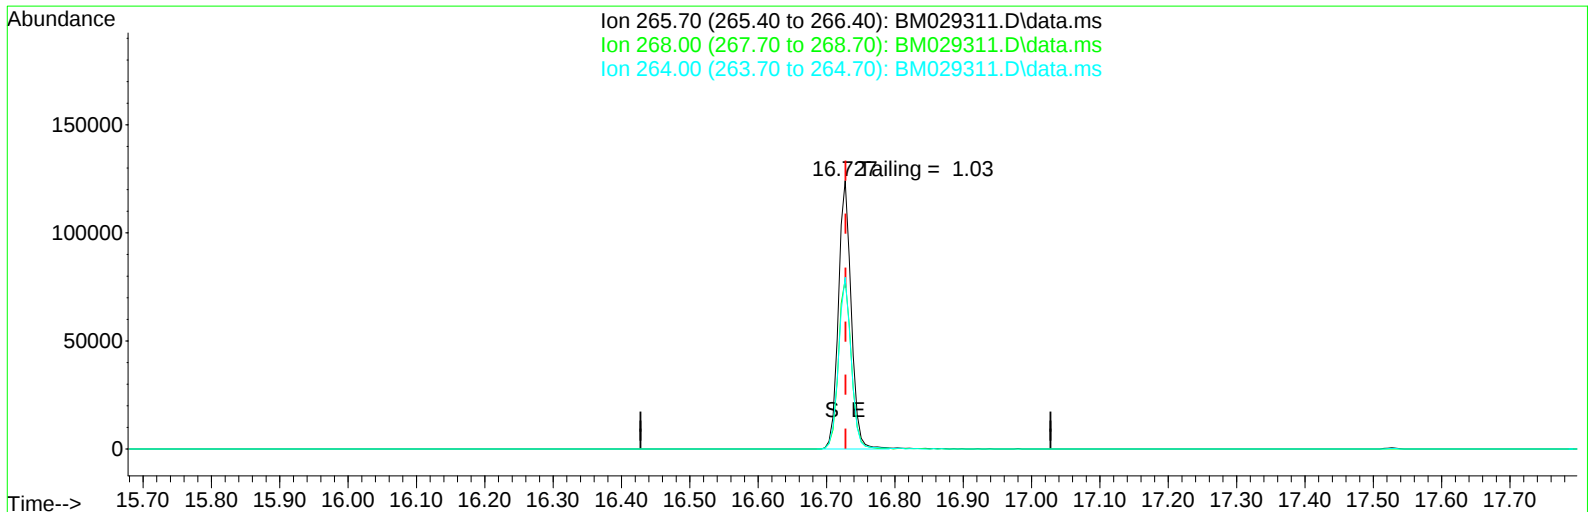

TIC: BM029311.D\data.ms

**(70) Pentachlorophenol (C)**

16.727min (-0.001) 446629.35 ng




response 161839

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.20  | 63.22  |
| 264.00 | 63.60  | 63.95  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040221\  
 Data File : BM029311.D  
 Acq On : 02 Apr 2021 08:17  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Apr 02 11:22:13 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM040121.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Apr 01 16:52:48 2021  
 Response via : Initial Calibration

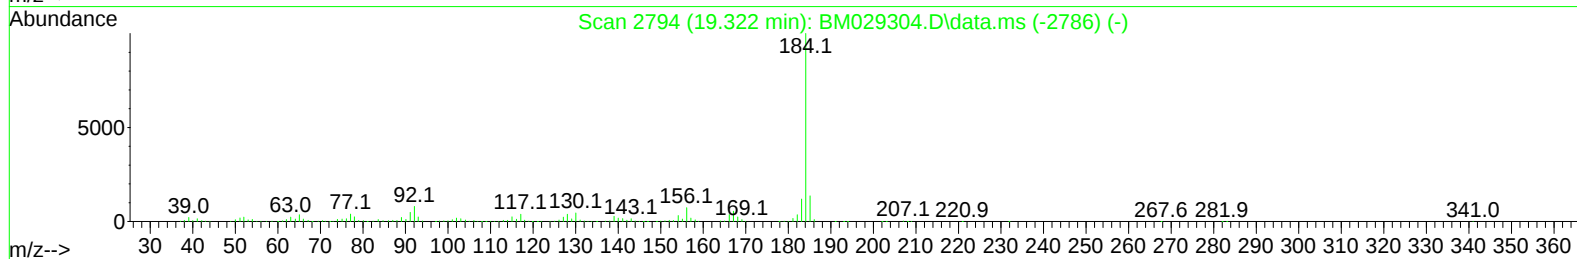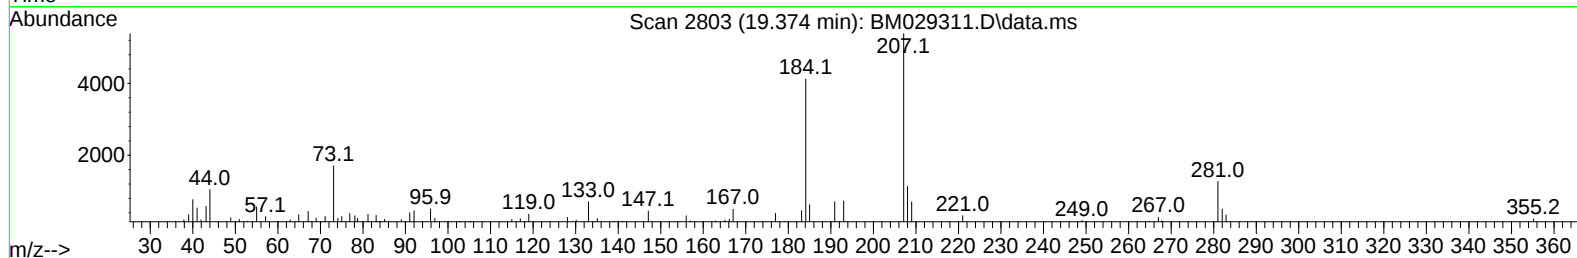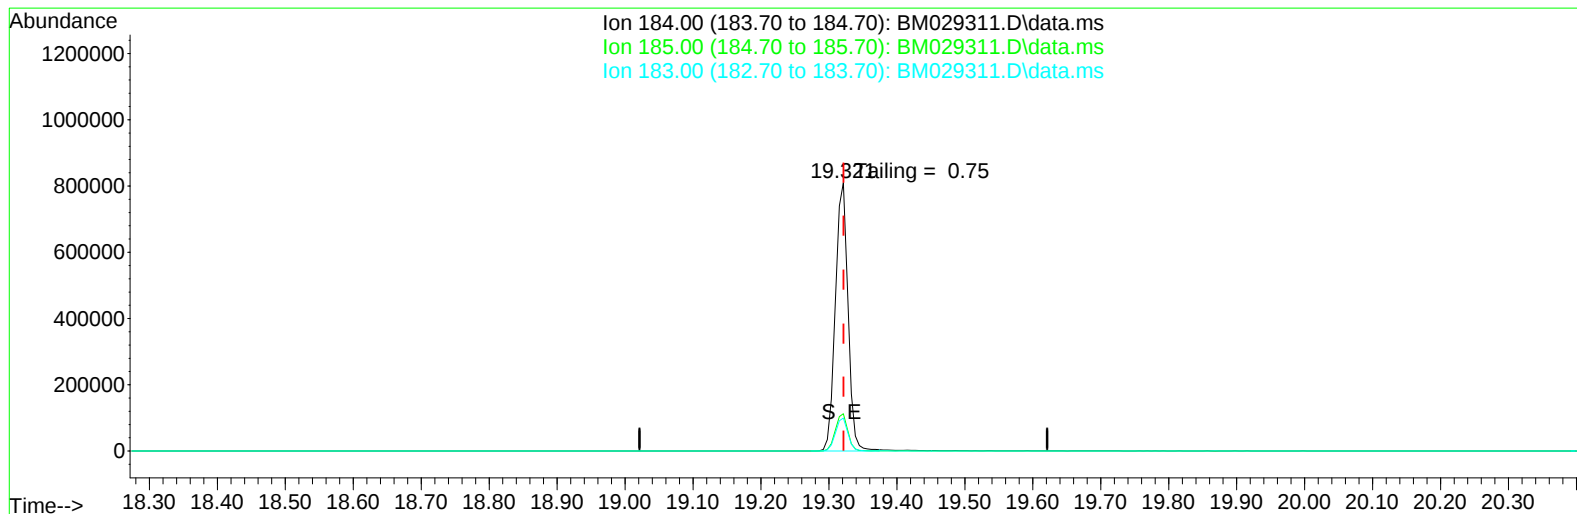

TIC: BM029311.D\data.ms

**(77) Benzidine**

19.321min (-0.000) 12237.65 ng

response 1049825

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 13.92  |
| 183.00 | 12.20  | 12.31  |
| 0.00   | 0.00   | 0.00   |