
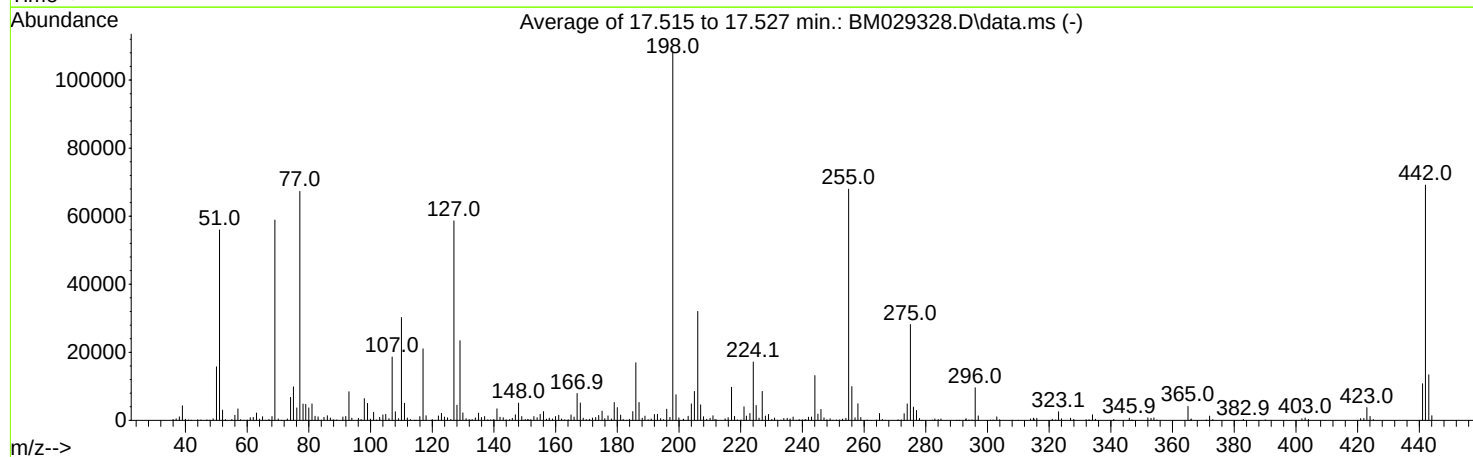


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040221\
 Data File : BM029328.D
 Acq On : 02 Apr 2021 20:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 01 16:52:48 2021

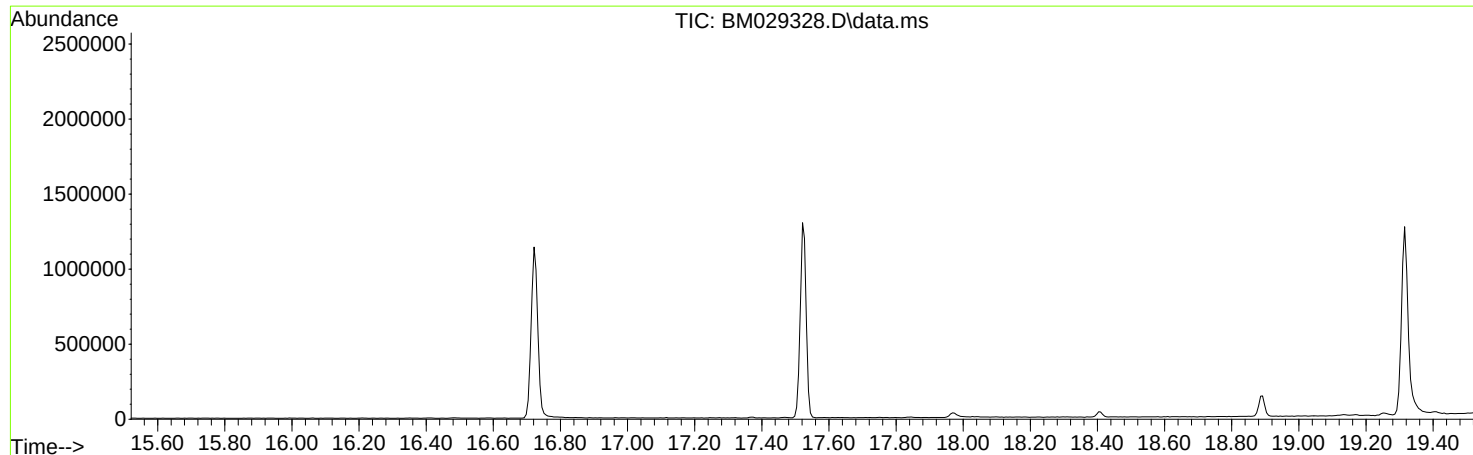

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.8	55977	PASS
68	69	0.00	2	1.9	1120	PASS
69	198	0.00	100	54.5	58890	PASS
70	69	0.00	2	0.8	451	PASS
127	198	10	80	54.3	58651	PASS
197	198	0.00	2	0.8	876	PASS
198	198	100	100	100.0	108112	PASS
199	198	5	9	7.0	7530	PASS
275	198	10	60	26.1	28181	PASS
365	198	1	100	3.8	4106	PASS
441	198	0.01	100	10.0	10791	PASS
442	442	50	100	100.0	69152	PASS
443	442	15	24	19.4	13403	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/2/2021	BNA_M	<u>BM029328.D</u>
Compound Name	Response	Retention Time
DDT	460853	20.55
DDD	12041	20.115
DDE	1102	19.615
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13143	473996	2.77

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040221\
Data File : BM029328.D
Acq On : 02 Apr 2021 20:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 03 01:22:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 16:52:48 2021
Response via : Initial Calibration

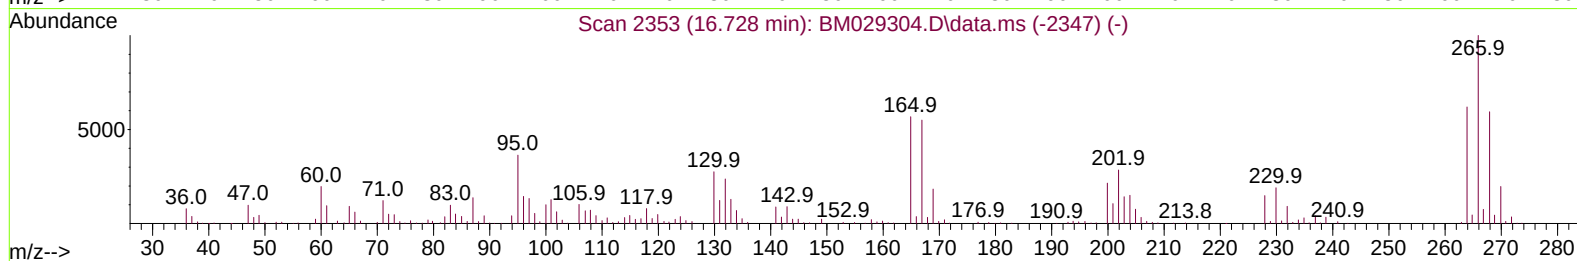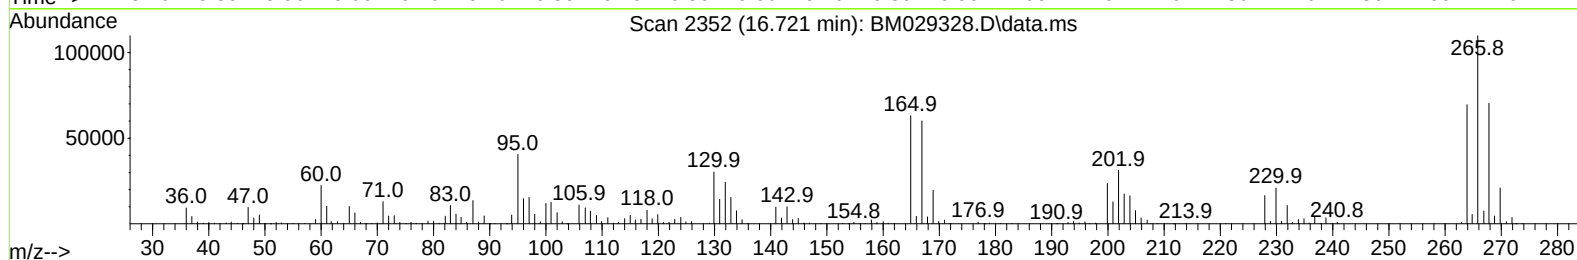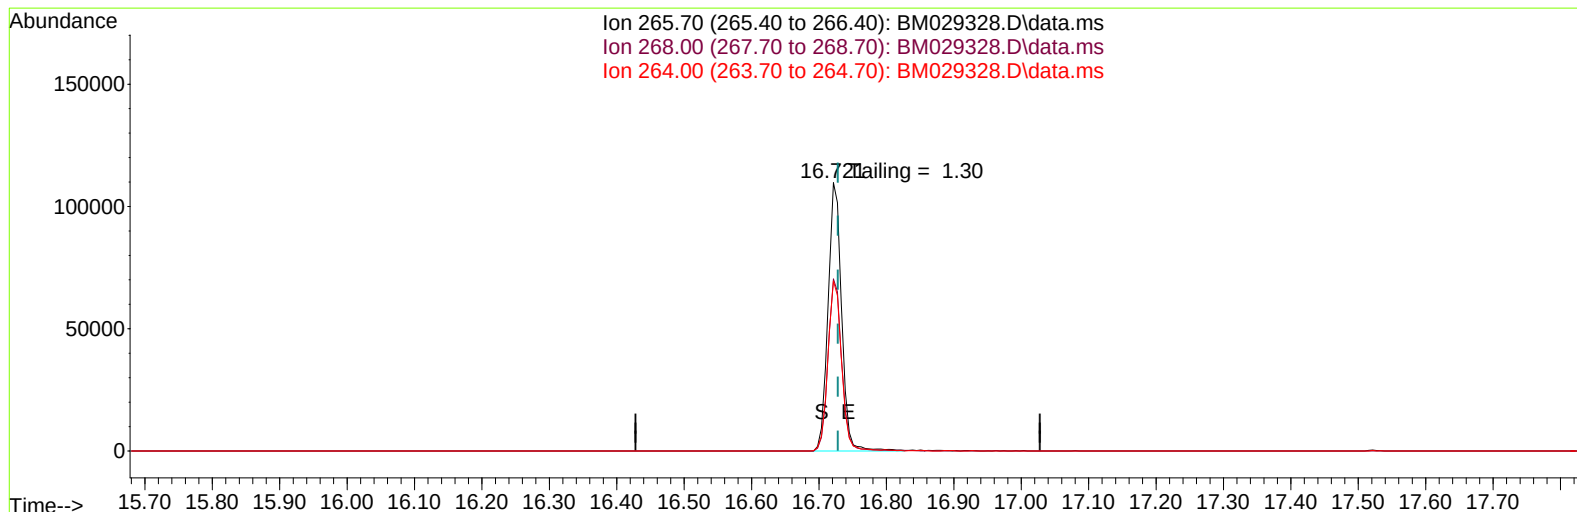

TIC: BM029328.D\data.ms

(70) Pentachlorophenol (C)

16.721min (-0.007) 91485.18 ng




response 153689

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	64.15
264.00	63.60	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040221\
 Data File : BM029328.D
 Acq On : 02 Apr 2021 20:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 03 01:22:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 16:52:48 2021
 Response via : Initial Calibration

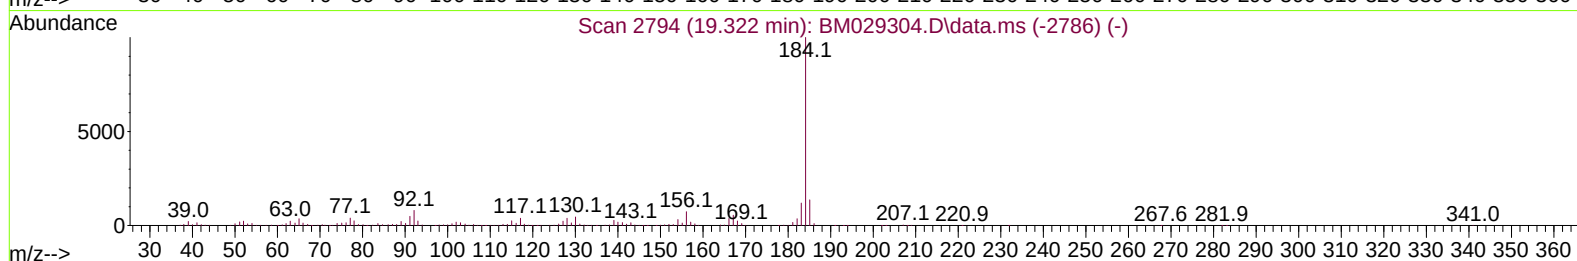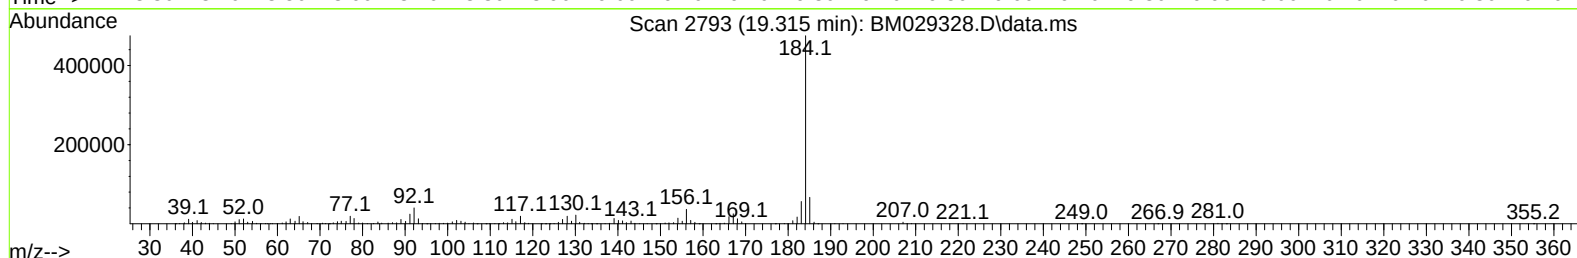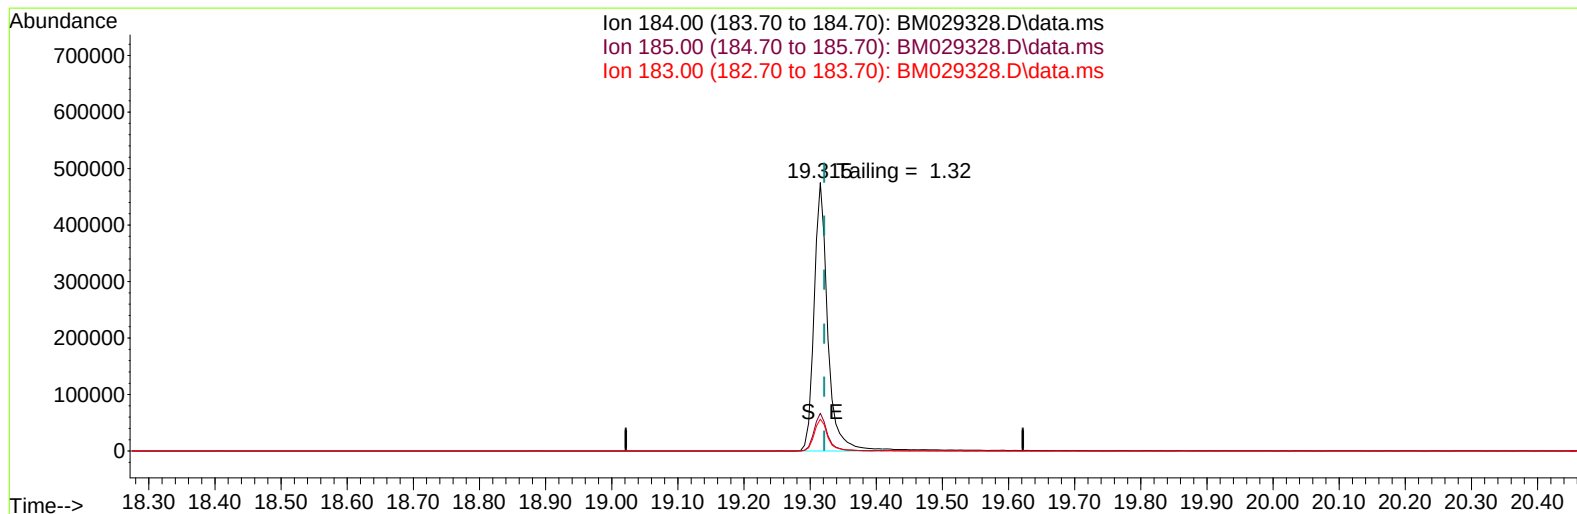

TIC: BM029328.D\data.ms

(77) Benzidine**19.315min (-0.006) 38144.40 ng****response 687858**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	12.20	11.88
0.00	0.00	0.00