
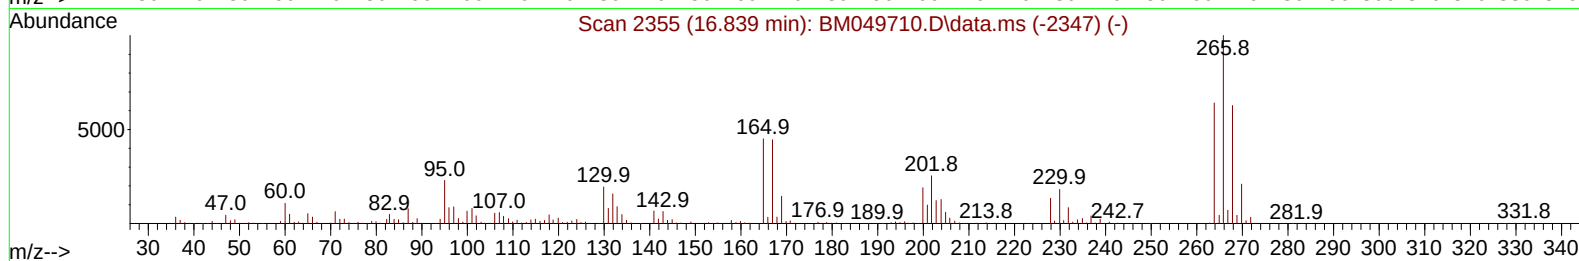
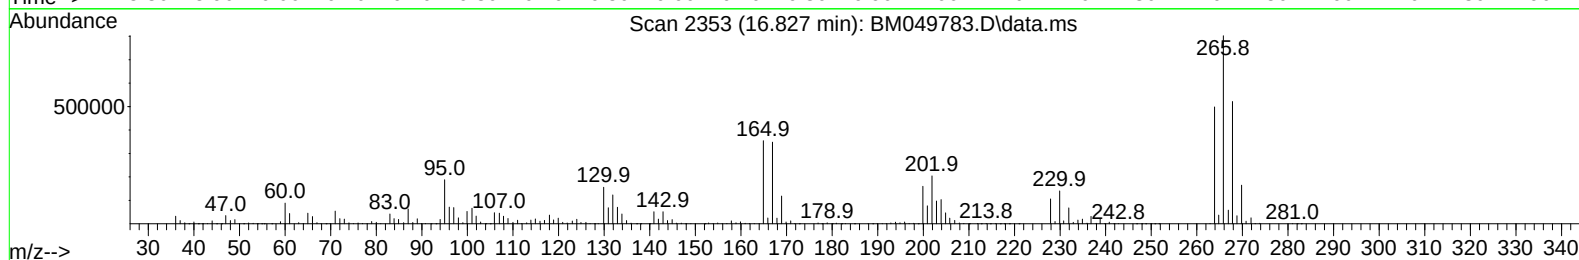


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040225\
Data File : BM049783.D
Acq On : 02 Apr 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 11:48:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

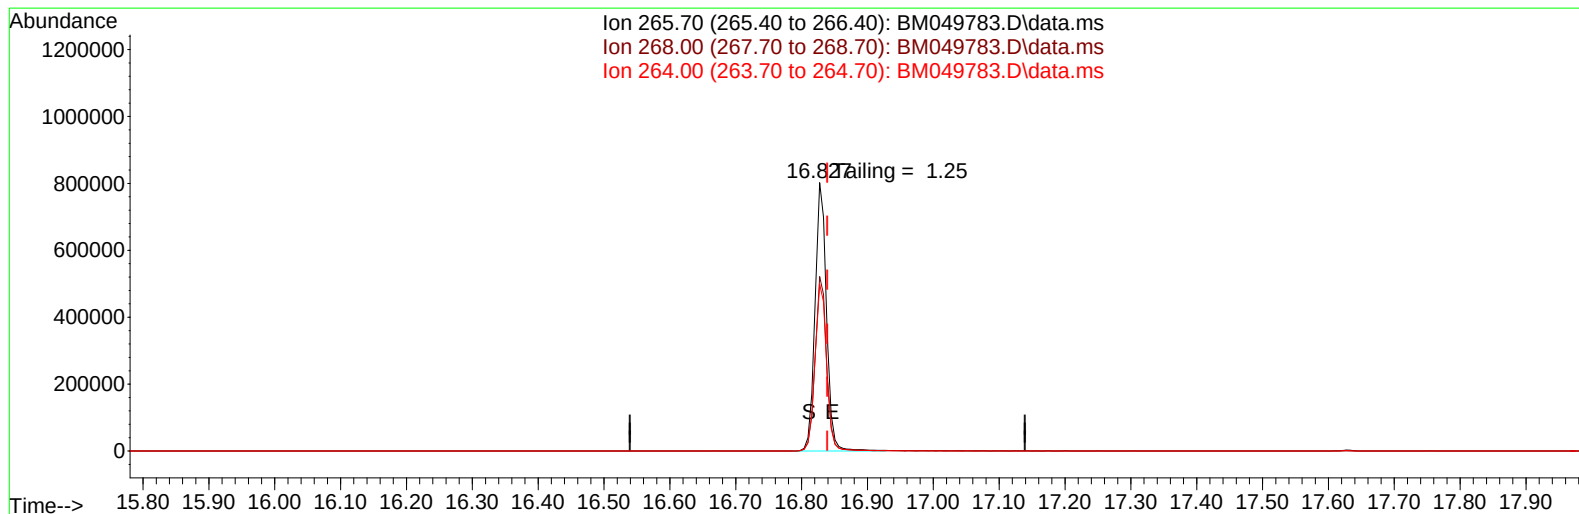

TIC: BM049783.D\data.ms

(70) Pentachlorophenol (C)




16.827min (-0.012) 68544.51 ng

response 974790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	65.02
264.00	64.10	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040225\
Data File : BM049783.D
Acq On : 02 Apr 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 11:48:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

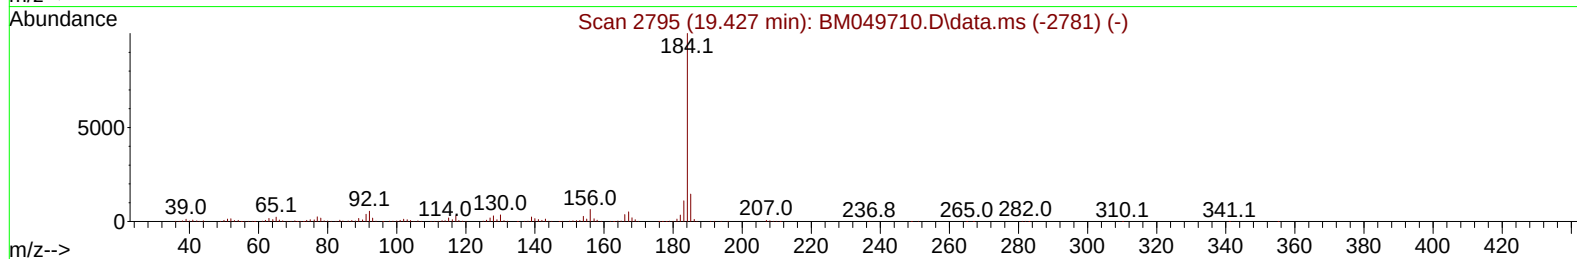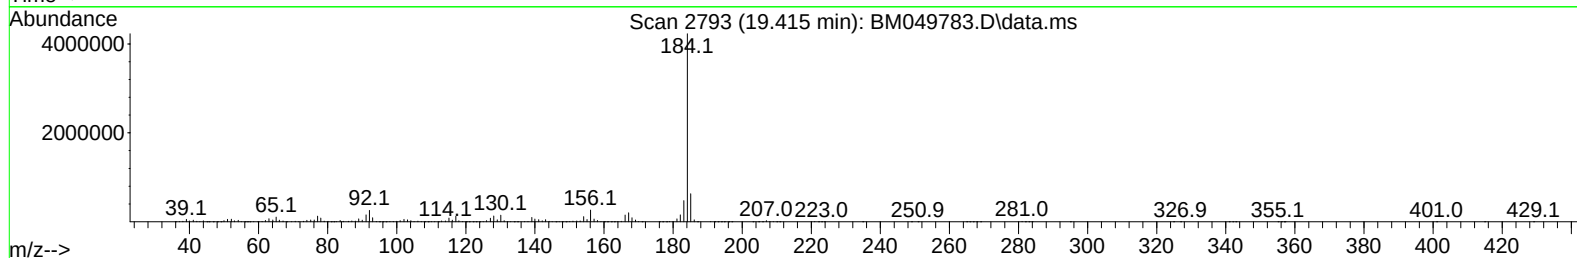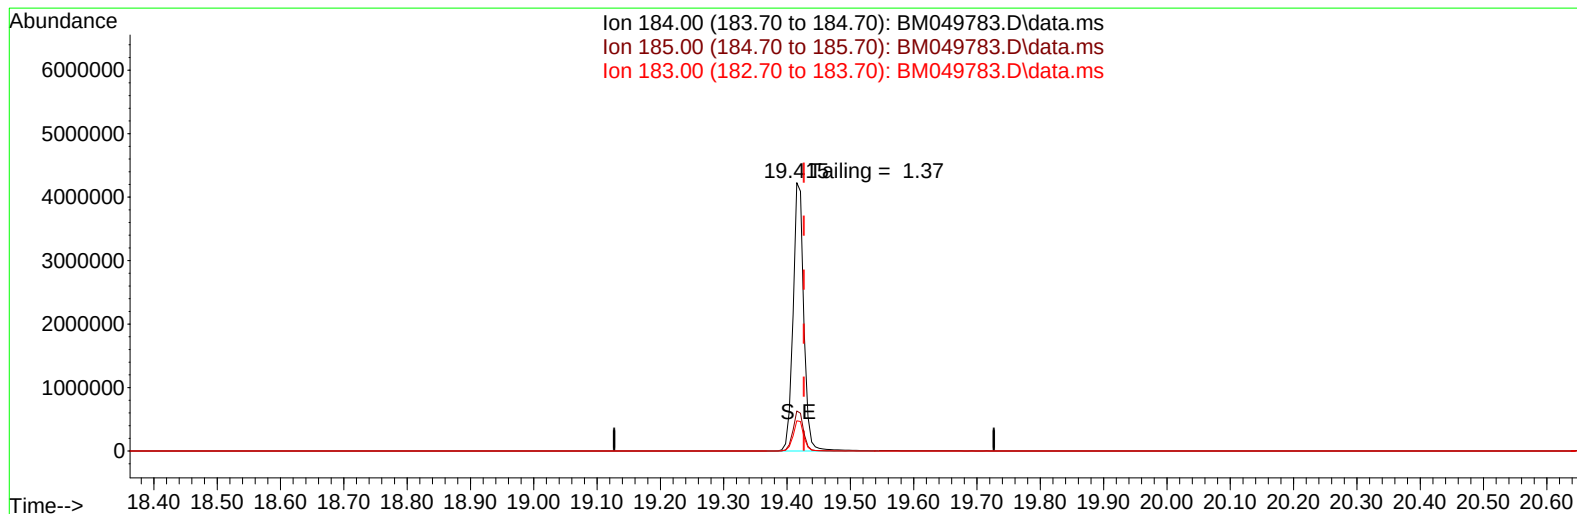

TIC: BM049783.D\data.ms

(77) Benzidine**19.415min (-0.012) 27579.90 ng****response 5011923**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.90
183.00	11.00	11.28
0.00	0.00	0.00