

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040225\
 Data File : BM049793.D
 Acq On : 02 Apr 2025 16:43
 Operator : RC/JU
 Sample : Q1664-09RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P001-BBDGA-002-01RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM049793.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.904	320	326	333	rBV	357073	486200	3.54%	0.815%
2	5.369	397	405	415	rBV	4022384	5456881	39.74%	9.152%
3	6.957	665	675	691	rBV	3873340	5768318	42.01%	9.674%
4	7.787	809	816	825	rVB	973015	1474003	10.73%	2.472%
5	8.939	1005	1012	1029	rBV	2180564	3437131	25.03%	5.764%
6	10.581	1282	1291	1302	rBV	1128011	1853546	13.50%	3.109%
7	13.051	1703	1711	1725	rBV	6186297	8352389	60.82%	14.008%
8	14.427	1933	1945	1956	rBV	1770501	2435535	17.74%	4.085%
9	15.786	2168	2176	2183	rBV	334741	444404	3.24%	0.745%
10	15.915	2190	2198	2219	rBV	4484459	6096626	44.40%	10.225%
11	17.168	2404	2411	2417	rBV	2143000	2773237	20.19%	4.651%
12	18.068	2559	2564	2573	rBV2	177992	272071	1.98%	0.456%
13	19.792	2852	2857	2865	rBV	12252295	13732344	100.00%	23.030%
14	21.092	3074	3078	3088	rBV2	182409	316547	2.31%	0.531%
15	21.403	3125	3131	3136	rBV	2388837	3374427	24.57%	5.659%
16	24.397	3632	3640	3655	rVB	1346929	3353155	24.42%	5.624%




Sum of corrected areas: 59626814

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040225\
Data File : BM049793.D
Acq On : 02 Apr 2025 16:43
Operator : RC/JU
Sample : Q1664-09RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P001-BBDGA-002-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

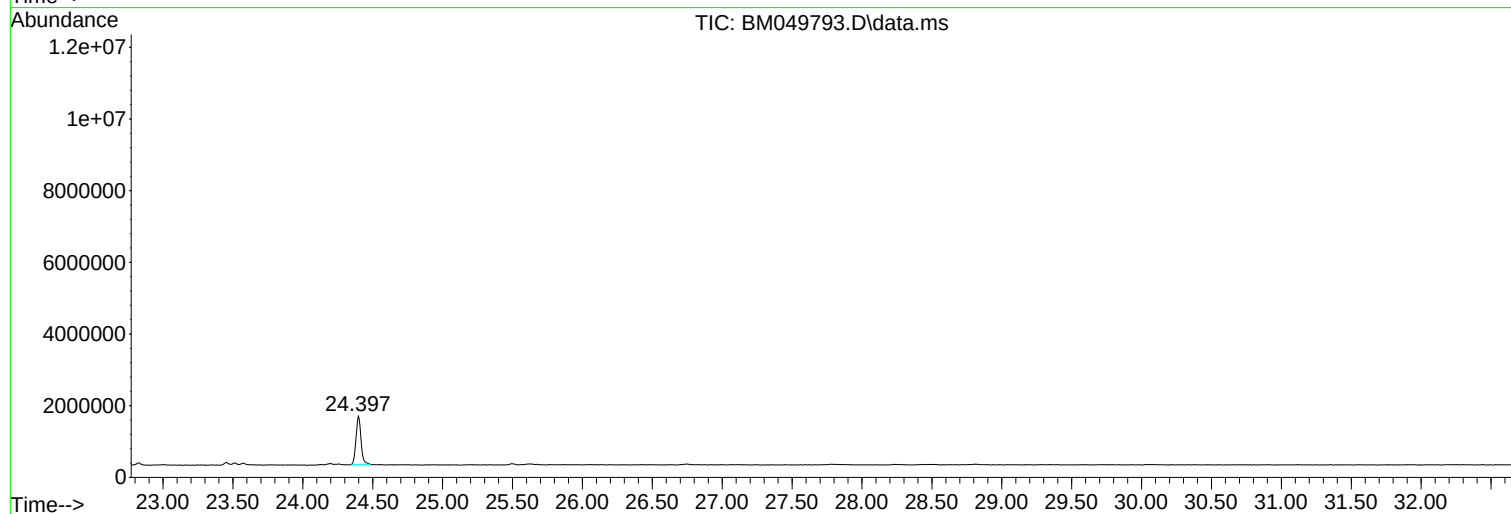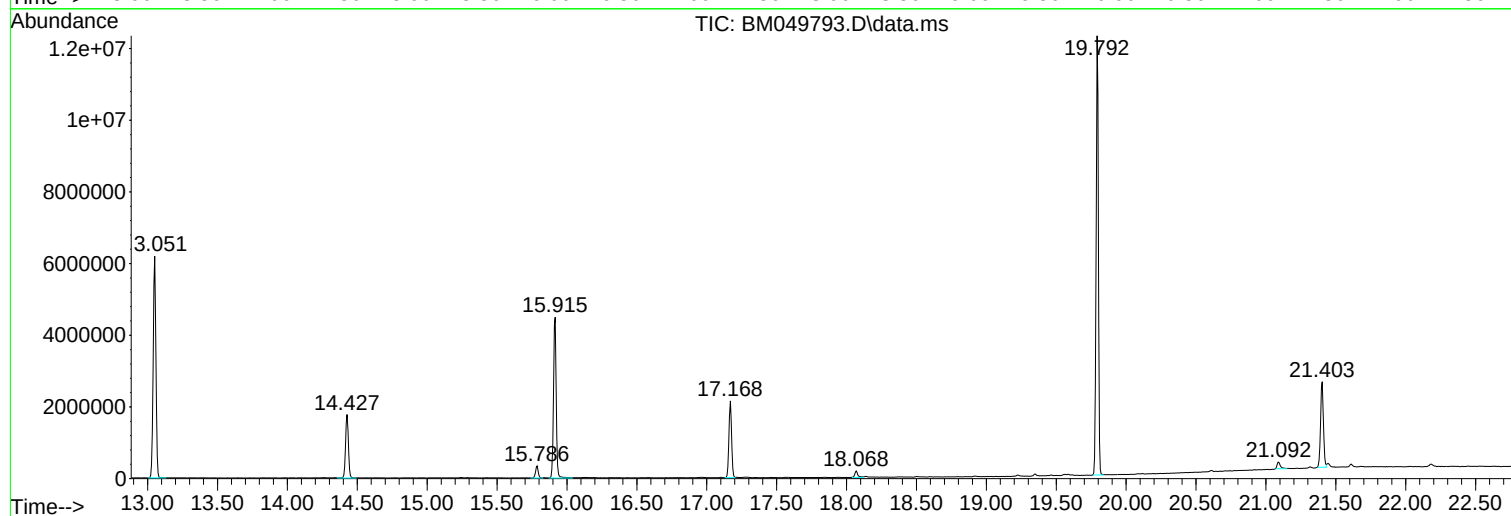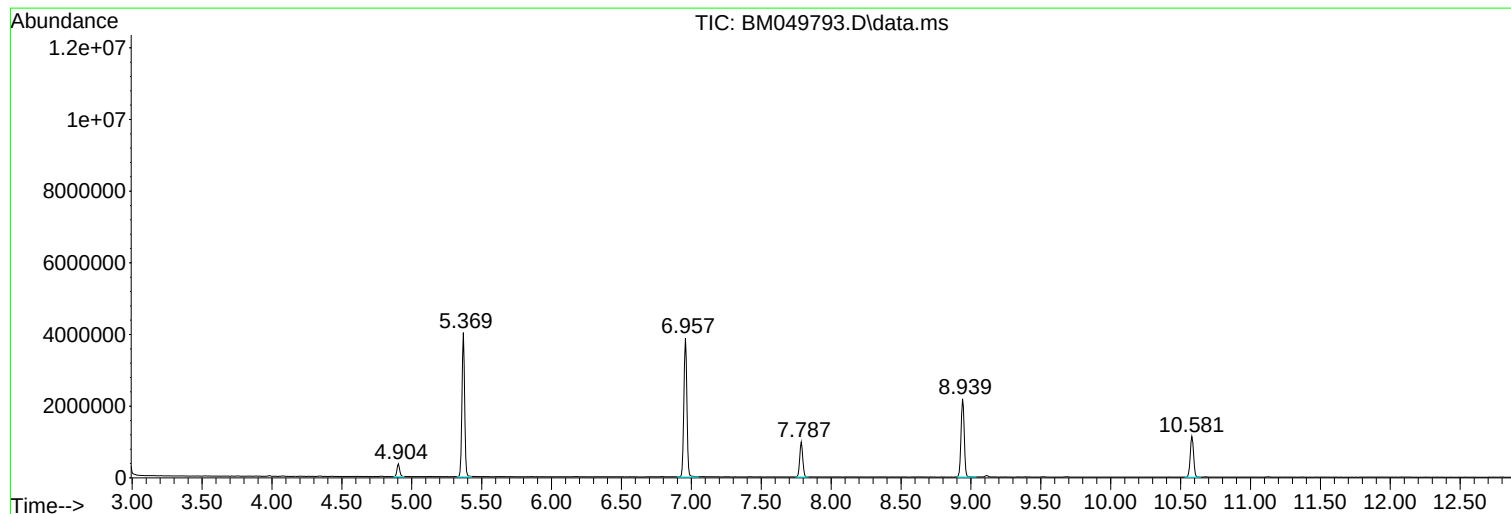

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040225\
Data File : BM049793.D
Acq On : 02 Apr 2025 16:43
Operator : RC/JU
Sample : Q1664-09RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P001-BBDGA-002-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040225\
Data File : BM049793.D
Acq On : 02 Apr 2025 16:43
Operator : RC/JU
Sample : Q1664-09RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P001-BBDGA-002-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------