

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040225\  
 Data File : BM049794.D  
 Acq On : 02 Apr 2025 17:22  
 Operator : RC/JU  
 Sample : Q1664-17RE  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 P001-BBDGA-006-01RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM049794.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.904       | 321           | 326         | 335          | rBV      | 417241         | 568759        | 3.60%           | 0.856%        |
| 2         | 5.369       | 398           | 405         | 416          | rBV      | 4802049        | 6447883       | 40.80%          | 9.701%        |
| 3         | 6.957       | 668           | 675         | 691          | rBV      | 4584654        | 6765779       | 42.82%          | 10.179%       |
| 4         | 7.787       | 809           | 816         | 825          | rBV      | 995167         | 1508035       | 9.54%           | 2.269%        |
| 5         | 8.939       | 1004          | 1012        | 1021         | rBV      | 2584820        | 4078187       | 25.81%          | 6.136%        |
| 6         | 10.580      | 1283          | 1291        | 1300         | rBV      | 1164214        | 1858186       | 11.76%          | 2.796%        |
| 7         | 13.051      | 1703          | 1711        | 1721         | rBV      | 6968745        | 9889233       | 62.58%          | 14.879%       |
| 8         | 14.427      | 1935          | 1945        | 1957         | rBV      | 1699689        | 2400040       | 15.19%          | 3.611%        |
| 9         | 15.786      | 2169          | 2176        | 2183         | rBV      | 310335         | 411046        | 2.60%           | 0.618%        |
| 10        | 15.915      | 2191          | 2198        | 2210         | rBV      | 5104144        | 6850582       | 43.35%          | 10.307%       |
| 11        | 17.168      | 2404          | 2411        | 2422         | rBV      | 1984550        | 2700651       | 17.09%          | 4.063%        |
| 12        | 18.068      | 2559          | 2564        | 2572         | rBV      | 229307         | 345574        | 2.19%           | 0.520%        |
| 13        | 19.792      | 2852          | 2857        | 2863         | rBV      | 14156724       | 15802329      | 100.00%         | 23.775%       |
| 14        | 21.092      | 3074          | 3078        | 3089         | rBV2     | 161740         | 291850        | 1.85%           | 0.439%        |
| 15        | 21.403      | 3125          | 3131        | 3136         | rBV      | 2343314        | 3262246       | 20.64%          | 4.908%        |
| 16        | 24.397      | 3632          | 3640        | 3656         | rVB      | 1323524        | 3286137       | 20.80%          | 4.944%        |




Sum of corrected areas: 66466517

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040225\  
Data File : BM049794.D  
Acq On : 02 Apr 2025 17:22  
Operator : RC/JU  
Sample : Q1664-17RE  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
P001-BBDGA-006-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

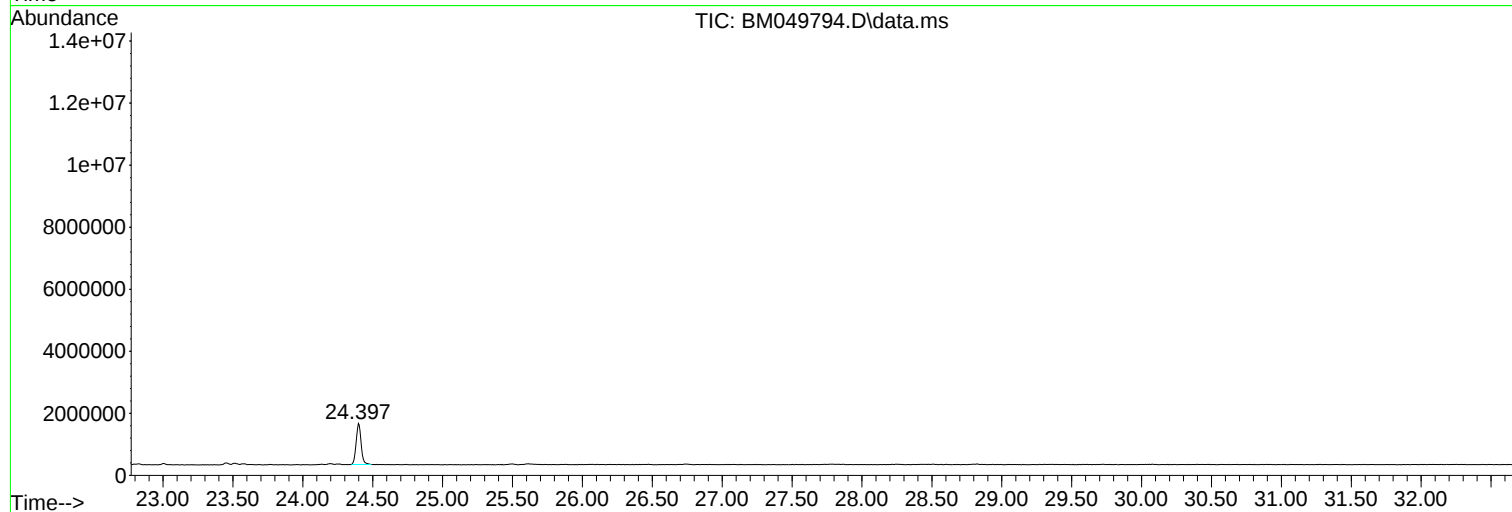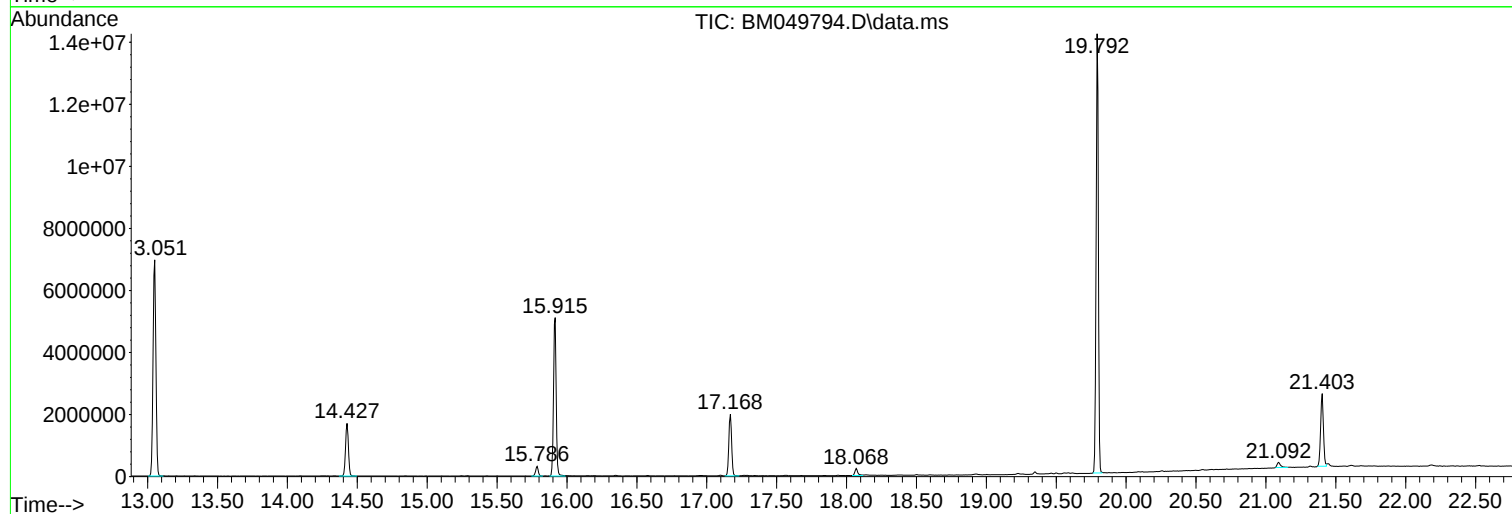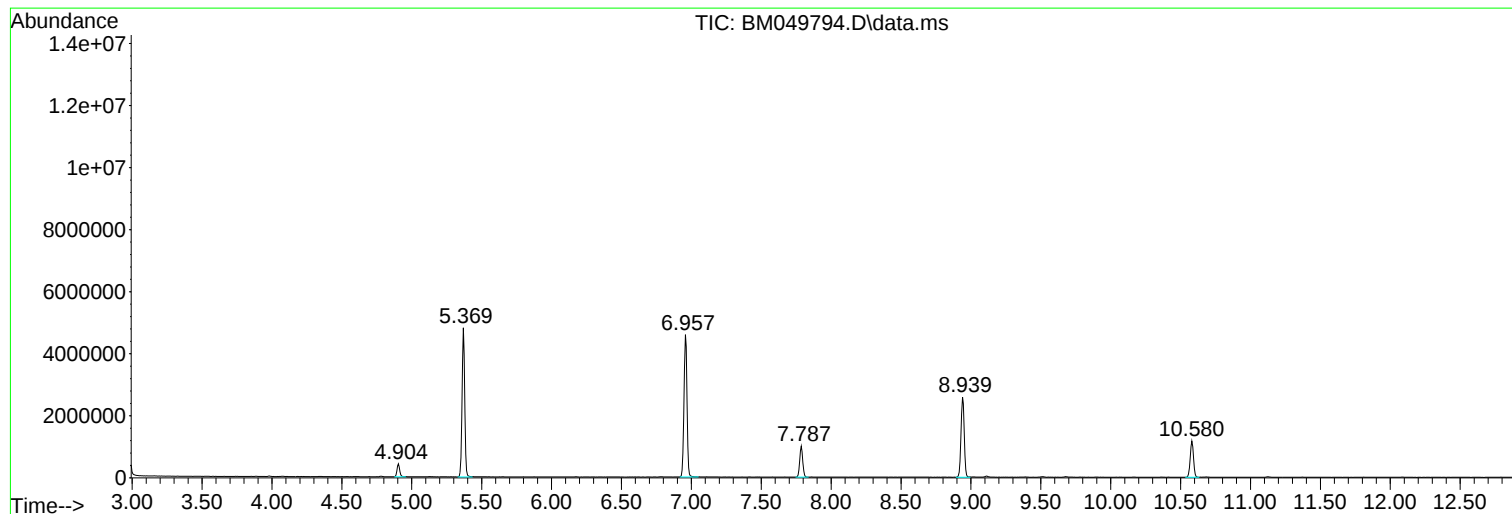

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040225\  
Data File : BM049794.D  
Acq On : 02 Apr 2025 17:22  
Operator : RC/JU  
Sample : Q1664-17RE  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
P001-BBDGA-006-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040225\  
Data File : BM049794.D  
Acq On : 02 Apr 2025 17:22  
Operator : RC/JU  
Sample : Q1664-17RE  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
P001-BBDGA-006-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|