
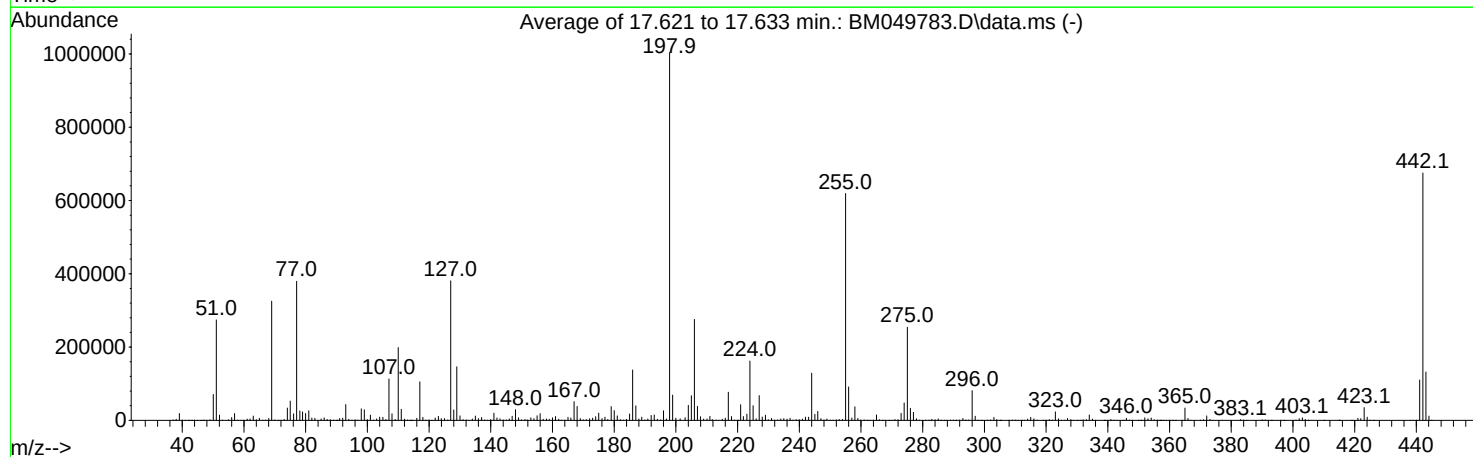


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040225\
Data File : BM049783.D
Acq On : 02 Apr 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 14:55:34 2025

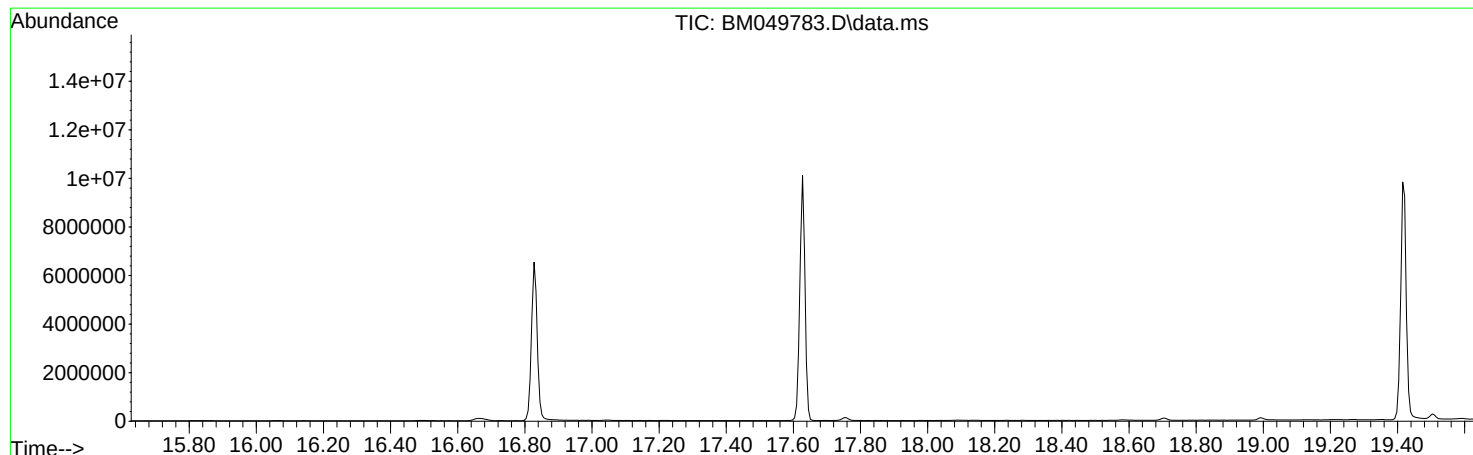

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	274186	PASS
68	69	0.00	2	1.6	5067	PASS
69	198	0.00	100	32.4	325499	PASS
70	69	0.00	2	0.4	1431	PASS
127	198	10	80	37.9	380693	PASS
197	198	0.00	2	0.4	3990	PASS
198	198	100	100	100.0	1003989	PASS
199	198	5	9	6.9	69243	PASS
275	198	10	60	25.3	254059	PASS
365	198	1	100	3.3	33576	PASS
441	198	0.01	100	11.0	110251	PASS
442	442	50	100	100.0	675136	PASS
443	442	15	24	19.5	131715	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/2/2025	BNA_M	<u>BM049783.D</u>
Compound Name	Response	Retention Time
DDT	3204234	20.656
DDD	23648	20.268
DDE	1983	19.709
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25631	3229865	0.79

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040225\
Data File : BM049783.D
Acq On : 02 Apr 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 02 11:48:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

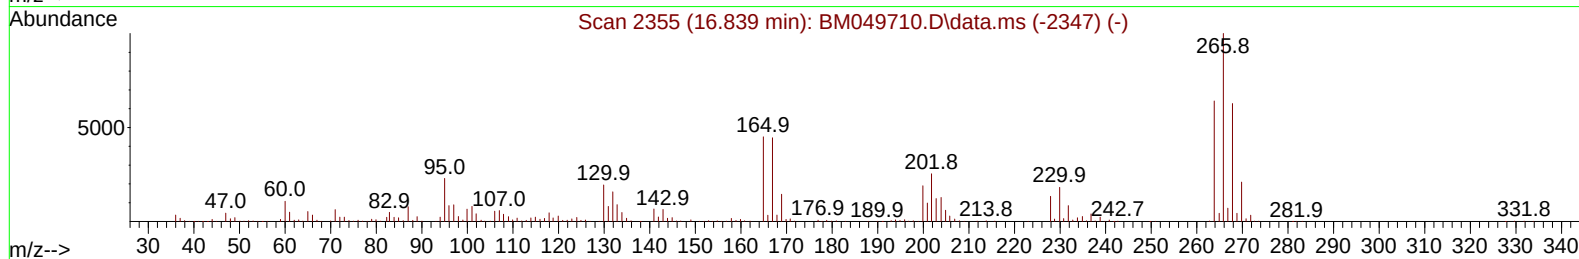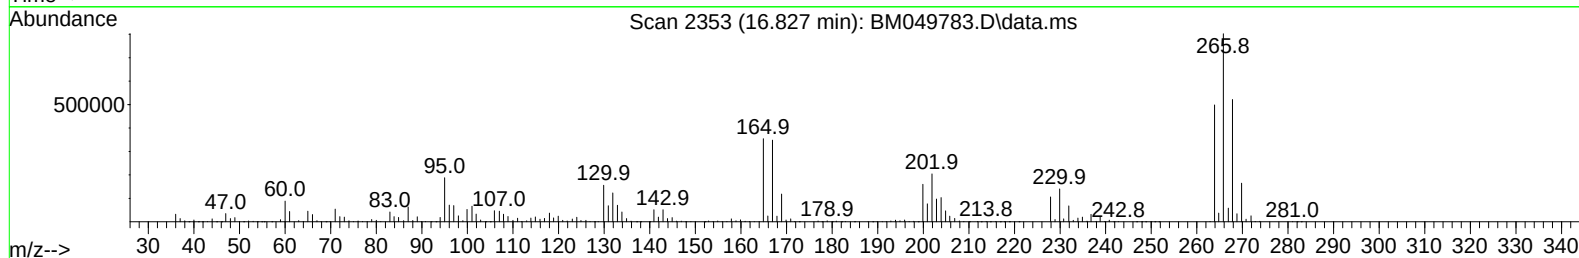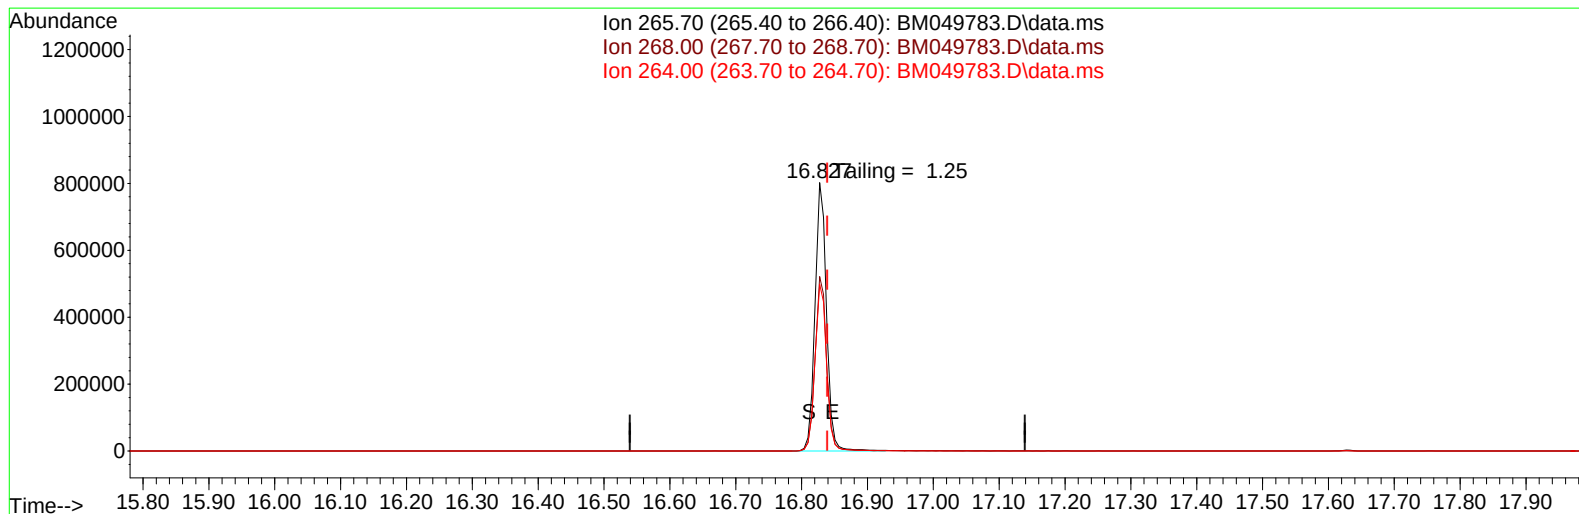

TIC: BM049783.D\data.ms

(70) Pentachlorophenol (C)

16.827min (-0.012) 68544.51 ng




response 974790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	65.02
264.00	64.10	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040225\
Data File : BM049783.D
Acq On : 02 Apr 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 02 11:48:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

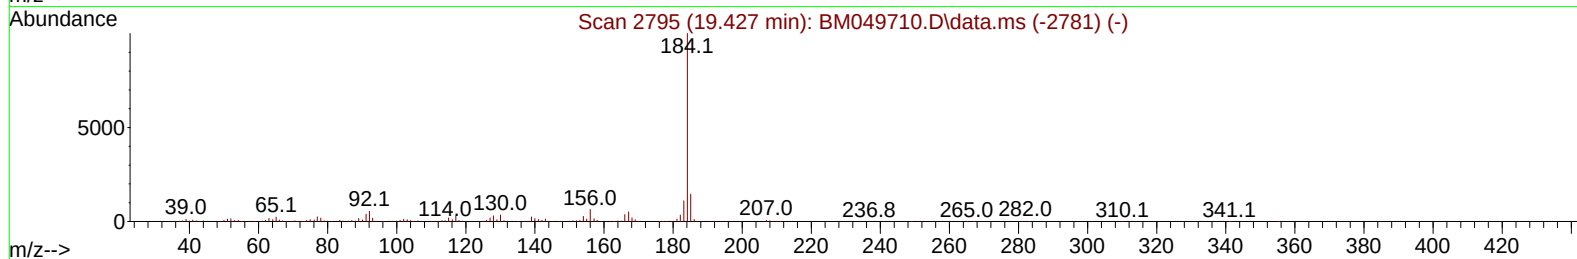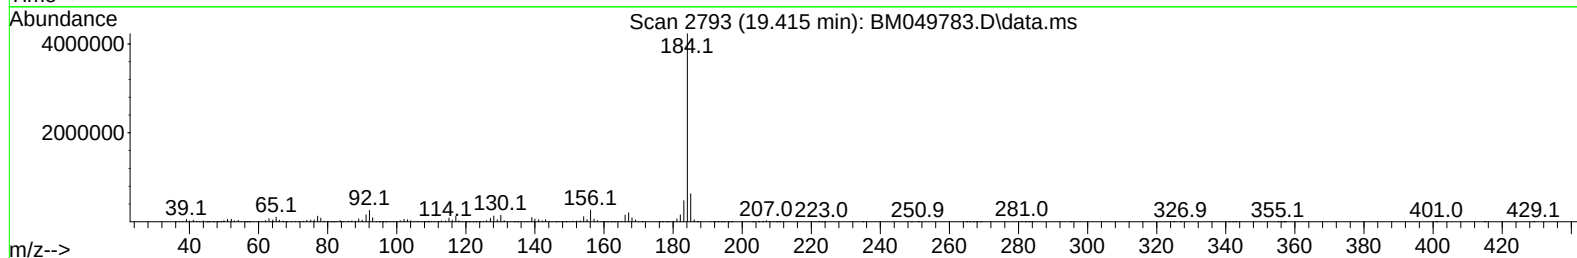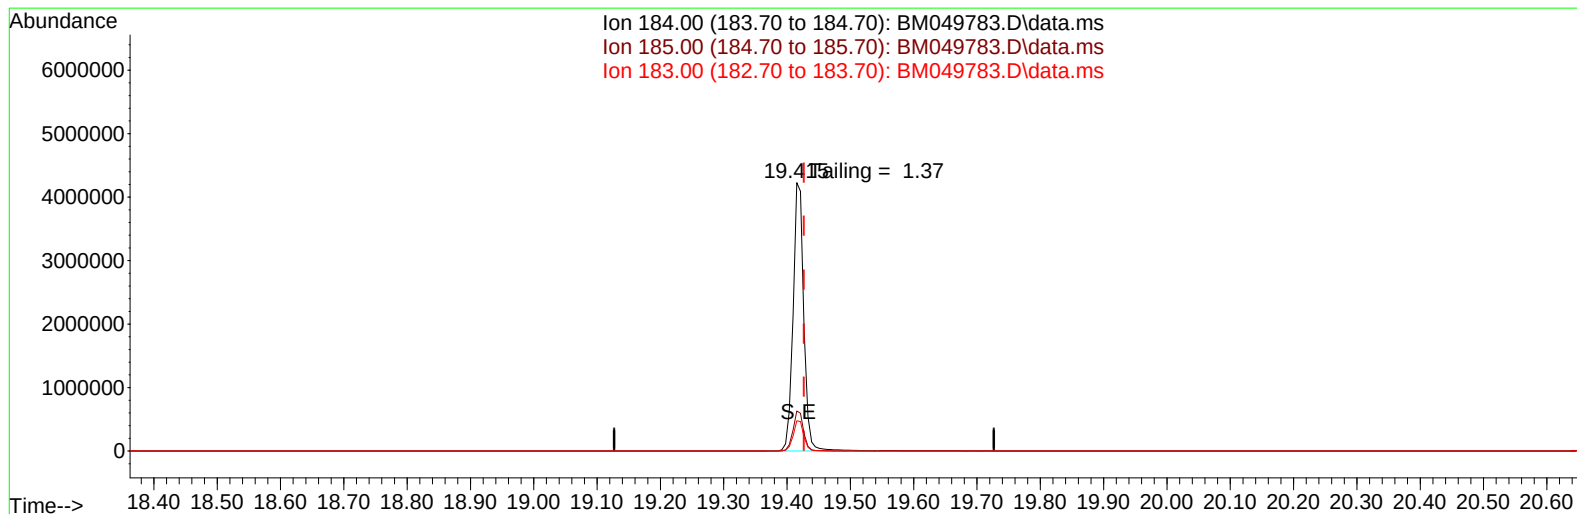

TIC: BM049783.D\data.ms

(77) Benzidine

19.415min (-0.012) 27579.90 ng

response 5011923

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.90
183.00	11.00	11.28
0.00	0.00	0.00