


Data Path : Z:\HPCHEM1\BNA_M\Data\BM040315\
 Data File : BM000840.D
 Acq On : 03 Apr 2015 17:37
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 03 18:16:53 2015

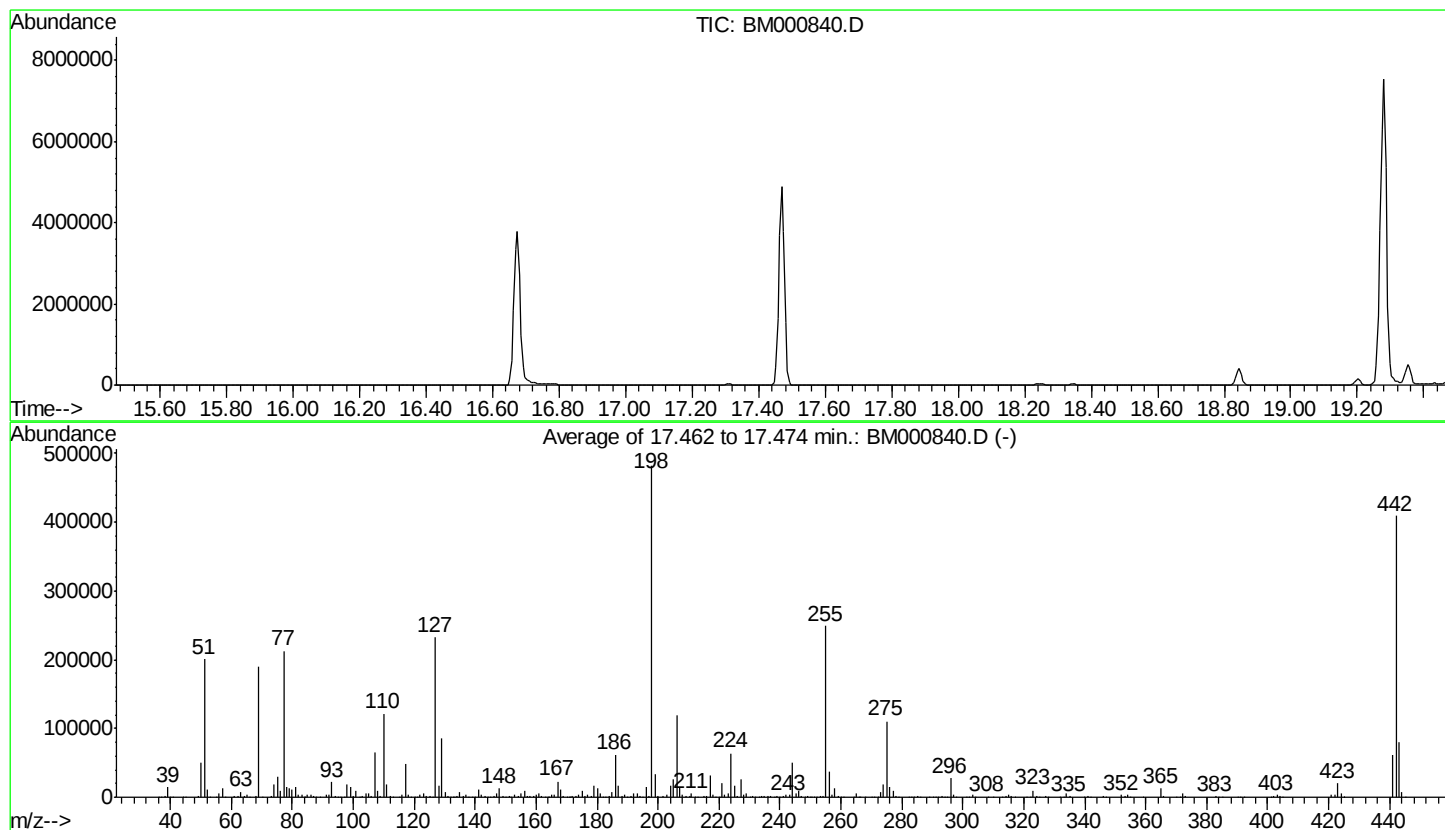

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	200832	PASS
68	69	0.00	2	1.4	2609	PASS
69	198	0.00	100	39.3	189461	PASS
70	69	0.00	2	0.5	983	PASS
127	198	10	80	48.3	232725	PASS
197	198	0.00	2	0.5	2554	PASS
198	198	100	100	100.0	482304	PASS
199	198	5	9	7.0	33552	PASS
275	198	10	60	22.9	110602	PASS
365	198	1	100	2.5	12291	PASS
441	442	0.01	24	14.9	60981	PASS
442	198	50	100	84.8	408938	PASS
443	442	15	24	19.7	80466	PASS