


Data Path : Z:\HPCHEM1\BNA M\DATA\BM040315\
 Data File : BM000810.D
 Acq On : 02 Apr 2015 17:22
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 03 18:16:53 2015

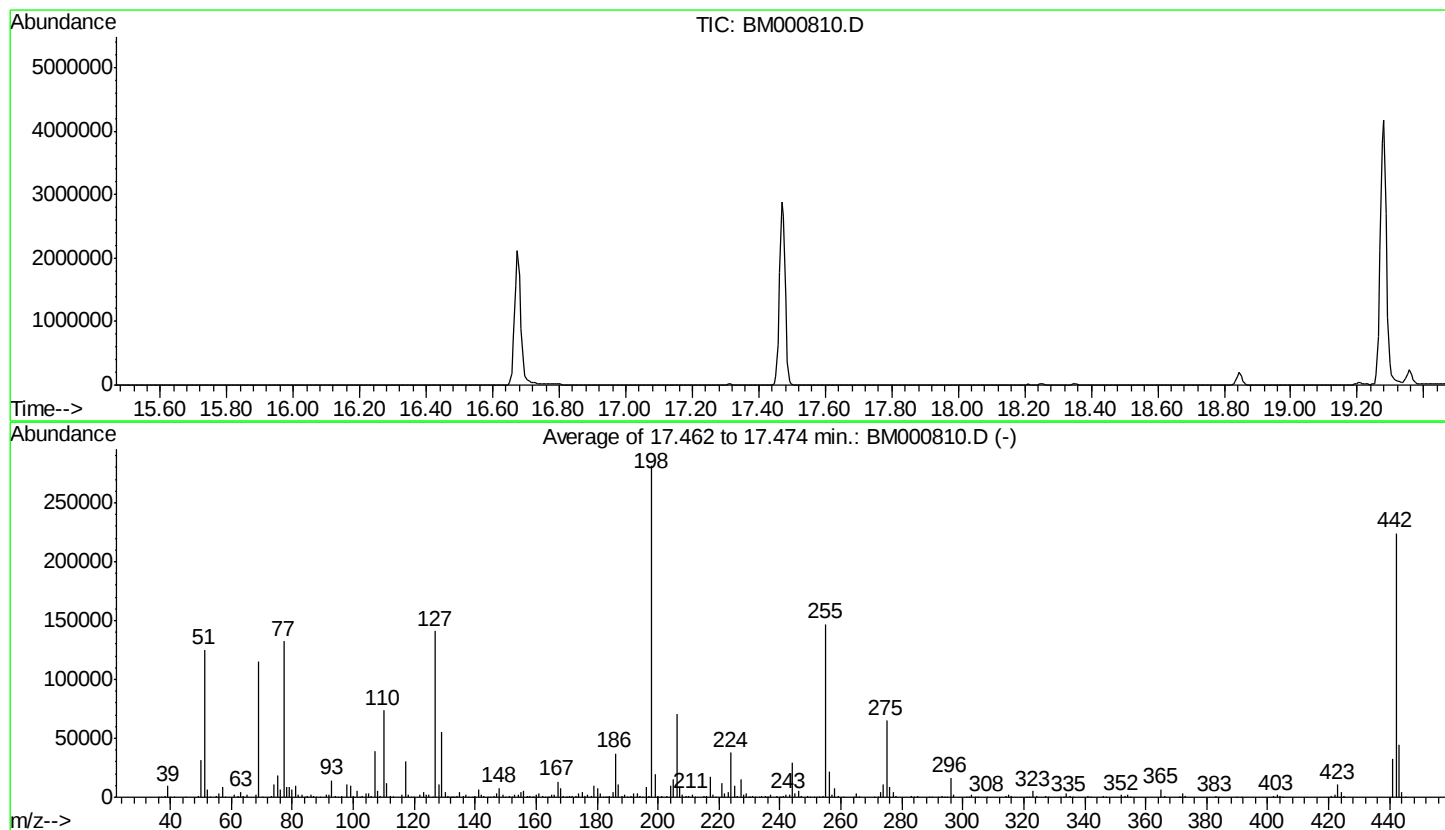

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	125266	PASS
68	69	0.00	2	1.7	1978	PASS
69	198	0.00	100	40.9	115149	PASS
70	69	0.00	2	0.5	557	PASS
127	198	10	80	50.1	141125	PASS
197	198	0.00	2	0.3	939	PASS
198	198	100	100	100.0	281578	PASS
199	198	5	9	6.8	19180	PASS
275	198	10	60	23.0	64768	PASS
365	198	1	100	2.5	7062	PASS
441	442	0.01	24	14.7	32882	PASS
442	198	50	100	79.7	224368	PASS
443	442	15	24	19.7	44229	PASS