

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040317\
 Data File : BM009512.D
 Acq On : 03 Apr 2017 22:17
 Operator : SJ/MA
 Sample : I2508-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-B53-B57-001

Quant Time: Apr 04 01:23:20 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 12:10:26 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	103837	20.00	ng	-0.02
21) Naphthalene-d8	10.64	136	407760	20.00	ng	-0.02
38) Acenaphthene-d10	14.49	164	172599	20.00	ng	-0.02
63) Phenanthrene-d10	17.24	188	541356	20.00	ng	-0.01
75) Chrysene-d12	21.42	240	654571	20.00	ng	-0.01
86) Perylene-d12	23.73	264	144790	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	958137	153.80	ng	-0.01
7) Phenol-d6	7.00	99	1131477	133.19	ng	-0.02
23) Nitrobenzene-d5	9.01	82	1012845	93.13	ng	-0.02
41) 2,4,6-Tribromophenol	15.98	330	467716	218.13	ng	-0.02
44) 2-Fluorobiphenyl	13.10	172	1772023	123.71	ng	-0.02
78) Terphenyl-d14	19.86	244	3039128	97.02	ng	-0.01
Target Compounds						
12) 1,3-Dichlorobenzene	7.73	146	17941	2.37	ng	# 82
13) 1,4-Dichlorobenzene	7.88	146	77908	9.97	ng	92
14) 1,2-Dichlorobenzene	8.20	146	679717	89.58	ng	# 94
16) 2,2'-oxybis(1-Chloropropan	8.37	45	33395	2.55	ng	96
31) Naphthalene	10.69	128	822807	38.02	ng	100
37) 2-Methylnaphthalene	12.30	142	237970	15.93	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040317\
Data File : BM009512.D
Acq On : 03 Apr 2017 22:17
Operator : SJ/MA
Sample : I2508-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-B53-B57-001

Quant Time: Apr 04 01:23:20 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 12:10:26 2017
Response via : Initial Calibration

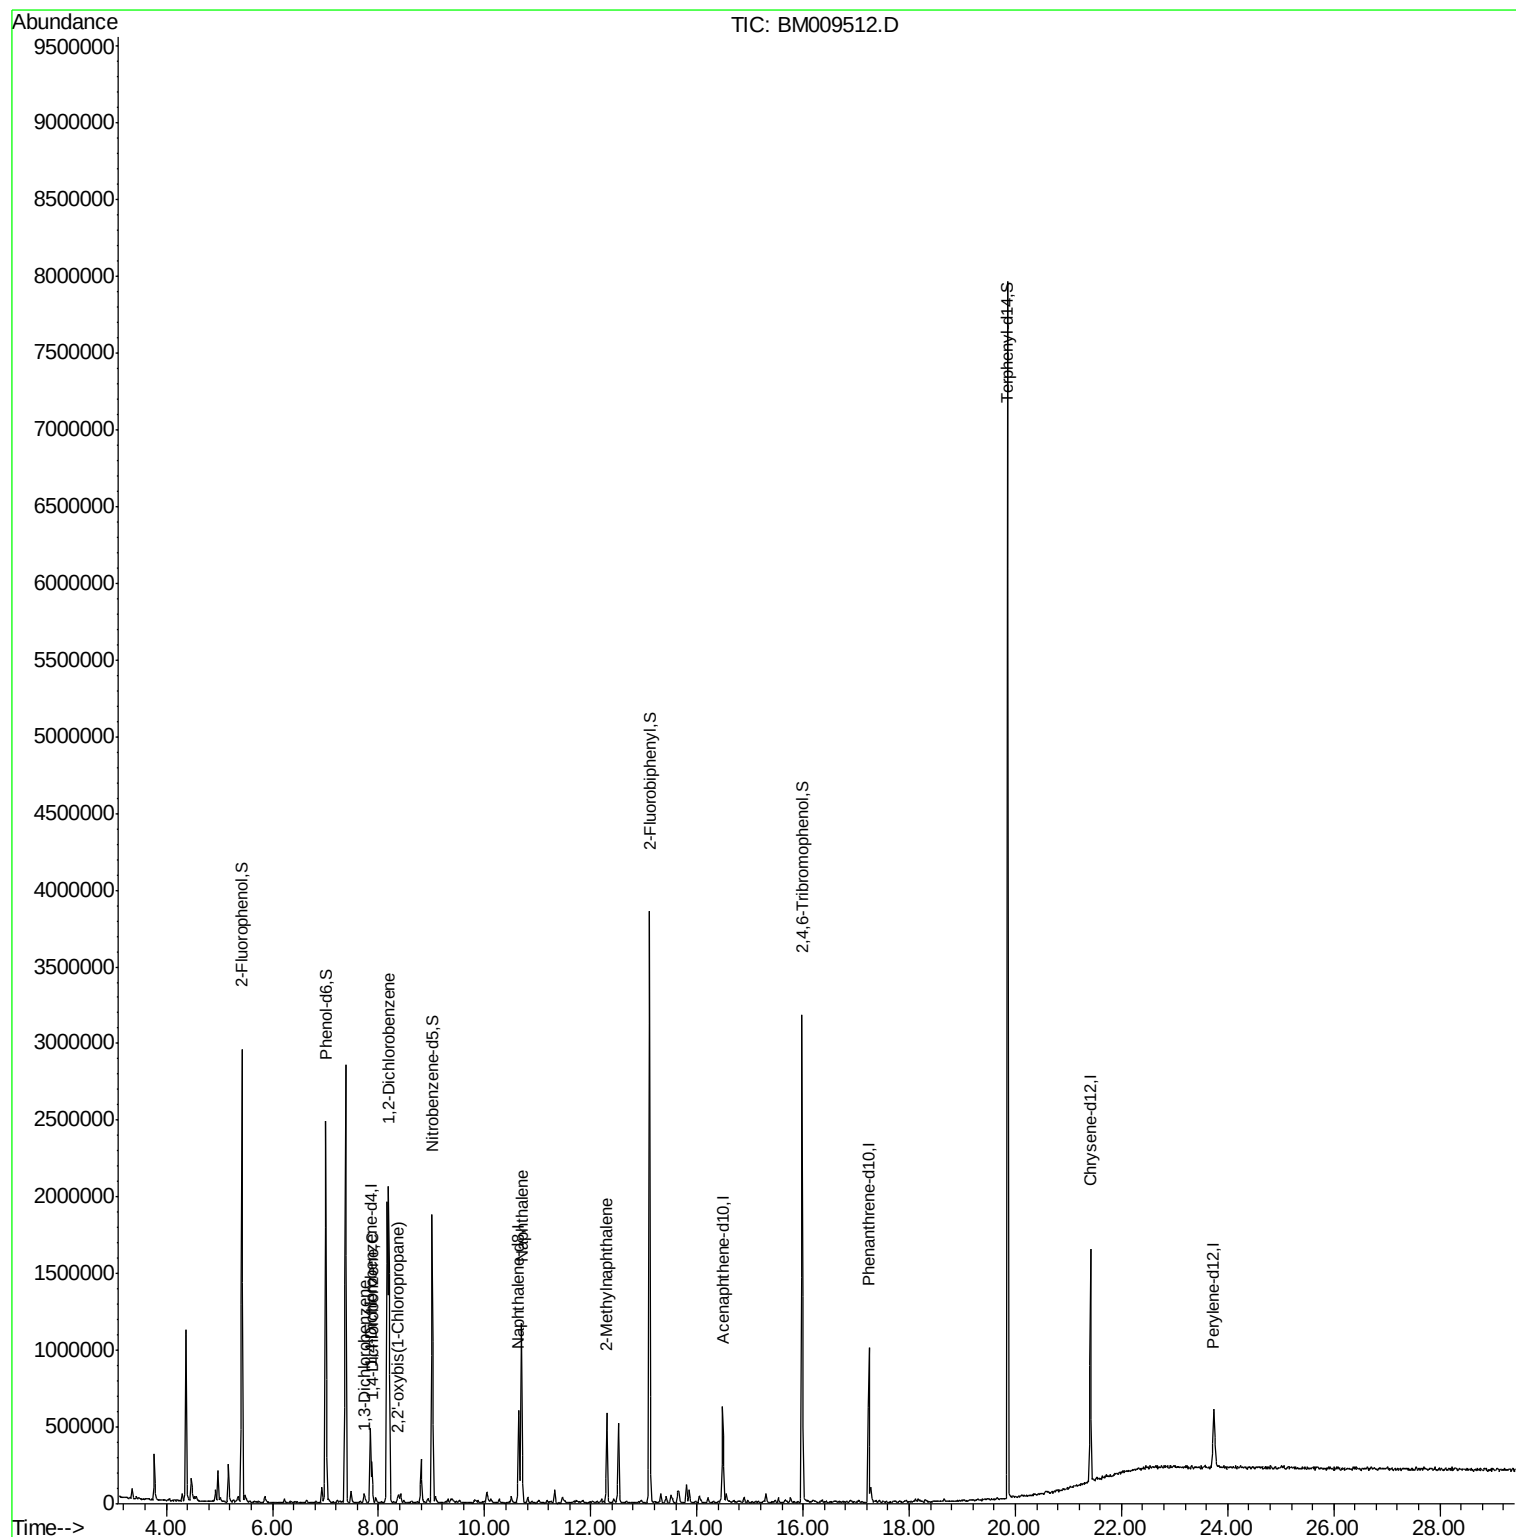

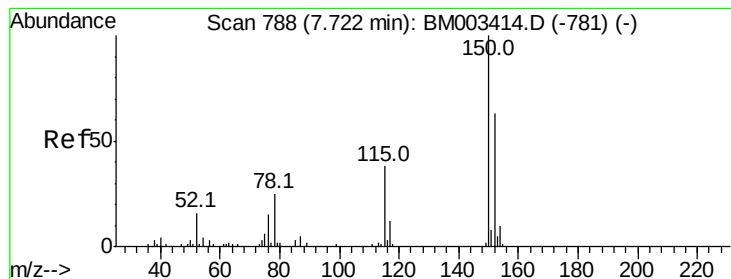


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.85 min Scan# 809
Delta R.T. -0.02 min
Lab File: BM009512.D
Acq: 03 Apr 2017 22:17

Instrument :
BNA_M
ClientSampleId :
WC-B53-B57-001

Tot Ion:152 Resp: 103837
Ion Ratio Lower Upper
152 100
150 161.1 119.5 179.3
115 74.1 43.0 64.4#




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

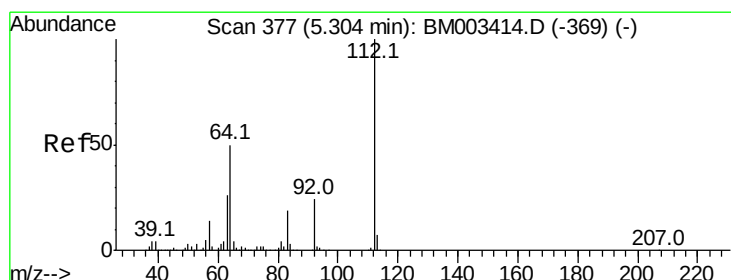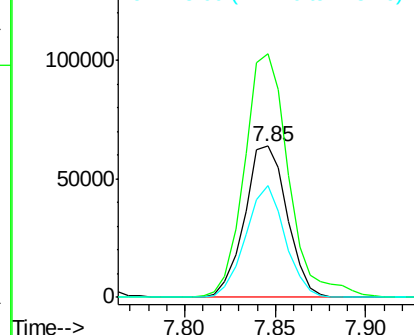



#5


2-Fluorophenol
Concen: 153.80 ng
RT: 5.42 min Scan# 397
Delta R.T. -0.01 min
Lab File: BM009512.D
Acq: 03 Apr 2017 22:17

Tgt Ion:112 Resp: 958137
Ion Ratio Lower Upper
112 100
64 77.9 38.6 57.8#
63 43.6 19.3 28.9#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

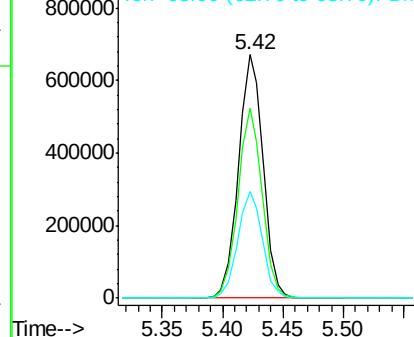



#7

Phenol-d6

Concen: 133.19 ng

RT: 7.00 min Scan# 666

Delta R.T. -0.02 min

Lab File: BM009512.D

Acq: 03 Apr 2017 22:17

Instrument :


BNA_M

ClientSampleId :

WC-B53-B57-001

Tot Ion: 99 Resp: 1131477

Ion	Ratio	Lower	Upper
99	100		
42	24.9	11.0	16.4#
71	44.0	23.4	35.2#






Abundance

Ion 99.00 (98.70 to 99.70): BM003414.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM003414.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM003414.D (-639) (-)

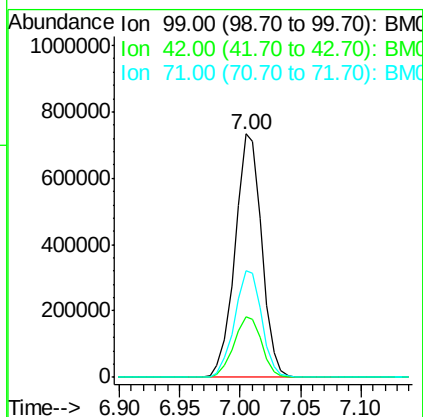

#12

1,3-Dichlorobenzene

Concen: 2.37 ng

RT: 7.73 min Scan# 790


Delta R.T. -0.01 min

Lab File: BM009512.D

Acq: 03 Apr 2017 22:17

Tgt Ion: 146 Resp: 17941

Ion	Ratio	Lower	Upper
146	100		
148	58.1	50.9	76.3
75	49.3	21.4	32.2#






Abundance

Ion 146.00 (145.70 to 146.70): BM003414.D (-762) (-)

Ion 148.00 (147.70 to 148.70): BM003414.D (-762) (-)

Ion 75.00 (74.70 to 75.70): BM003414.D (-762) (-)

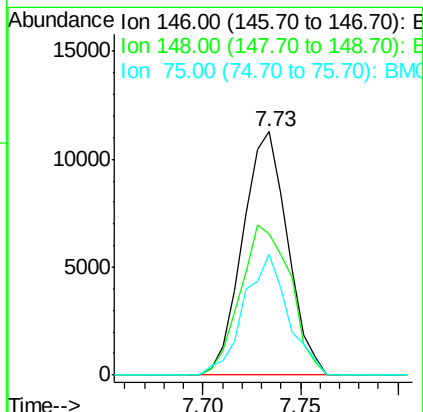

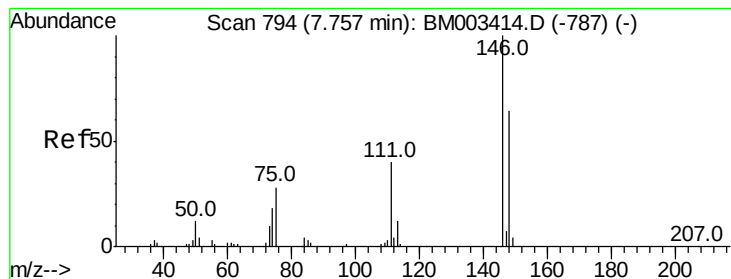

#13

1,4-Dichlorobenzene

Concen: 9.97 ng

RT: 7.88 min Scan# 815

Delta R.T. -0.02 min

Lab File: BM009512.D

Acq: 03 Apr 2017 22:17

Instrument :

BNA_M

ClientSampleId :

WC-B53-B57-001


Tot Ion:146 Resp: 77908

Ion Ratio Lower Upper

146 100

148 70.6 51.9 77.9




111 42.3 29.2 43.8



Abundance Ion 146.00 (145.70 to 146.70): E

Ion 148.00 (147.70 to 148.70): E

Ion 111.00 (110.70 to 111.70): E

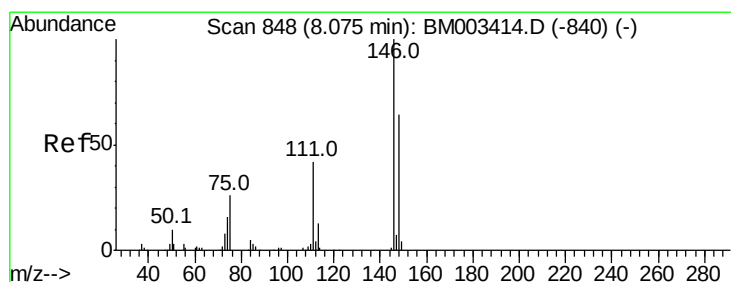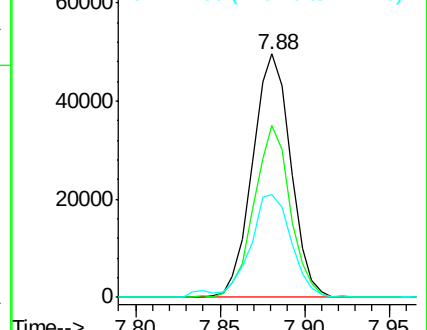

#14

1,2-Dichlorobenzene

Concen: 89.58 ng

RT: 8.20 min Scan# 869

Delta R.T. -0.02 min

Lab File: BM009512.D

Acq: 03 Apr 2017 22:17


Tgt Ion:146 Resp: 679717

Ion Ratio Lower Upper

146 100

148 64.8 52.3 78.5



111 46.5 30.6 45.8#

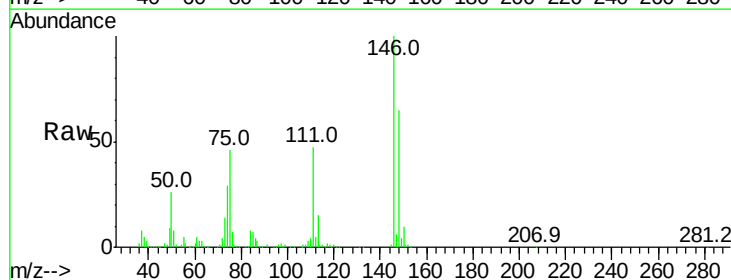


Abundance Ion 146.00 (145.70 to 146.70): E

Ion 148.00 (147.70 to 148.70): E

Ion 111.00 (110.70 to 111.70): E




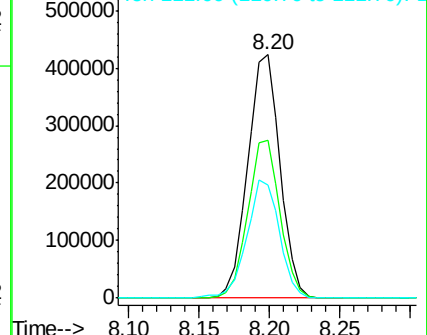


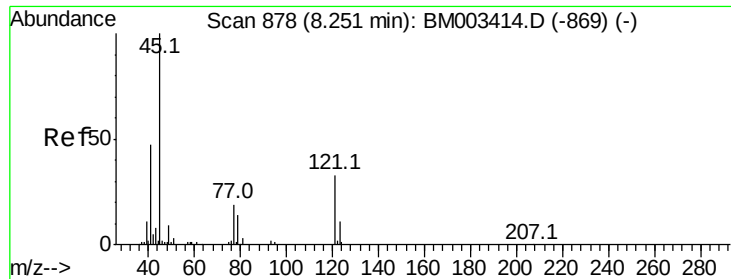

#16
 2,2'-oxvbis(1-Chloropropane)
 Concen: 2.55 ng
 RT: 8.37 min Scan# 898
 Delta R.T. -0.02 min
 Lab File: BM009512.D
 Acq: 03 Apr 2017 22:17




Instrument :
 BNA_M
 ClientSampleId :
 WC-B53-B57-001


Tot Ion:	45	Resp:	33395
Ion	Ratio	Lower	Upper
45	100		
77	14.6	0.0	35.2
79	14.5	0.0	32.0

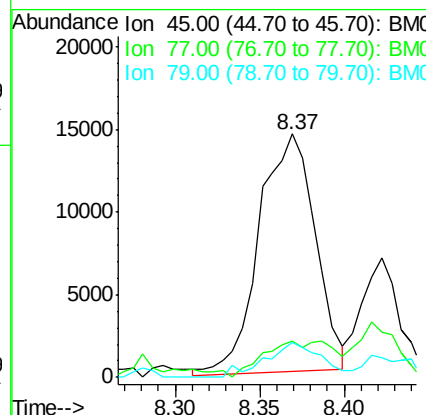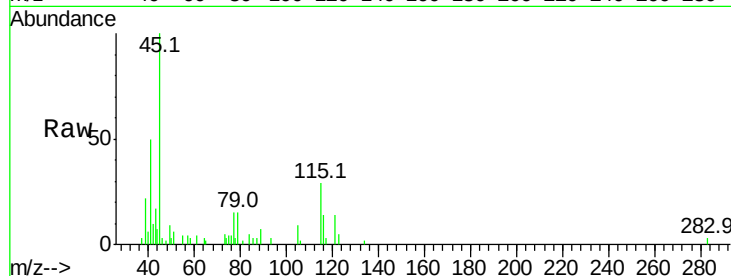

#21
 Naphthalene-d8
 Concen: 20.00 ng
 RT: 10.64 min Scan# 1284
 Delta R.T. -0.02 min
 Lab File: BM009512.D
 Acq: 03 Apr 2017 22:17

Tgt Ion:	136	Resp:	407760
Ion	Ratio	Lower	Upper
136	100		
137	11.6	8.7	13.1
54	12.7	4.6	6.8#
68	7.1	3.7	5.5#



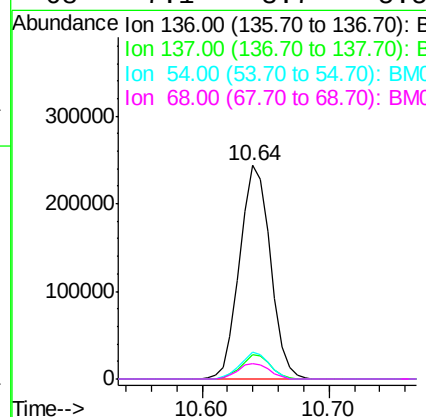



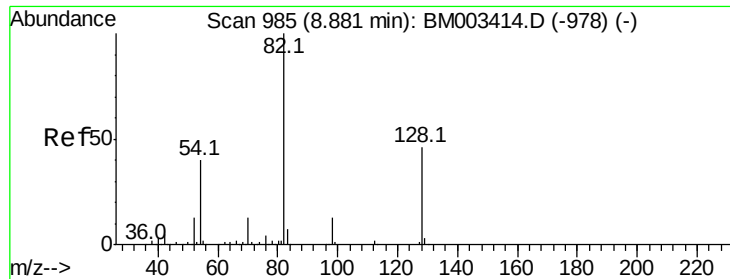

#23
 Nitrobenzene-d5
 Concen: 93.13 ng
 RT: 9.01 min Scan# 1007
 Delta R.T. -0.02 min
 Lab File: BM009512.D
 Acq: 03 Apr 2017 22:17




Instrument :
 BNA_M
 ClientSampleId :
 WC-B53-B57-001


Tot Ion: 82 Resp: 1012845
 Ion Ratio Lower Upper
 82 100
 128 32.2 32.8 49.2#
 54 56.3 40.6 60.8

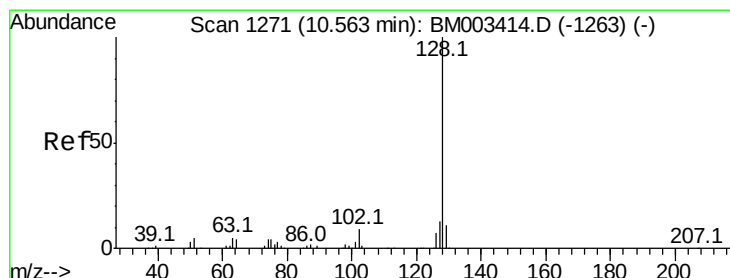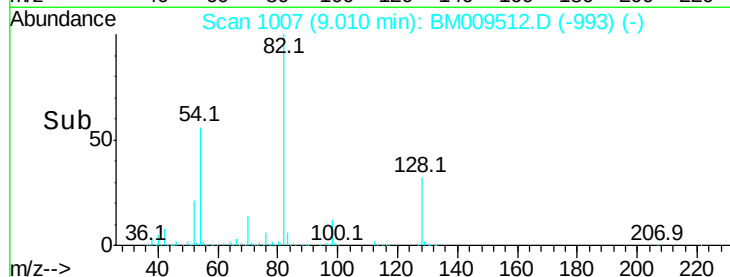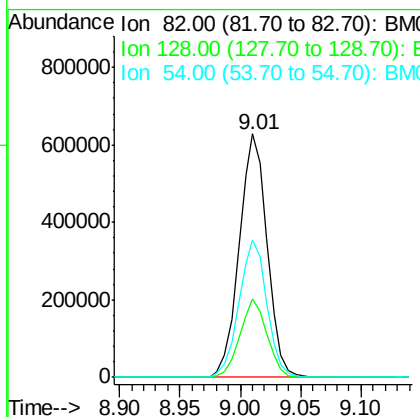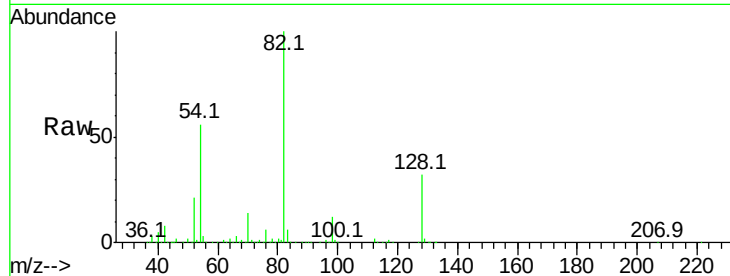

#31
 Naphthalene
 Concen: 38.02 ng
 RT: 10.69 min Scan# 1293
 Delta R.T. -0.02 min
 Lab File: BM009512.D
 Acq: 03 Apr 2017 22:17

Tgt Ion: 128 Resp: 822807
 Ion Ratio Lower Upper
 128 100
 129 10.8 8.9 13.3
 127 13.1 10.4 15.6


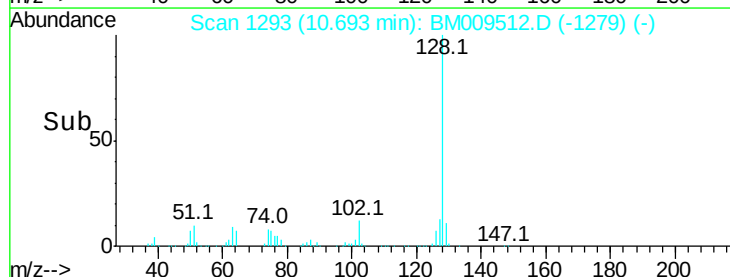
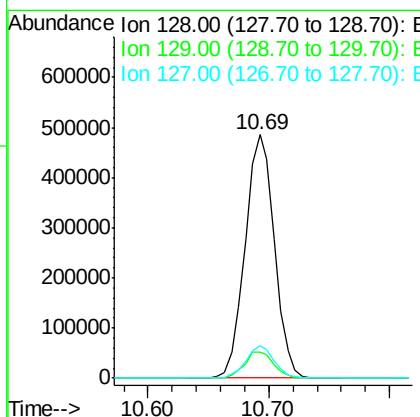
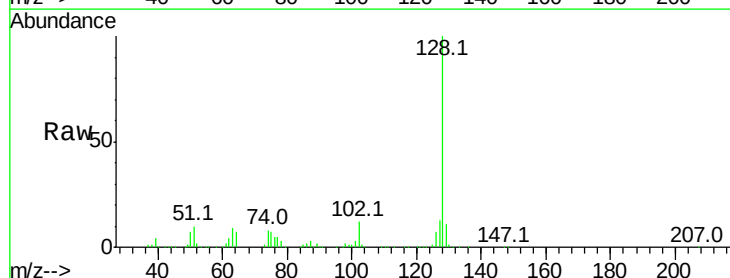


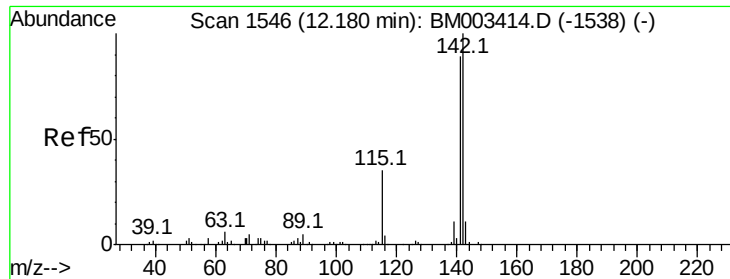

#37
 2-Methylnaphthalene
 Concen: 15.93 ng
 RT: 12.30 min Scan# 1567
 Delta R.T. -0.02 min
 Lab File: BM009512.D
 Acq: 03 Apr 2017 22:17




Instrument :
 BNA_M
 ClientSampleId :
 WC-B53-B57-001


Tot Ion	Ratio	Lower	Upper
142	100		
141	90.2	71.9	107.9
115	41.0	25.4	38.0

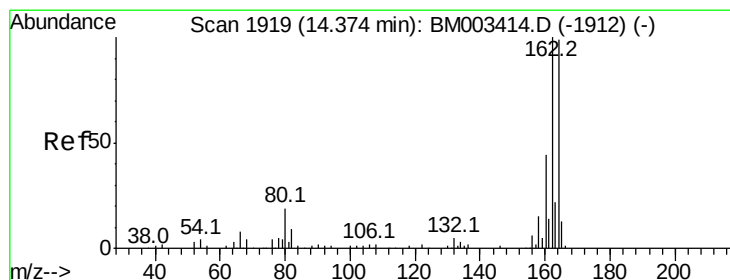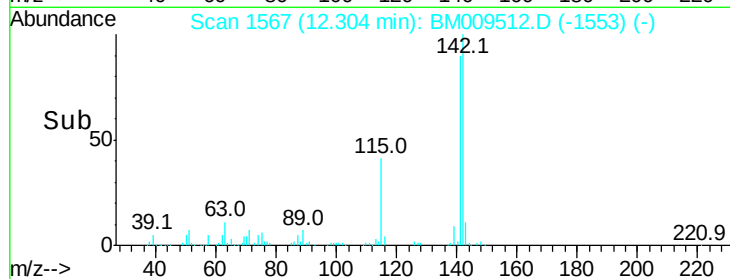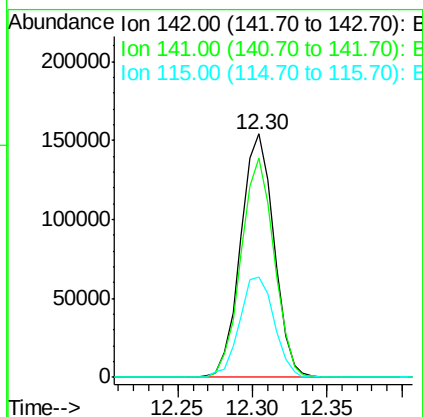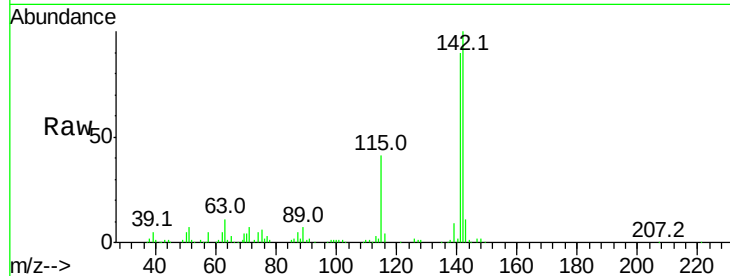

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.49 min Scan# 1938
 Delta R.T. -0.02 min
 Lab File: BM009512.D
 Acq: 03 Apr 2017 22:17

Tgt Ion	Ratio	Lower	Upper
164	100		
162	101.7	82.4	123.6
160	50.9	35.8	53.6

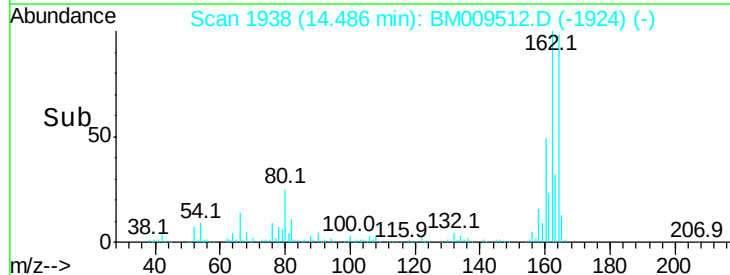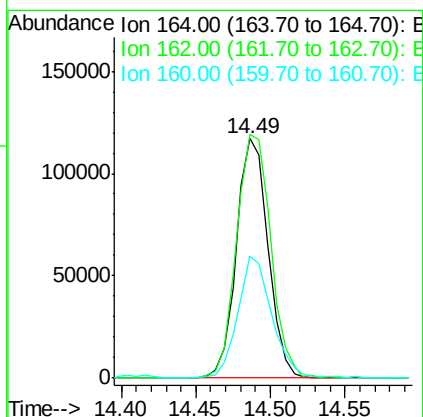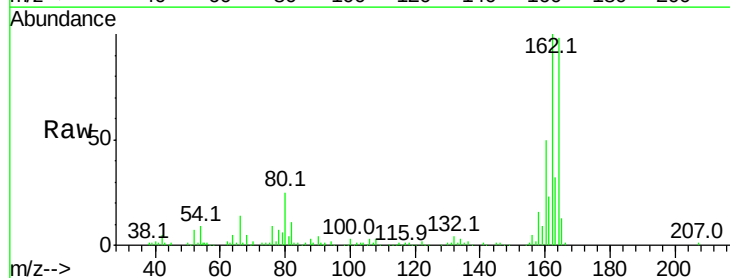

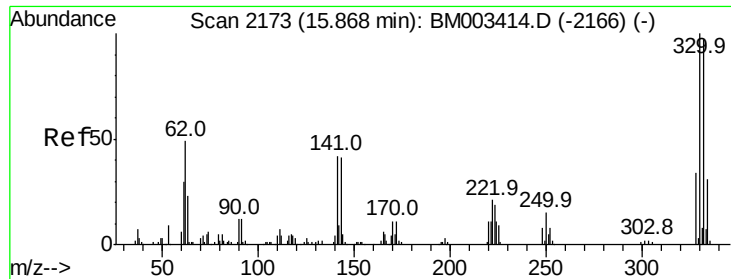

#41

2,4,6-Tribromophenol

Concen: 218.13 ng

RT: 15.98 min Scan# 2192

Delta R.T. -0.02 min

Lab File: BM009512.D

Acq: 03 Apr 2017 22:17

Instrument :

BNA_M

ClientSampleId :

WC-B53-B57-001


Tot Ion:330 Resp: 467716

Ion Ratio Lower Upper

330 100

332 97.1 0.0 0.0#




141 41.5 0.0 0.0#



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

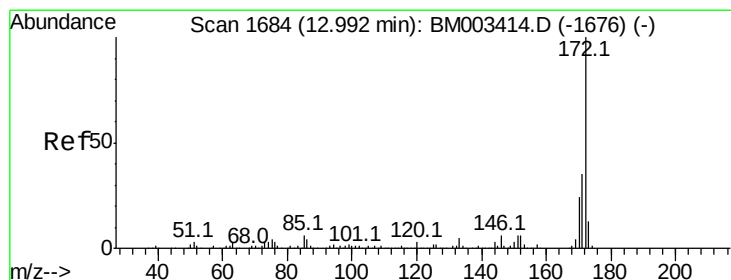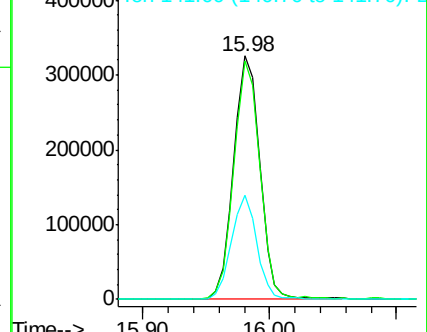

#44

2-Fluorobiphenyl

Concen: 123.71 ng

RT: 13.10 min Scan# 1703

Delta R.T. -0.02 min

Lab File: BM009512.D

Acq: 03 Apr 2017 22:17


Tgt Ion:172 Resp: 1772023

Ion Ratio Lower Upper

172 100

171 33.8 28.5 42.7



170 22.7 18.8 28.2




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

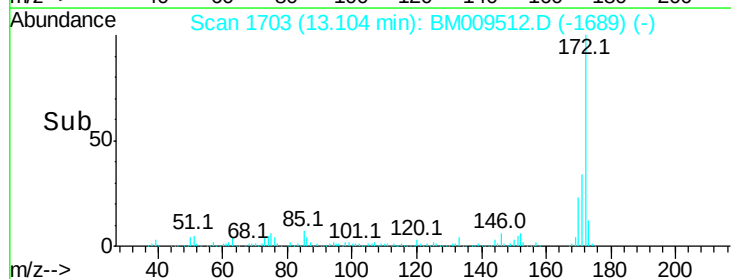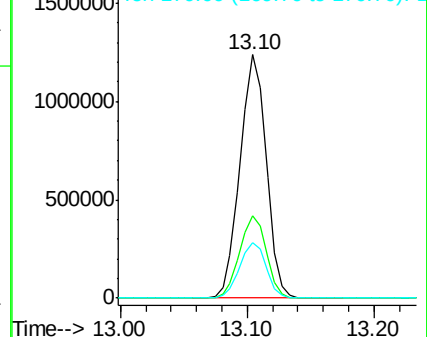







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.24 min Scan# 2406
Delta R.T. -0.01 min
Lab File: BM009512.D
Acq: 03 Apr 2017 22:17

Instrument :
BNA_M
ClientSampleId :
WC-B53-B57-001

Tot Ion:188 Resp: 541356
Ion Ratio Lower Upper
188 100
94 8.2 8.7 13.1#
80 10.5 9.3 13.9




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

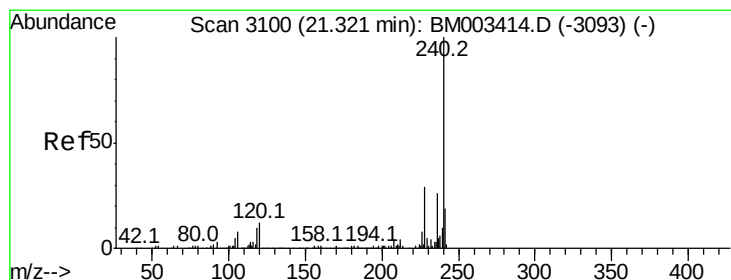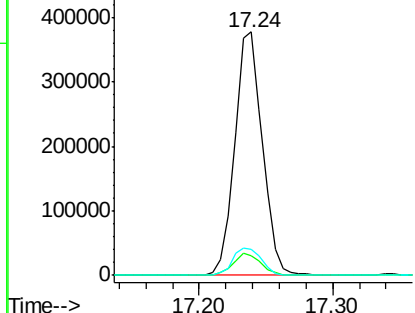




#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.42 min Scan# 3116
Delta R.T. -0.01 min
Lab File: BM009512.D
Acq: 03 Apr 2017 22:17

Tgt Ion:240 Resp: 654571
Ion Ratio Lower Upper
240 100
120 9.2 8.2 12.2
236 26.2 20.0 30.0



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

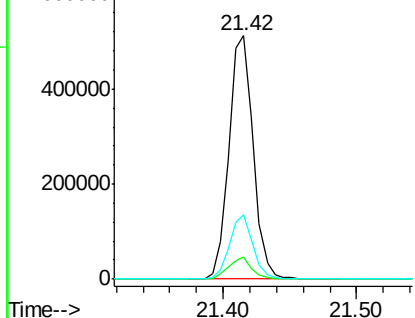

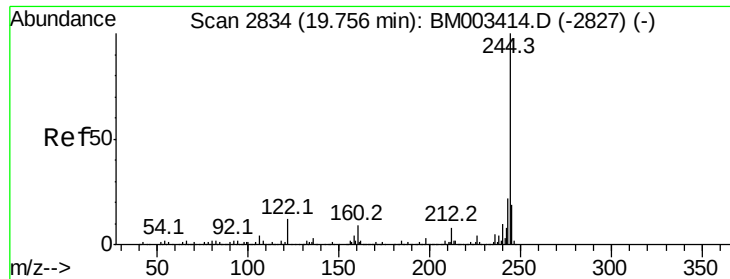

#78

Terphenyl-d14

Concen: 97.02 ng

RT: 19.86 min Scan# 2851

Delta R.T. -0.01 min

Lab File: BM009512.D

Acq: 03 Apr 2017 22:17

Instrument :

BNA_M

ClientSampleId :

WC-B53-B57-001


Tot Ion:244 Resp: 3039128

Ion Ratio Lower Upper

244 100

212 7.1 4.9 7.3




122 9.3 6.2 9.4

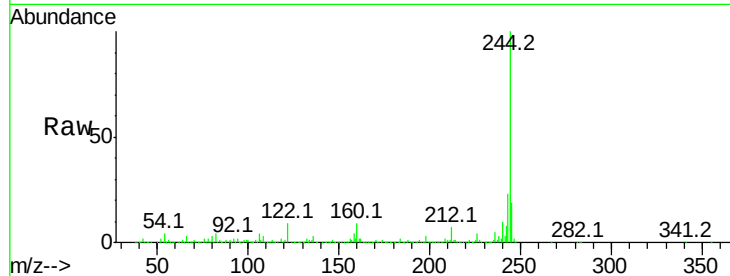

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

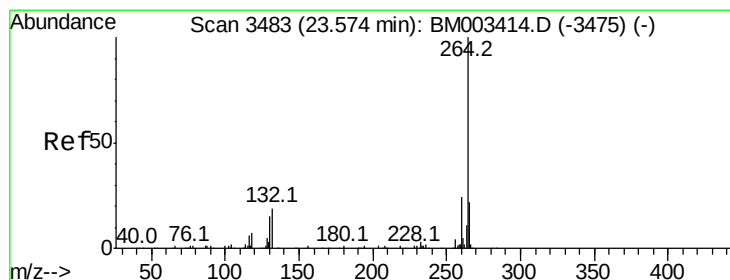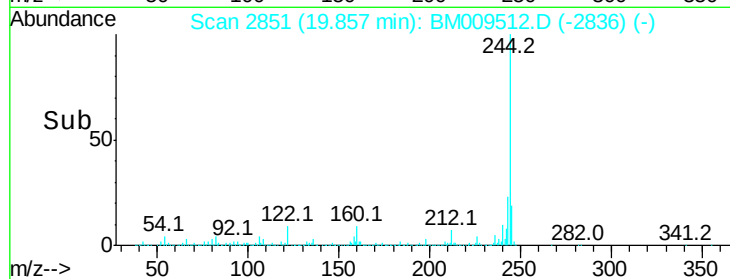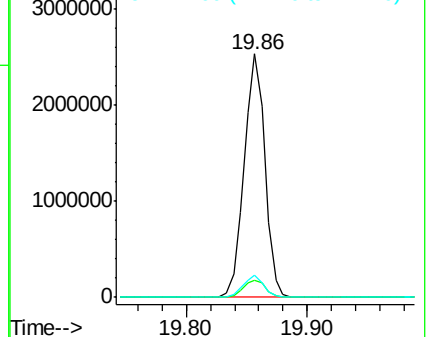

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.73 min Scan# 3510

Delta R.T. -0.02 min

Lab File: BM009512.D

Acq: 03 Apr 2017 22:17


Tgt Ion:264 Resp: 144790

Ion Ratio Lower Upper

264 100

260 34.3 18.6 27.8#

265 22.7 17.3 25.9

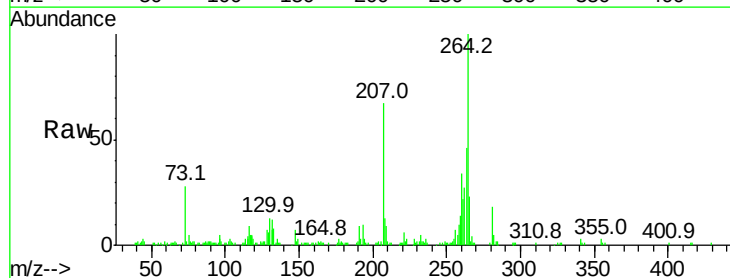

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

