
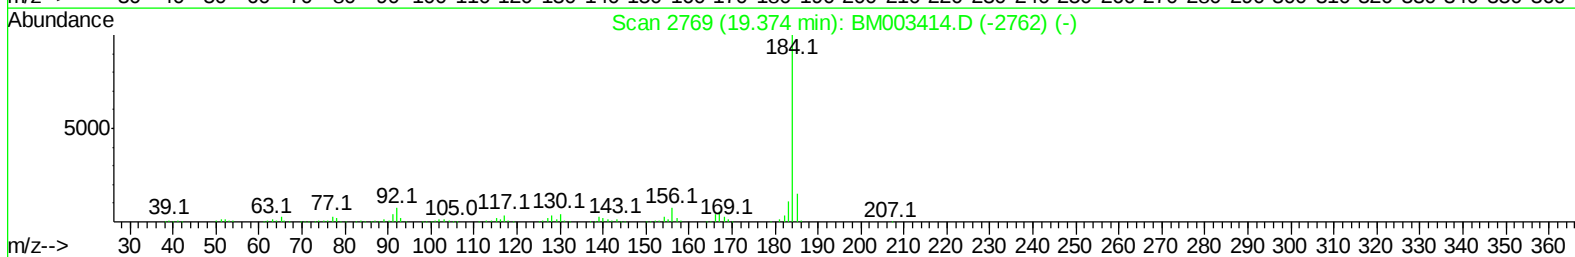
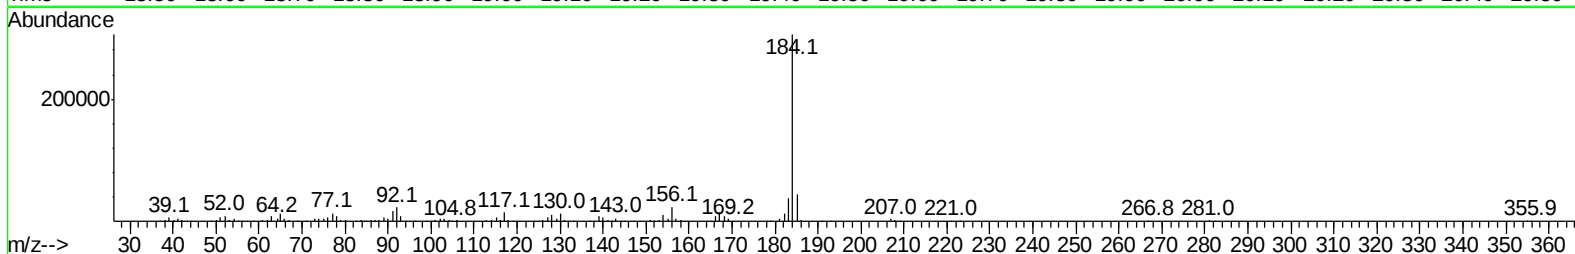


Data Path : U:\HPCHEM1\BNA M\Data\BM040317\
 Data File : BM009494.D
 Acq On : 03 Apr 2017 11:19
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 07:20:45 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 12:10:26 2017
 Response via : Initial Calibration

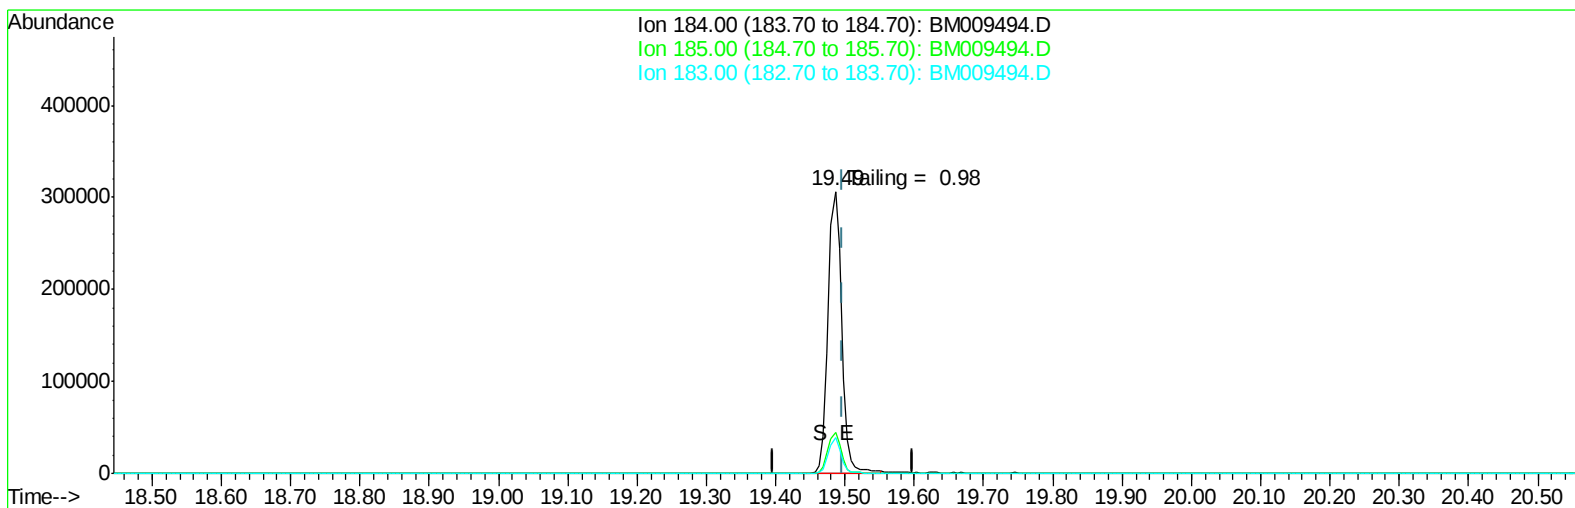

TIC: BM009494.D

(76) Benzidine




19.486min (-0.012) 53734.68ng

response 417984

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.36
183.00	11.10	12.65
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA M\Data\BM040317\
Data File : BM009494.D
Acq On : 03 Apr 2017 11:19
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 07:20:45 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 12:10:26 2017
Response via : Initial Calibration

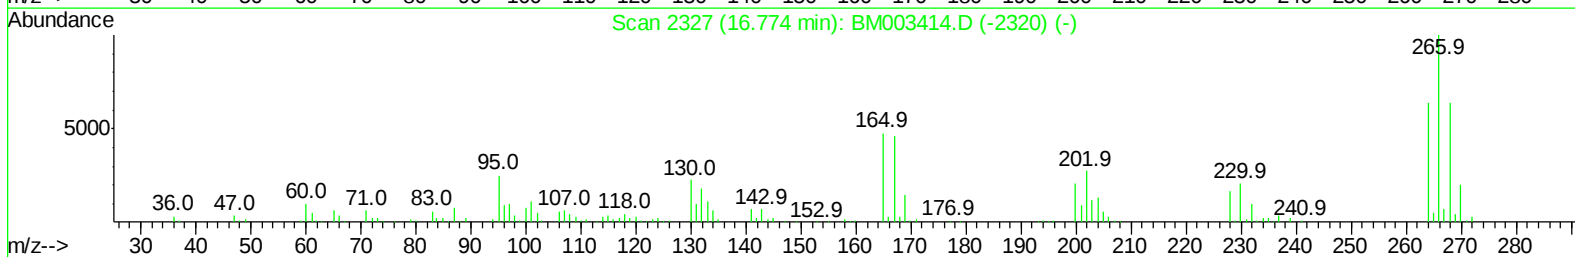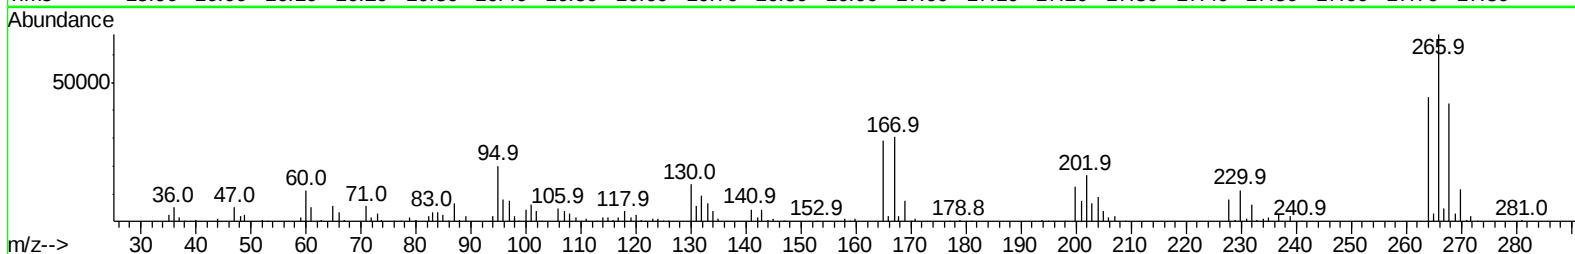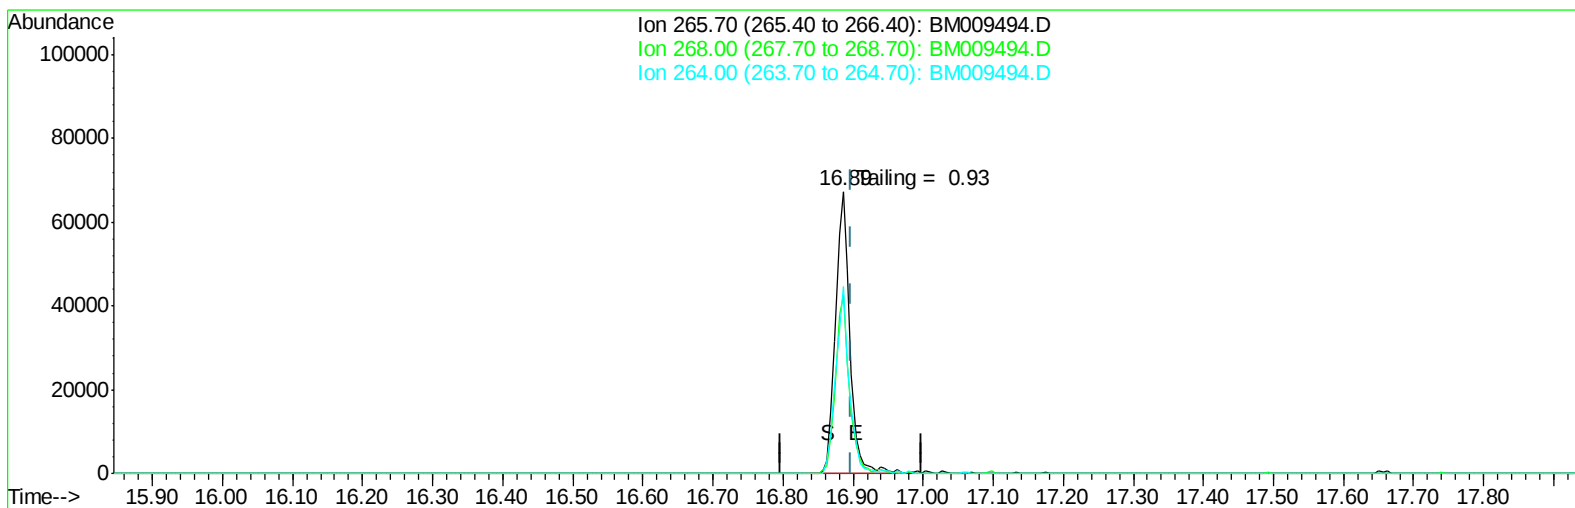

TIC: BM009494.D

(69) Pentachlorophenol (C)

16.886min (-0.012) 0.00ng

response 93855

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.11
264.00	61.20	66.28
0.00	0.00	0.00