
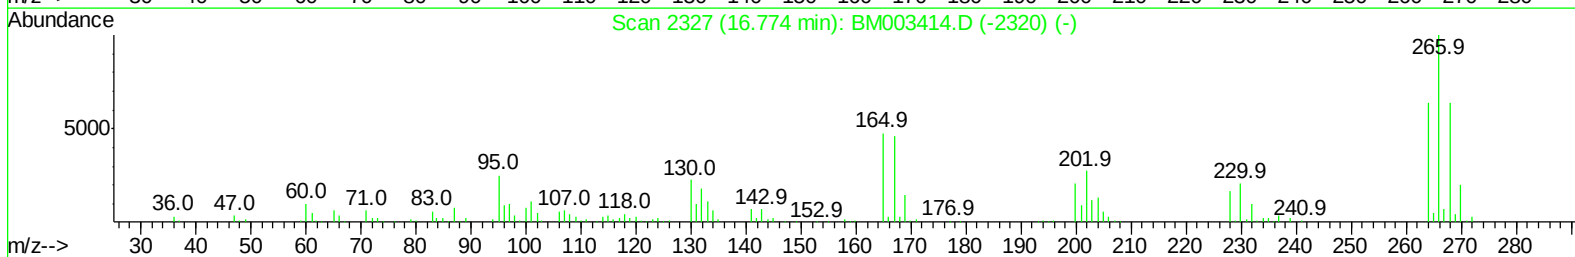
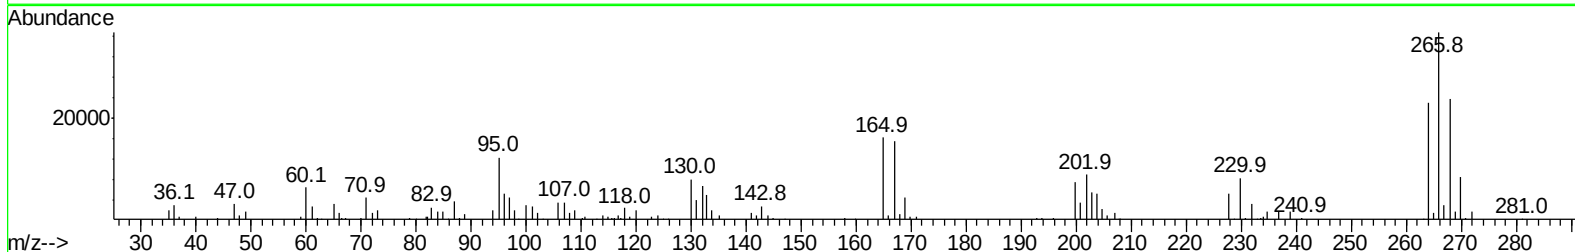


Data Path : U:\HPCHEM1\BNA M\Data\BM040317\
Data File : BM009498.D
Acq On : 03 Apr 2017 13:48
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 07:21:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 12:10:26 2017
Response via : Initial Calibration

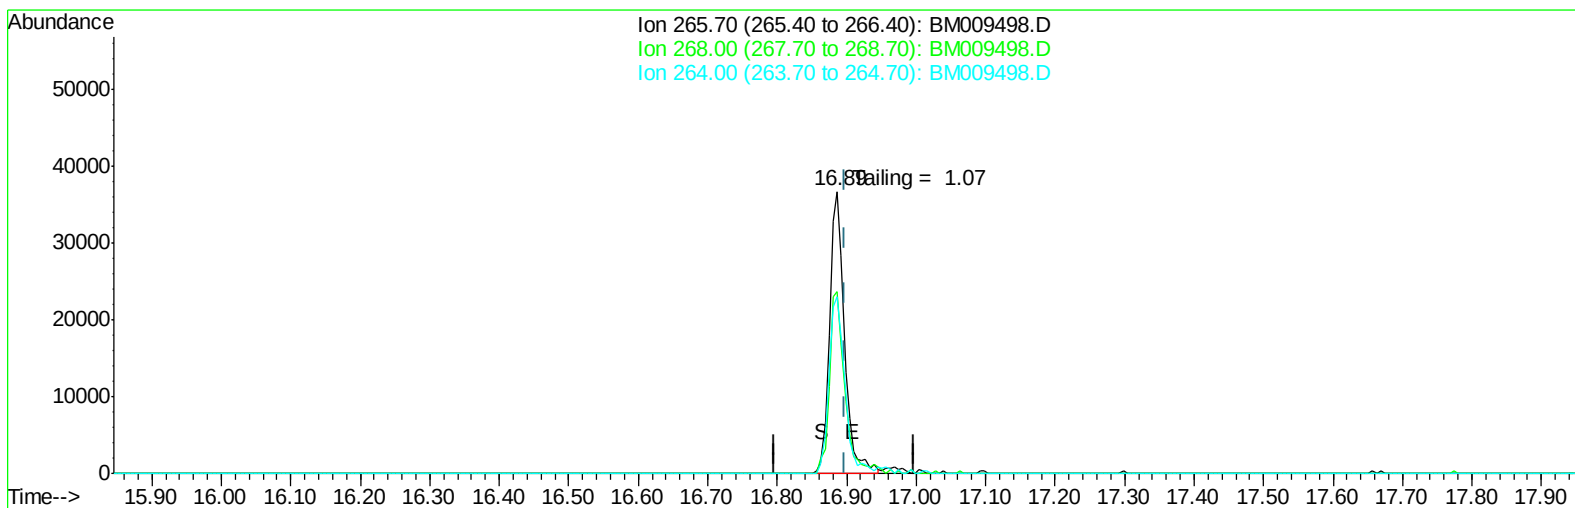

TIC: BM009498.D

(69) Pentachlorophenol (C)




16.886min (-0.011) 0.00ng

response 54880

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.71
264.00	61.20	62.94
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA M\Data\BM040317\
Data File : BM009498.D
Acq On : 03 Apr 2017 13:48
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 07:21:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 12:10:26 2017
Response via : Initial Calibration

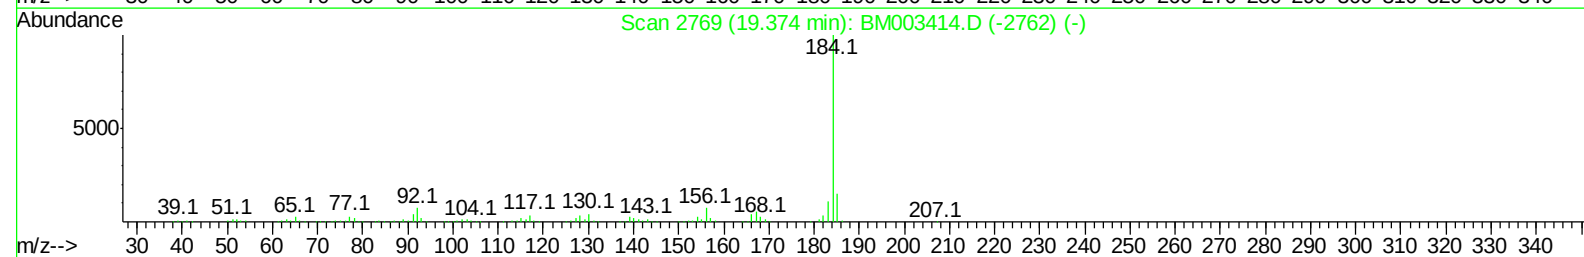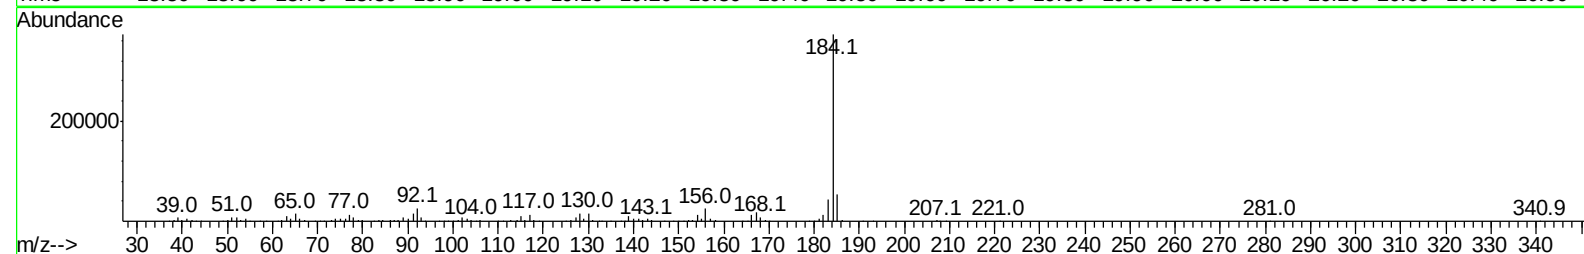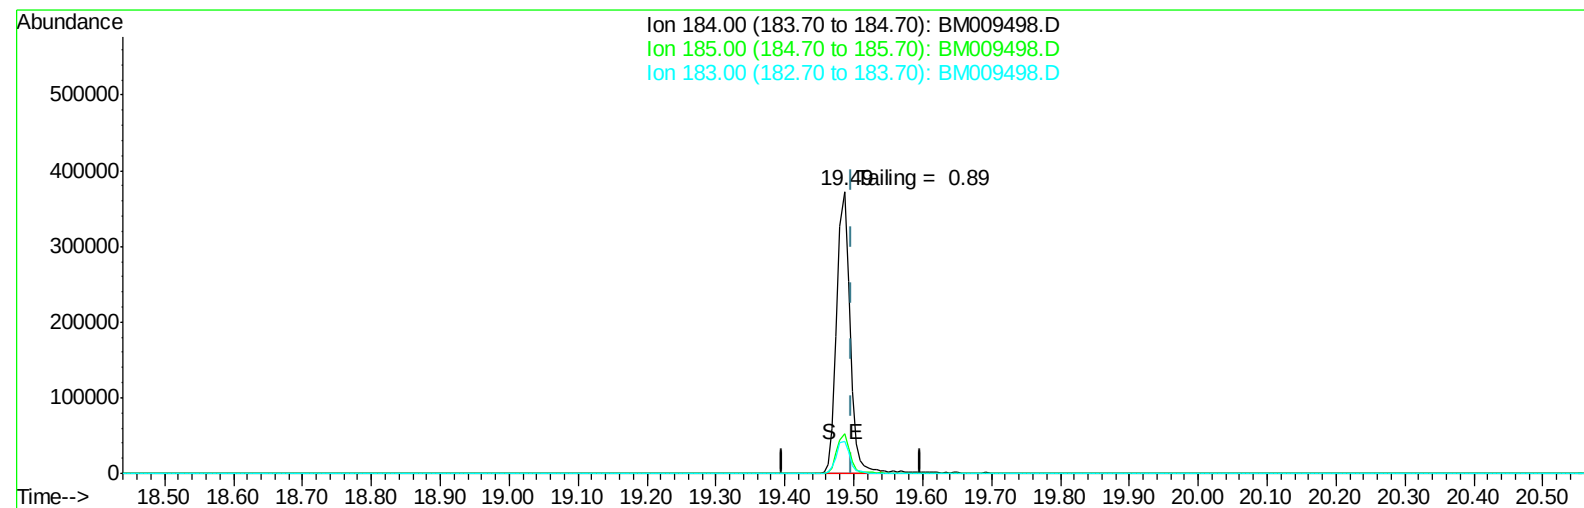

TIC: BM009498.D

(76) Benzidine

19.486min (-0.011) 25142.74ng

response 498309

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.25
183.00	11.10	11.41
0.00	0.00	0.00