

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040317\
 Data File : BM009500.D
 Acq On : 03 Apr 2017 15:05
 Operator : SJ/MA
 Sample : PB97981BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB97981BL

Quant Time: Apr 04 01:20:13 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 12:10:26 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	113027	20.00	ng	-0.02
21) Naphthalene-d8	10.65	136	416627	20.00	ng	-0.02
38) Acenaphthene-d10	14.49	164	230504	20.00	ng	-0.02
63) Phenanthrene-d10	17.24	188	556757	20.00	ng	-0.01
75) Chrysene-d12	21.42	240	769678	20.00	ng	-0.01
86) Perylene-d12	23.74	264	730102	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	951950	140.39	ng	-0.01
7) Phenol-d6	7.00	99	1289590	139.46	ng	-0.02
23) Nitrobenzene-d5	9.01	82	893588	80.42	ng	-0.02
41) 2,4,6-Tribromophenol	15.98	330	383274	133.85	ng	-0.02
44) 2-Fluorobiphenyl	13.10	172	1592806	83.26	ng	-0.02
78) Terphenyl-d14	19.86	244	2620692	71.15	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040317\
Data File : BM009500.D
Acq On : 03 Apr 2017 15:05
Operator : SJ/MA
Sample : PB97981BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB97981BL

Quant Time: Apr 04 01:20:13 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 12:10:26 2017
Response via : Initial Calibration

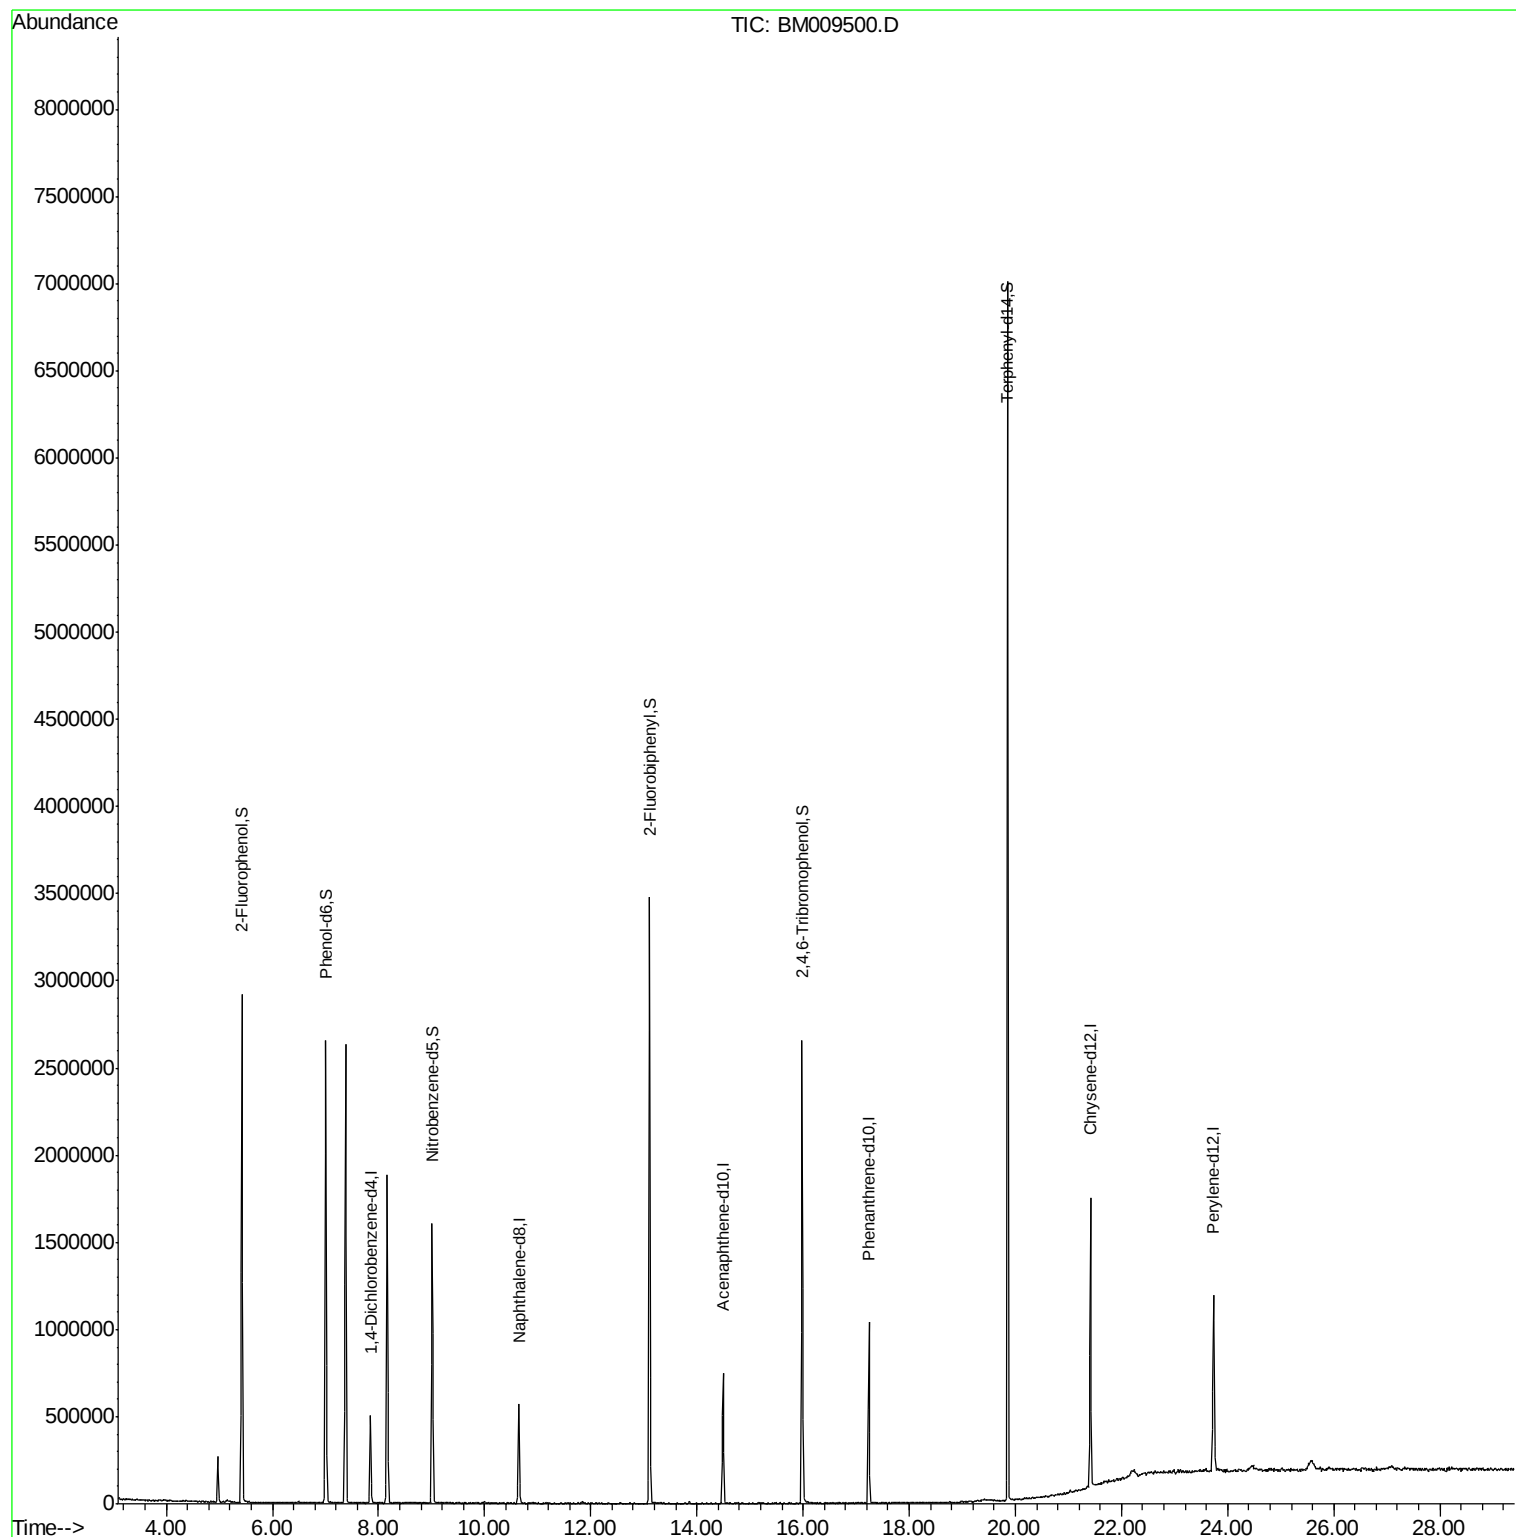

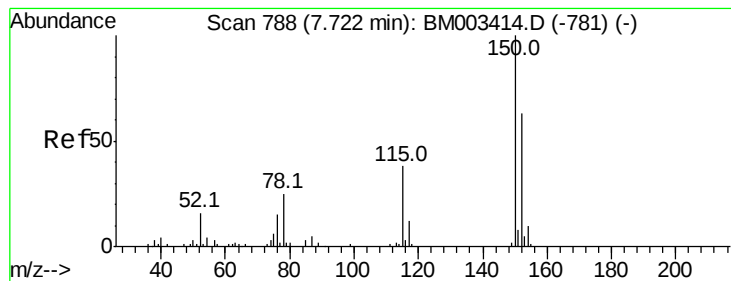


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.85 min Scan# 809
Delta R.T. -0.02 min
Lab File: BM009500.D
Acq: 03 Apr 2017 15:05

Instrument :
BNA_M
ClientSampleId :
PB97981BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.3	119.5	179.3
115	58.0	43.0	64.4

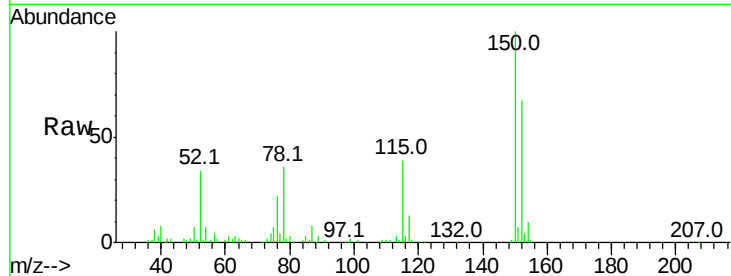


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

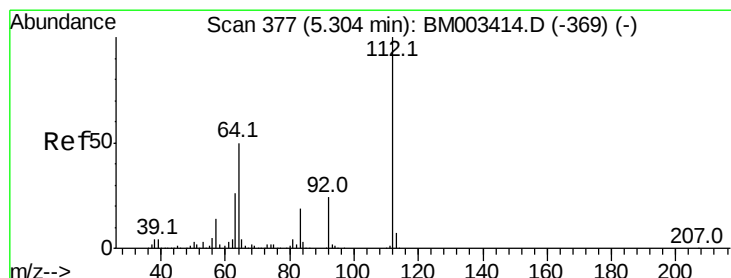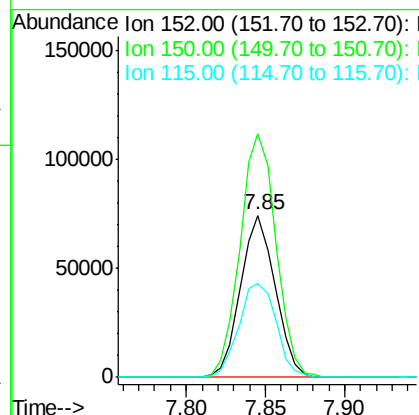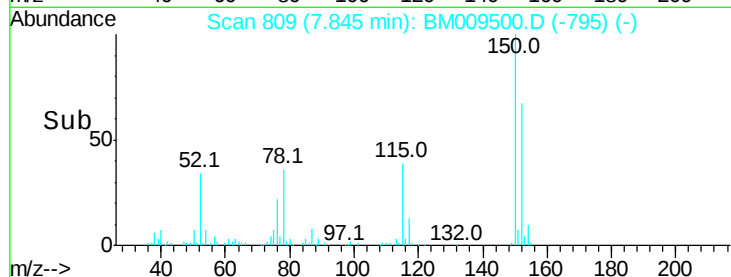



#5


2-Fluorophenol
Concen: 140.39 ng
RT: 5.42 min Scan# 397
Delta R.T. -0.01 min
Lab File: BM009500.D
Acq: 03 Apr 2017 15:05

Tgt Ion	Ratio	Lower	Upper
112	100		
64	74.1	38.6	57.8#
63	43.0	19.3	28.9#

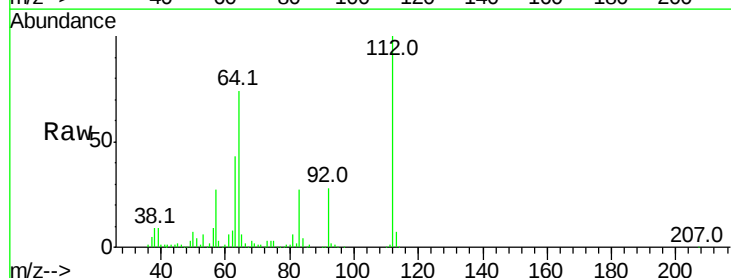

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

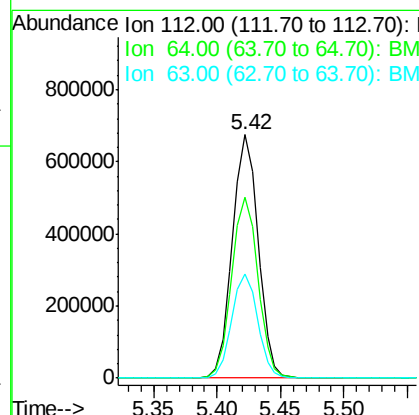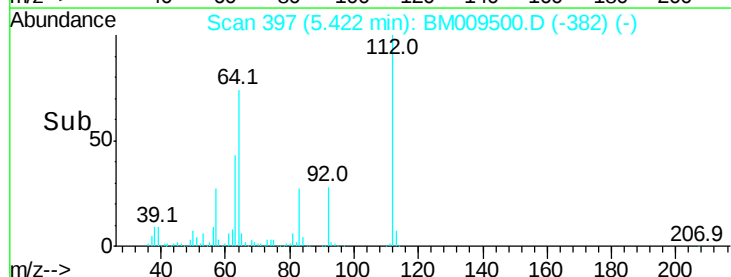

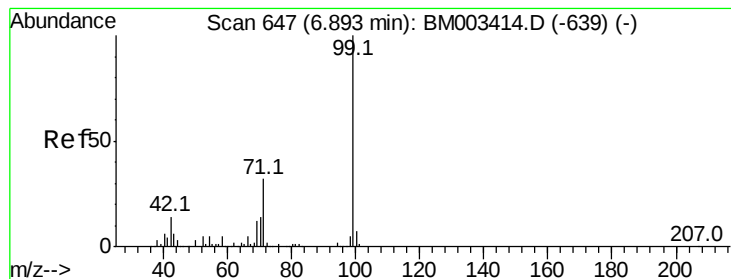

#7

Phenol-d6

Concen: 139.46 ng

RT: 7.00 min Scan# 666

Delta R.T. -0.02 min

Lab File: BM009500.D

Acq: 03 Apr 2017 15:05

Instrument :

BNA_M

ClientSampled :

PB97981BL


Tot Ion: 99 Resp: 1289590

Ion Ratio Lower Upper

99 100

42 24.5 11.0 16.4#




71 44.0 23.4 35.2#

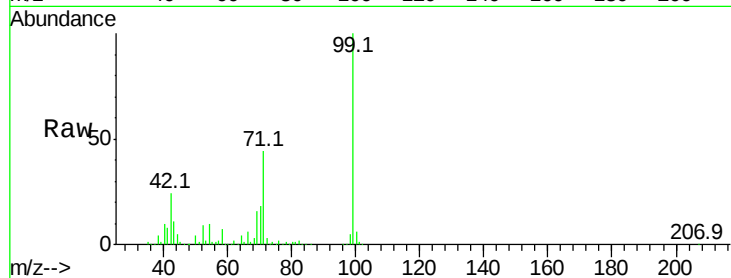

Abundance Ion 99.00 (98.70 to 99.70): BM003414.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM003414.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM003414.D (-639) (-)

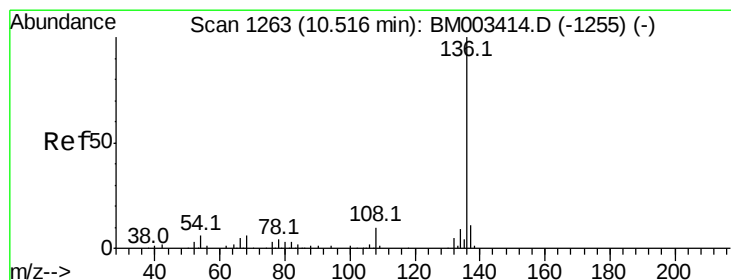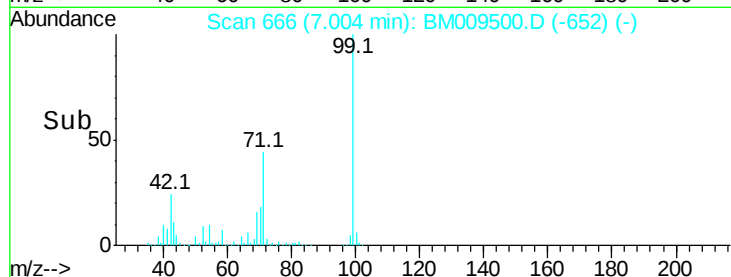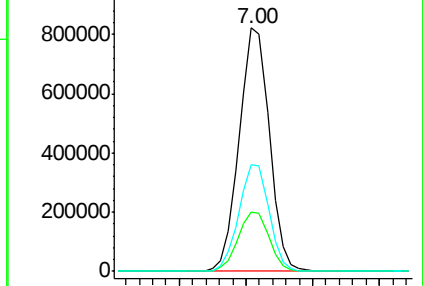

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.65 min Scan# 1285

Delta R.T. -0.02 min

Lab File: BM009500.D

Acq: 03 Apr 2017 15:05

Tgt Ion: 136 Resp: 416627


Ion Ratio Lower Upper

136 100

137 10.0 8.7 13.1

54 11.0 4.6 6.8#

68 6.9 3.7 5.5#


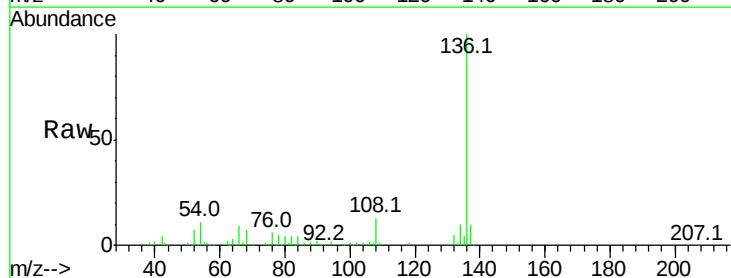



Abundance Ion 136.00 (135.70 to 136.70): BM003414.D (-1255) (-)

Ion 137.00 (136.70 to 137.70): BM003414.D (-1255) (-)

Ion 54.00 (53.70 to 54.70): BM003414.D (-1255) (-)

Ion 68.00 (67.70 to 68.70): BM003414.D (-1255) (-)



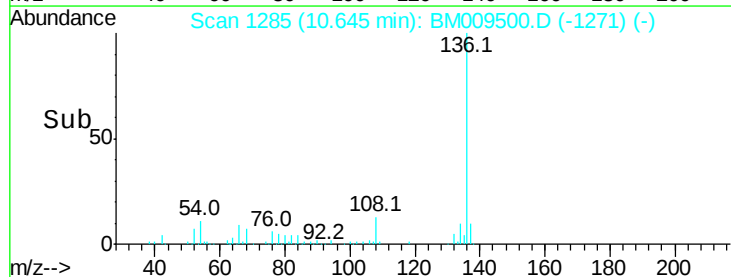
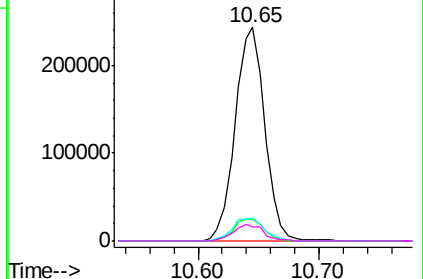


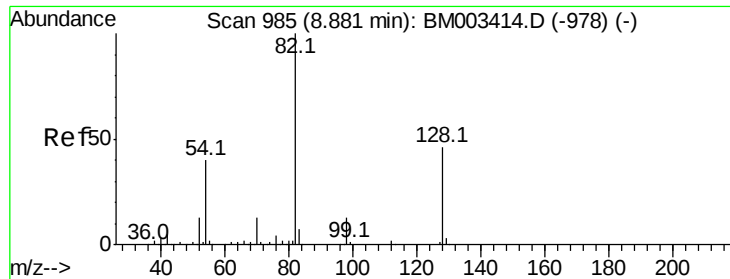

#23
Nitrobenzene-d5
Concen: 80.42 ng
RT: 9.01 min Scan# 1007
Delta R.T. -0.02 min
Lab File: BM009500.D
Acq: 03 Apr 2017 15:05




Instrument :
BNA_M
ClientSampleId :
PB97981BL


Tot Ion: 82 Resp: 893588
Ion Ratio Lower Upper
82 100
128 31.0 32.8 49.2#
54 55.1 40.6 60.8

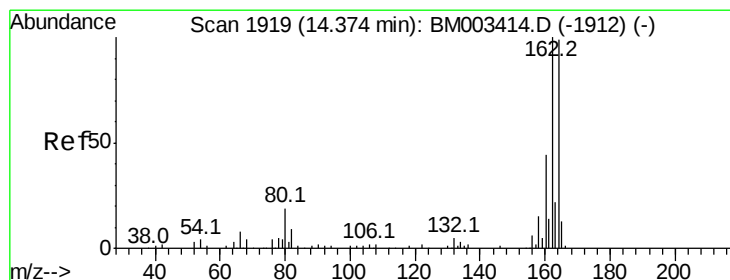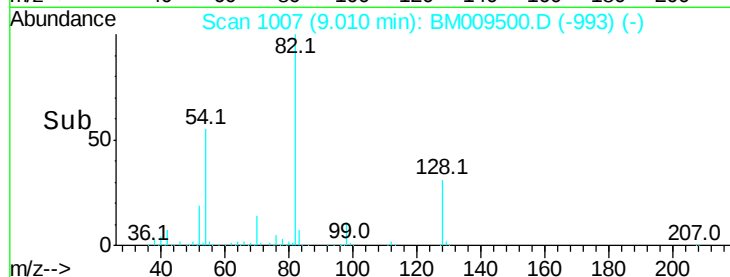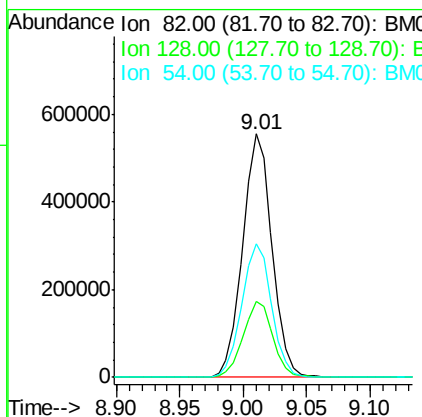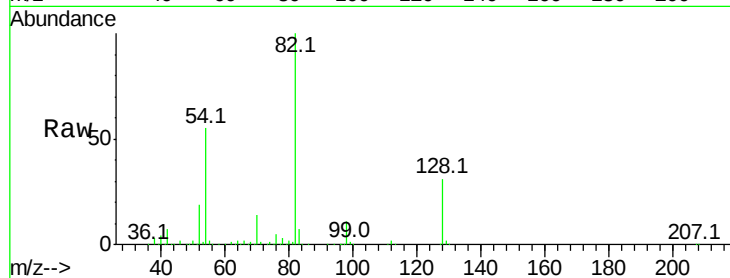

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.49 min Scan# 1938
Delta R.T. -0.02 min
Lab File: BM009500.D
Acq: 03 Apr 2017 15:05

Tgt Ion:164 Resp: 230504
Ion Ratio Lower Upper
164 100
162 96.9 82.4 123.6
160 42.5 35.8 53.6

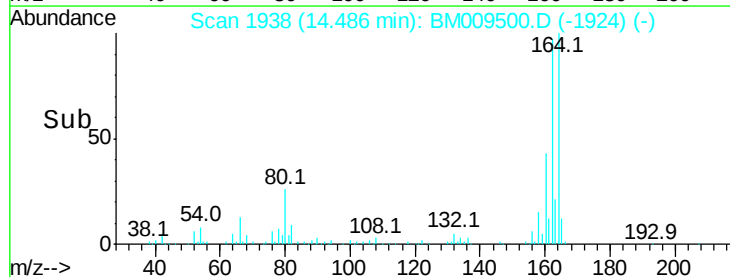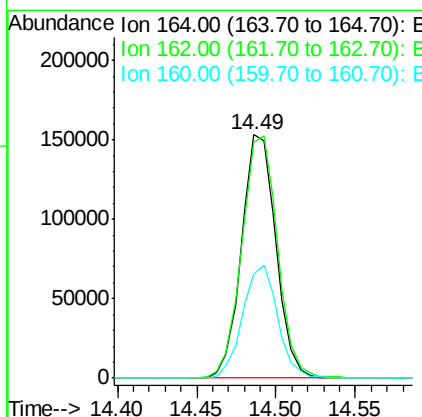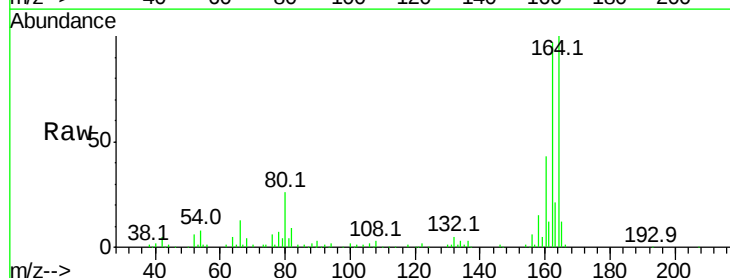


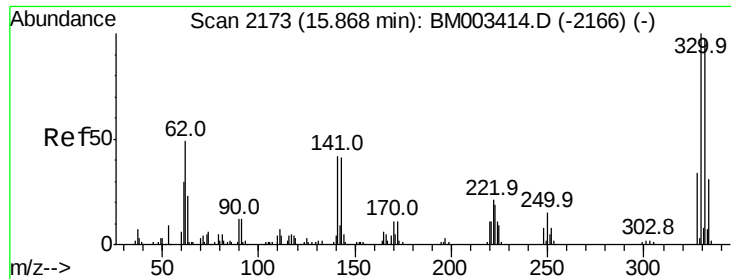




#41
 2,4,6-Tribromophenol
 Concen: 133.85 ng
 RT: 15.98 min Scan# 2192
 Delta R.T. -0.02 min
 Lab File: BM009500.D
 Acq: 03 Apr 2017 15:05

Instrument :
 BNA_M
 ClientSampleId :
 PB97981BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	0.0	0.0#
141	40.8	0.0	0.0#

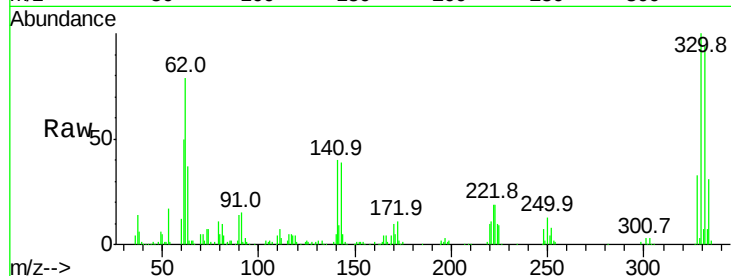


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

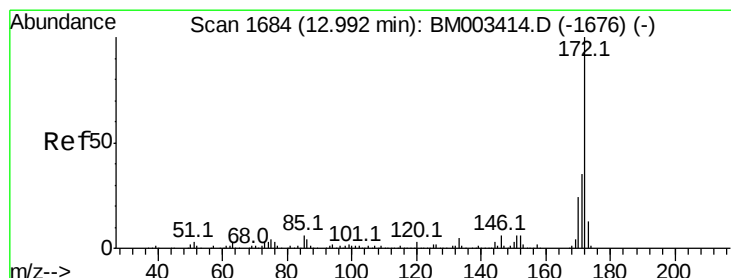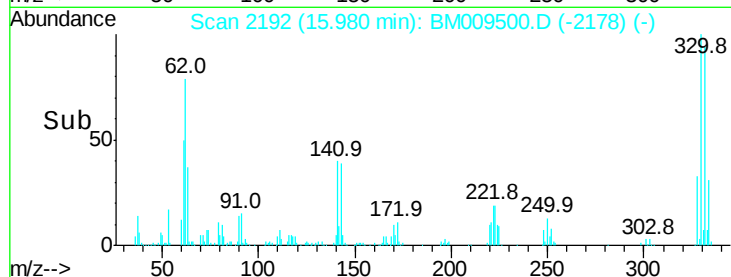
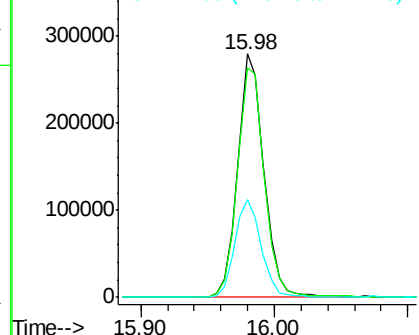



#44
 2-Fluorobiphenyl
 Concen: 83.26 ng
 RT: 13.10 min Scan# 1703
 Delta R.T. -0.02 min
 Lab File: BM009500.D
 Acq: 03 Apr 2017 15:05

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.0	28.5	42.7
170	22.7	18.8	28.2

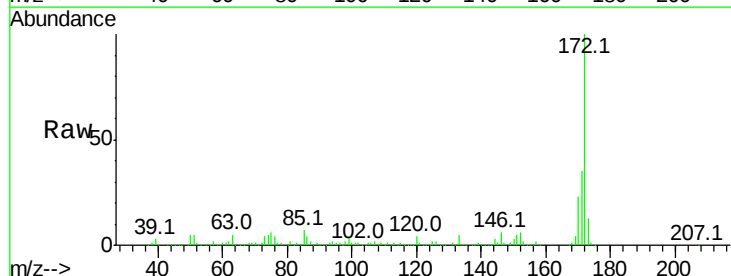

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



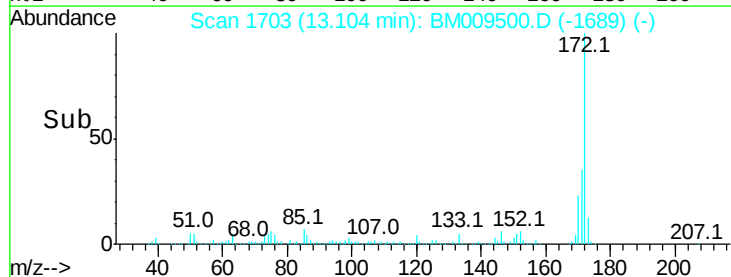
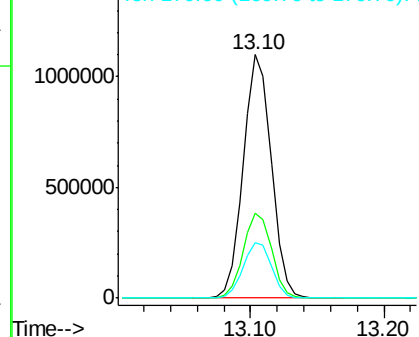


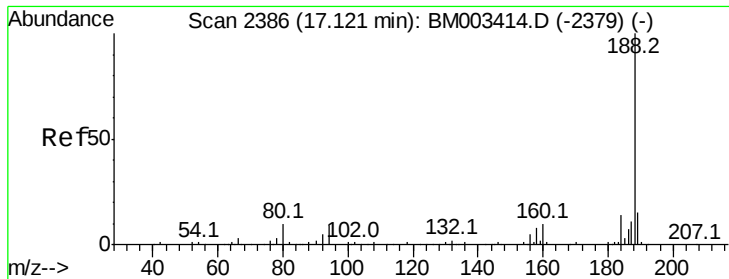

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.24 min Scan# 2406
Delta R.T. -0.01 min
Lab File: BM009500.D
Acq: 03 Apr 2017 15:05




Instrument :
BNA_M
ClientSampleId :
PB97981BL


Tot Ion:188 Resp: 556757
Ion Ratio Lower Upper
188 100
94 9.3 8.7 13.1
80 11.5 9.3 13.9

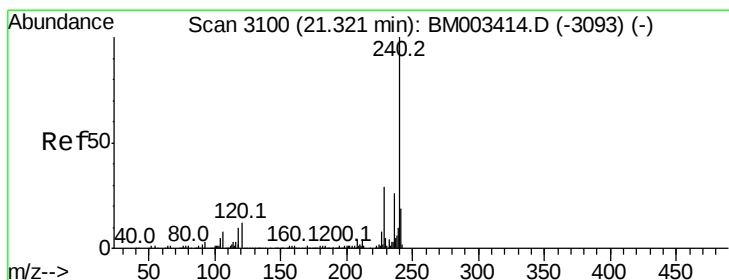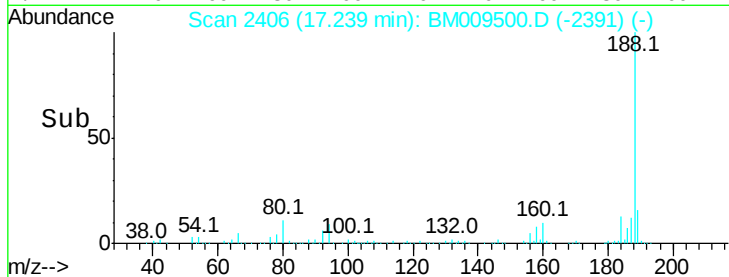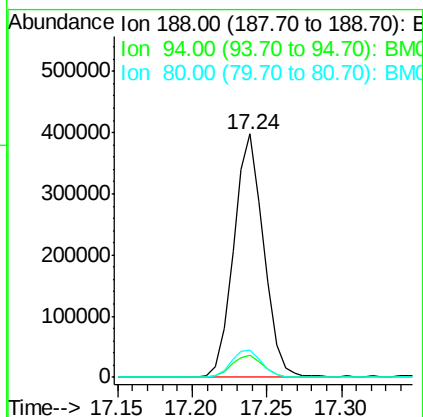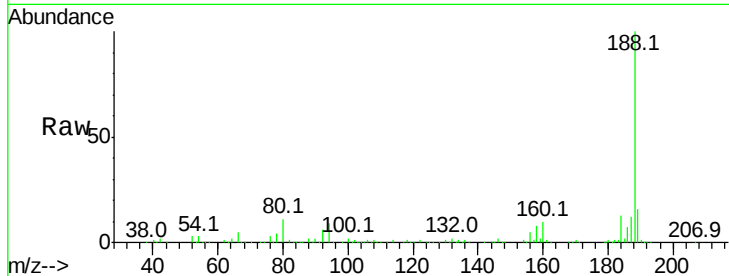

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.42 min Scan# 3116
Delta R.T. -0.01 min
Lab File: BM009500.D
Acq: 03 Apr 2017 15:05

Tgt Ion:240 Resp: 769678
Ion Ratio Lower Upper
240 100
120 7.8 8.2 12.2#
236 24.3 20.0 30.0

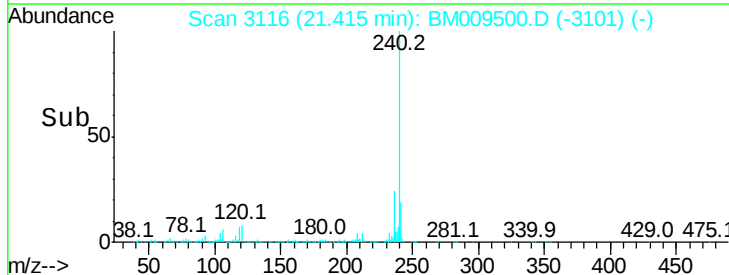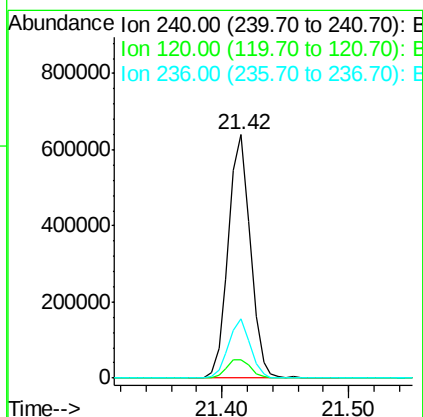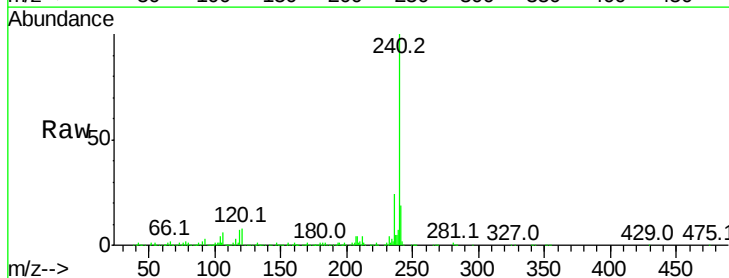

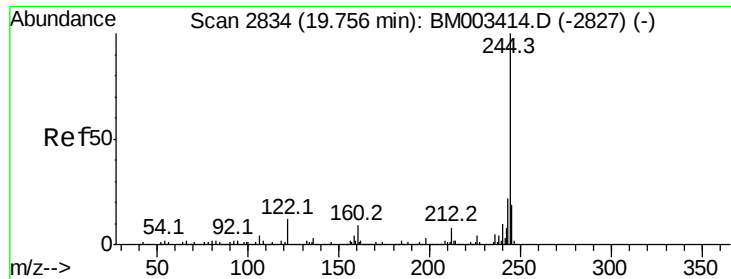

#78

Terphenyl-d14

Concen: 71.15 ng

RT: 19.86 min Scan# 2851

Delta R.T. -0.01 min

Lab File: BM009500.D

Acq: 03 Apr 2017 15:05

Instrument :

BNA_M

ClientSampleId :

PB97981BL


Tot Ion:244 Resp: 2620692

Ion Ratio Lower Upper

244 100

212 7.3 4.9 7.3

122 8.8 6.2 9.4

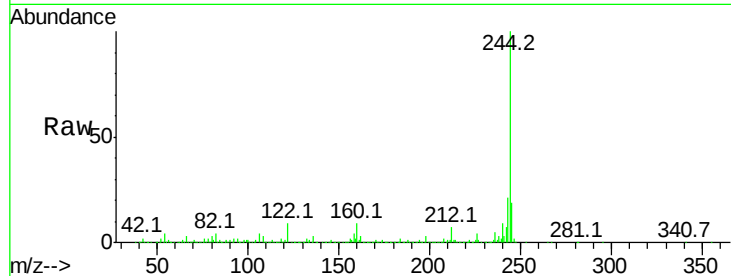

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

19.86

2500000

2000000



1500000

1000000

500000

0

Time-->

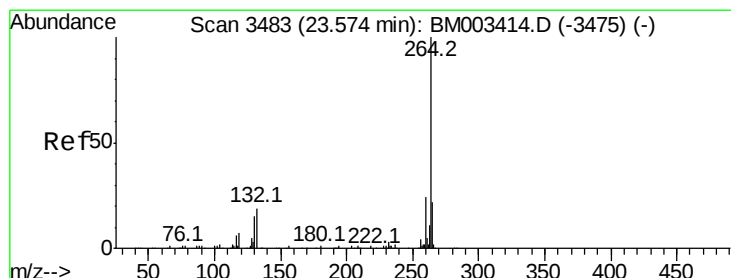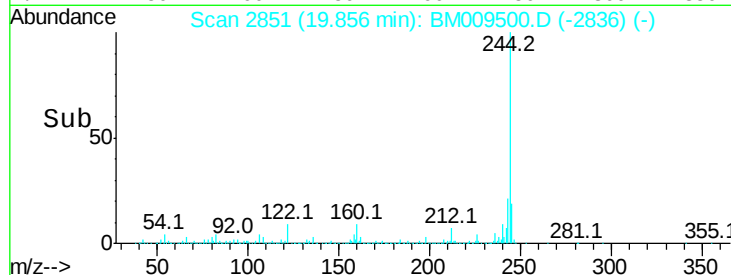

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.74 min Scan# 3511

Delta R.T. -0.02 min

Lab File: BM009500.D

Acq: 03 Apr 2017 15:05


Tgt Ion:264 Resp: 730102

Ion Ratio Lower Upper

264 100

260 24.0 18.6 27.8

265 20.9 17.3 25.9

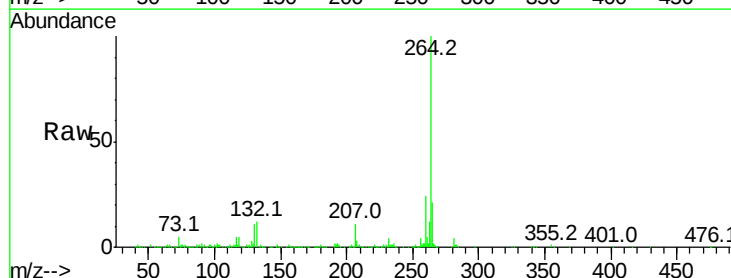

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

23.74

500000

400000

300000

200000

100000

0

Time-->

