


Data Path : Z:\HPCHEM1\BNA M\DATA\BM040317\
 Data File : BM009494.D
 Acq On : 03 Apr 2017 11:19
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 31 14:38:29 2017

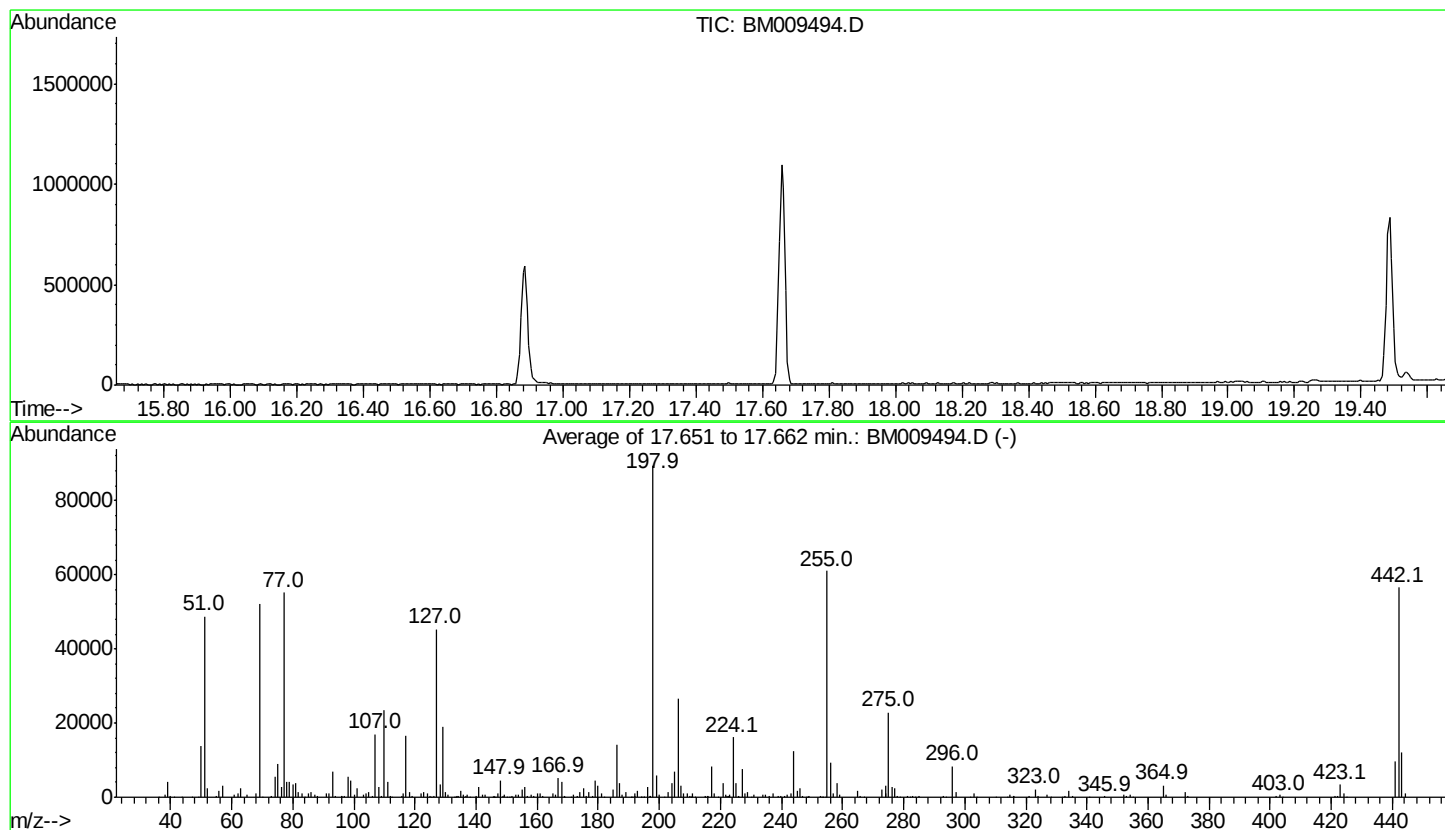

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.6	48829	PASS
68	69	0.00	2	2.0	1028	PASS
69	198	0.00	100	58.4	52245	PASS
70	69	0.00	2	0.2	106	PASS
127	198	10	80	50.6	45256	PASS
197	198	0.00	2	0.5	425	PASS
198	198	100	100	100.0	89400	PASS
199	198	5	9	6.8	6044	PASS
275	198	10	60	25.6	22898	PASS
365	198	1	100	3.6	3193	PASS
441	442	0.01	24	16.8	9505	PASS
442	198	50	100	63.2	56533	PASS
443	442	15	24	21.1	11939	PASS