

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040323\
 Data File : BM039277.D
 Acq On : 03 Apr 2023 13:50
 Operator : CG/JU
 Sample : PB151823BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM039277.D\data.ms




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.004	286	292	301	rBV	1649068	2211194	19.12%	3.721%
2	5.475	365	372	383	rBV	3936516	5493202	47.49%	9.245%
3	7.086	638	646	659	rBV	3378371	5377563	46.49%	9.050%
4	7.916	780	787	794	rBV	1037973	1600249	13.84%	2.693%
5	9.086	978	986	1004	rBV	3144860	5141523	44.45%	8.653%
6	10.727	1256	1265	1279	rBV	1296631	2220173	19.20%	3.736%
7	13.186	1676	1683	1700	rBV	7194998	10305737	89.10%	17.344%
8	14.562	1911	1917	1925	rBV	1819060	2642142	22.84%	4.447%
9	16.051	2164	2170	2188	rBV	2946609	4449958	38.47%	7.489%
10	17.309	2378	2384	2394	rBV	1941939	2825950	24.43%	4.756%
11	18.203	2532	2536	2544	rBV	88819	172429	1.49%	0.290%
12	19.933	2825	2830	2844	rBV	8894387	11565993	100.00%	19.465%
13	21.497	3091	3096	3105	rBV	2023621	2766569	23.92%	4.656%
14	23.909	3500	3506	3518	rVB2	1303007	2646500	22.88%	4.454%

Sum of corrected areas: 59419182

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040323\
Data File : BM039277.D
Acq On : 03 Apr 2023 13:50
Operator : CG/JU
Sample : PB151823BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

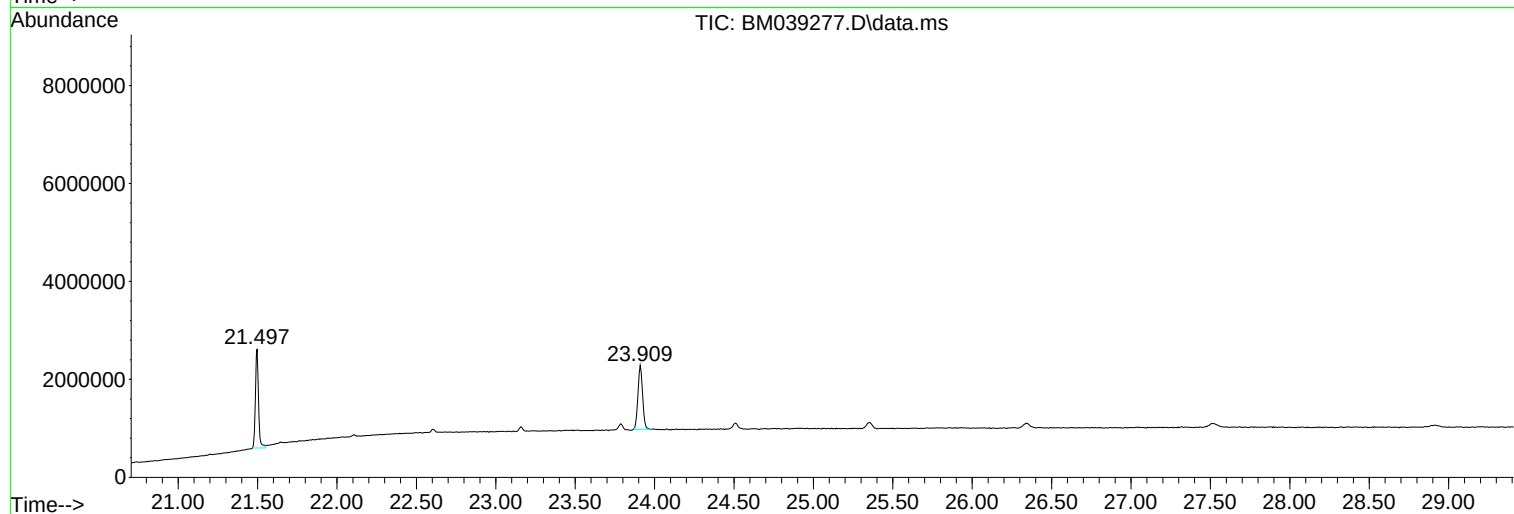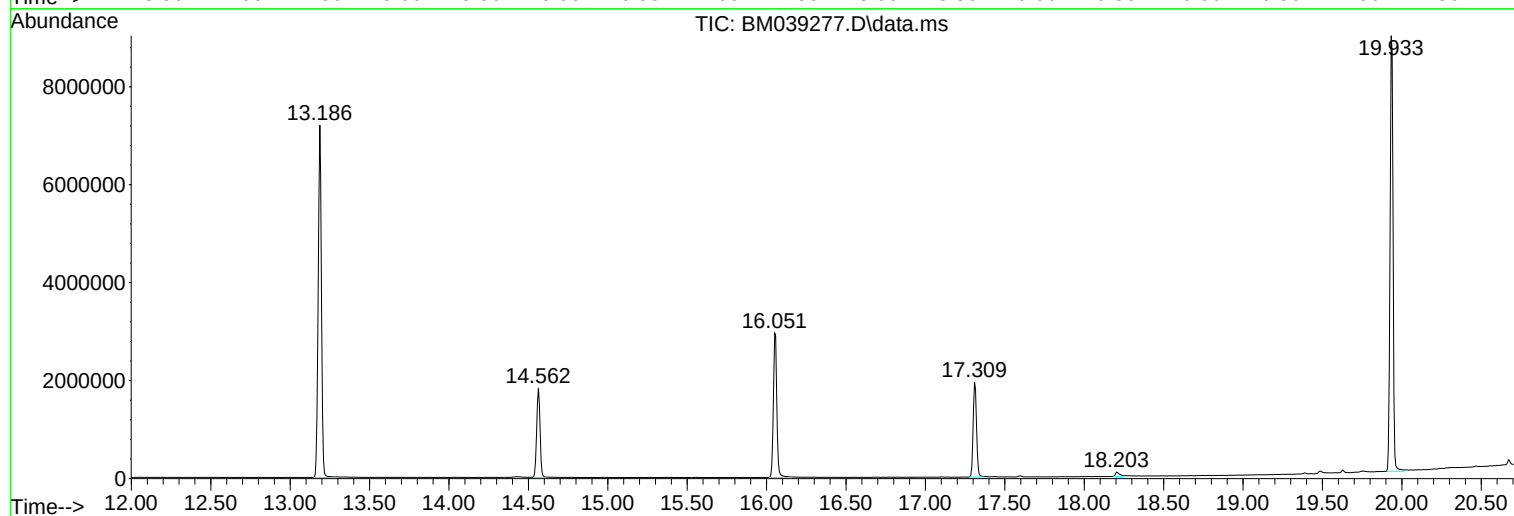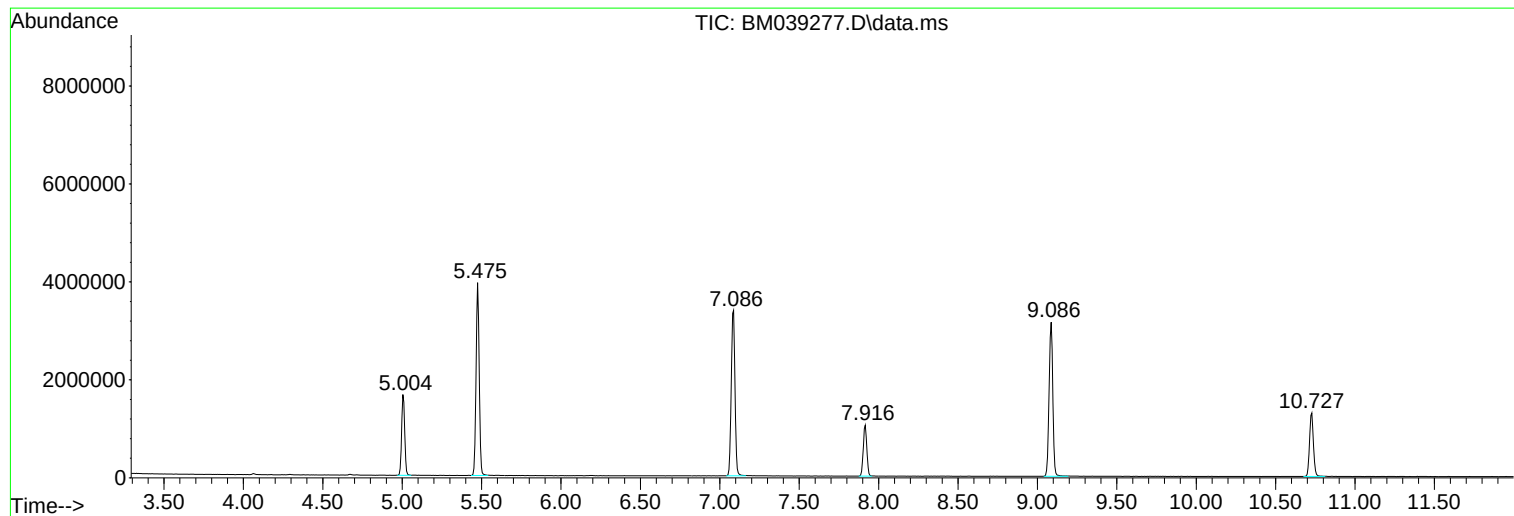

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040323\
Data File : BM039277.D
Acq On : 03 Apr 2023 13:50
Operator : CG/JU
Sample : PB151823BL
Misc :
ALS Vial : 6 Sample Multiplier: 1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.004	27.64 ng	2211190	1,4-Dichlorobenzene-d4	7.916

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
4	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

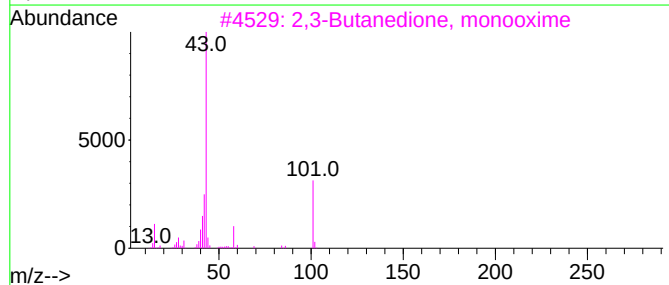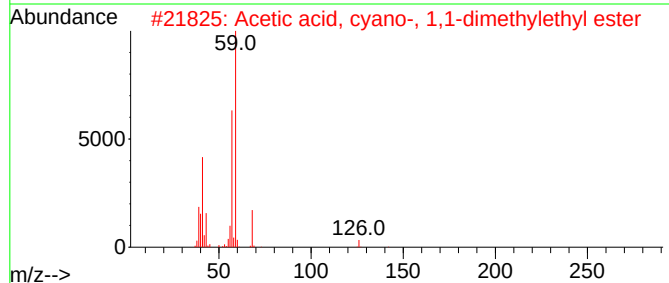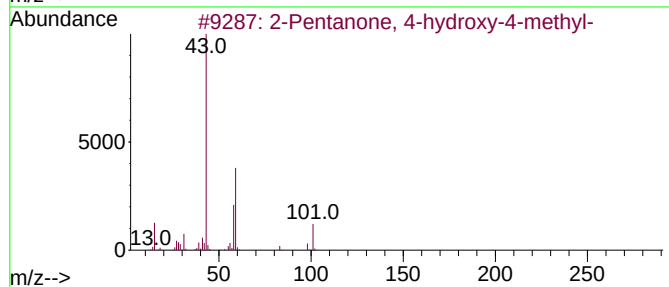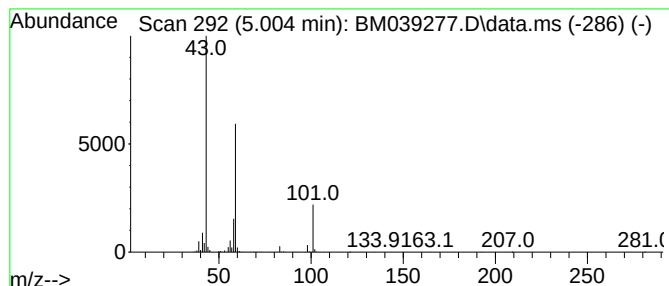

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040323\
Data File : BM039277.D
Acq On : 03 Apr 2023 13:50
Operator : CG/JU
Sample : PB151823BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.004	27.6	ng	2211190	1	7.916	1600250	20.0