
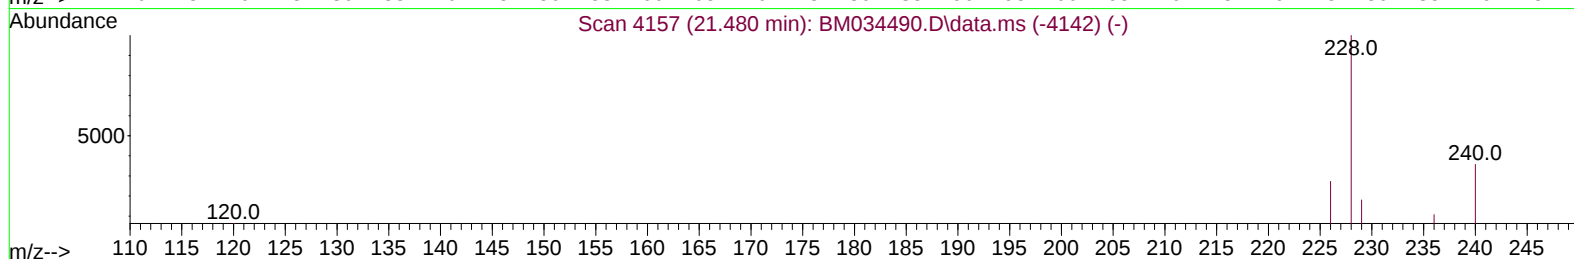
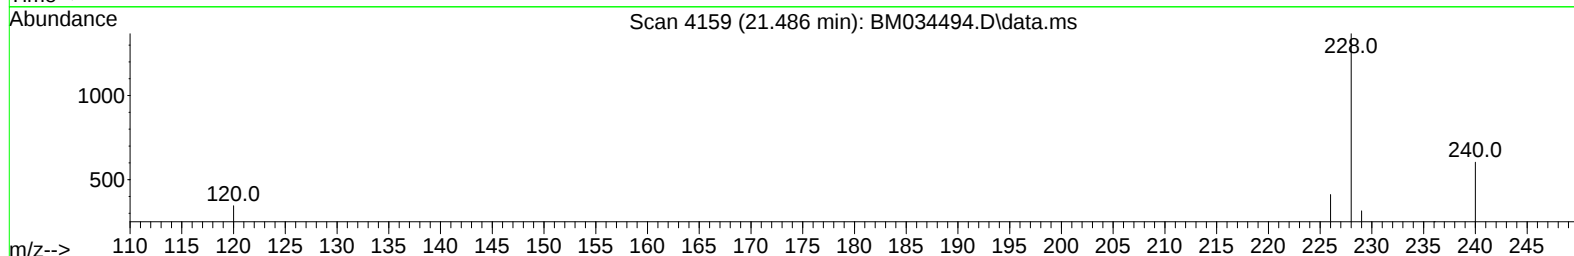


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040422\
Data File : BM034494.D
Acq On : 04 Apr 2022 19:23
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Apr 05 12:12:00 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 11:50:53 2022
Response via : Initial Calibration

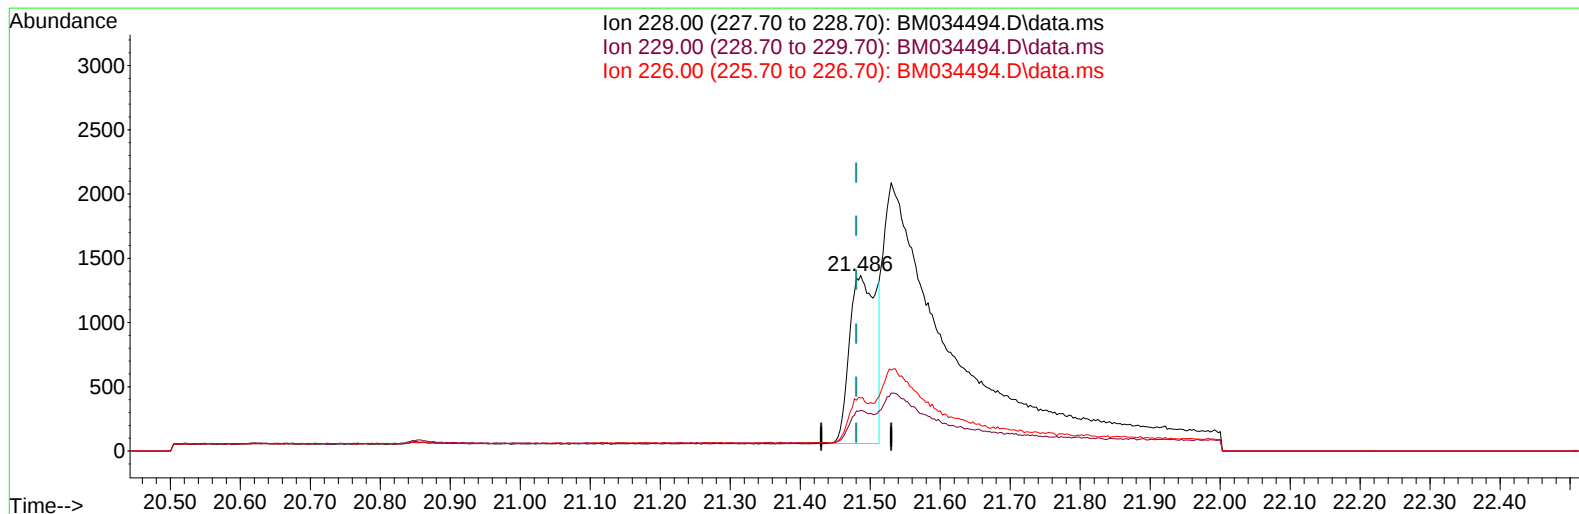

TIC: BM034494.D\data.ms

(21) Benzo(a)anthracene

21.486min (+ 0.006) 0.43 ng/u1

response 3447

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	21.60	23.04
226.00	29.00	30.14
0.00	0.00	0.00