
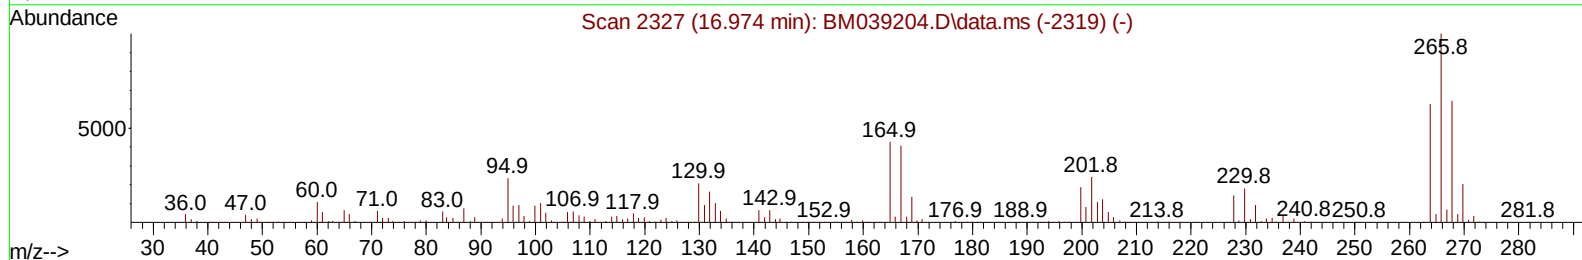
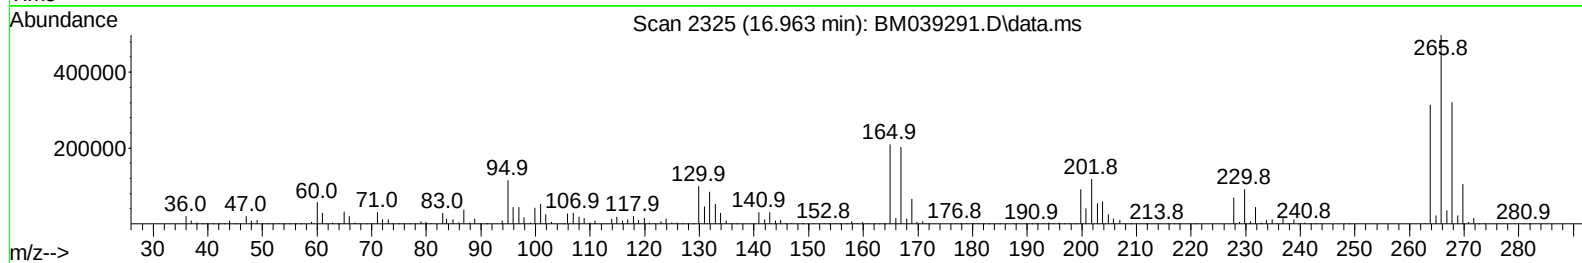


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040423\
Data File : BM039291.D
Acq On : 04 Apr 2023 09:59
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 17:43:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 17:03:41 2023
Response via : Initial Calibration

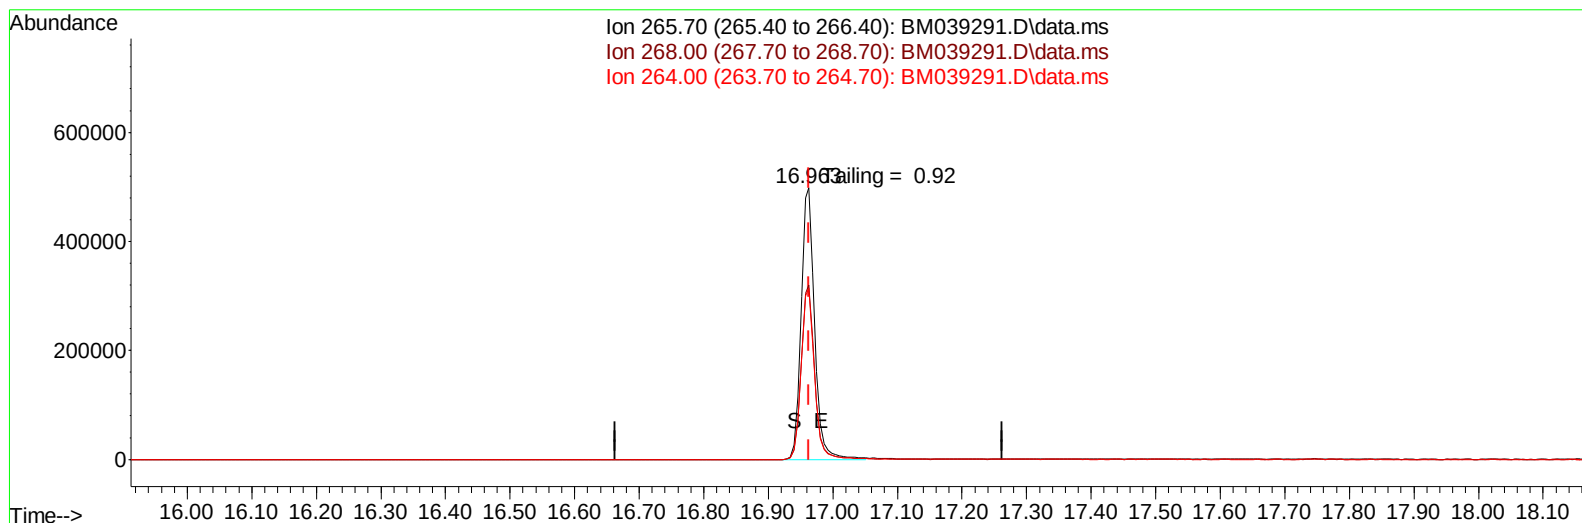




TIC: BM039291.D\data.ms

(70) Pentachlorophenol (C)**16.963min (+ 0.000) 612427.34 ng****response 747926**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.31
264.00	62.80	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040423\
Data File : BM039291.D
Acq On : 04 Apr 2023 09:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 17:43:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 17:03:41 2023
Response via : Initial Calibration

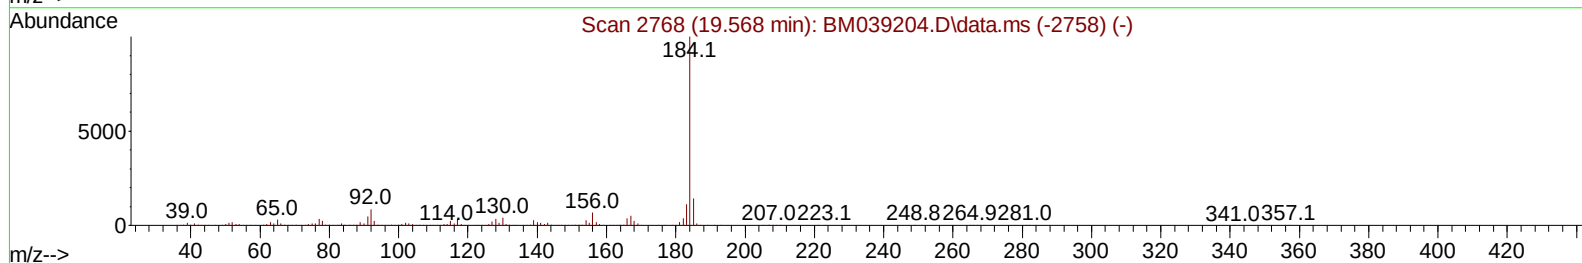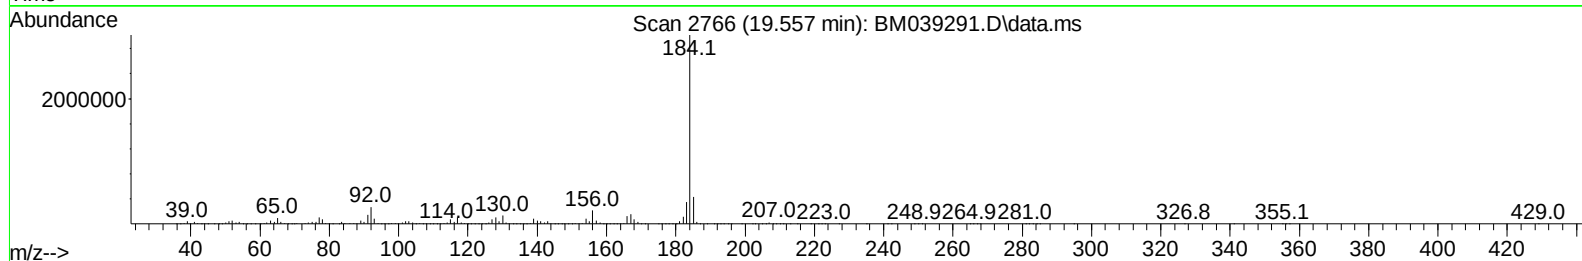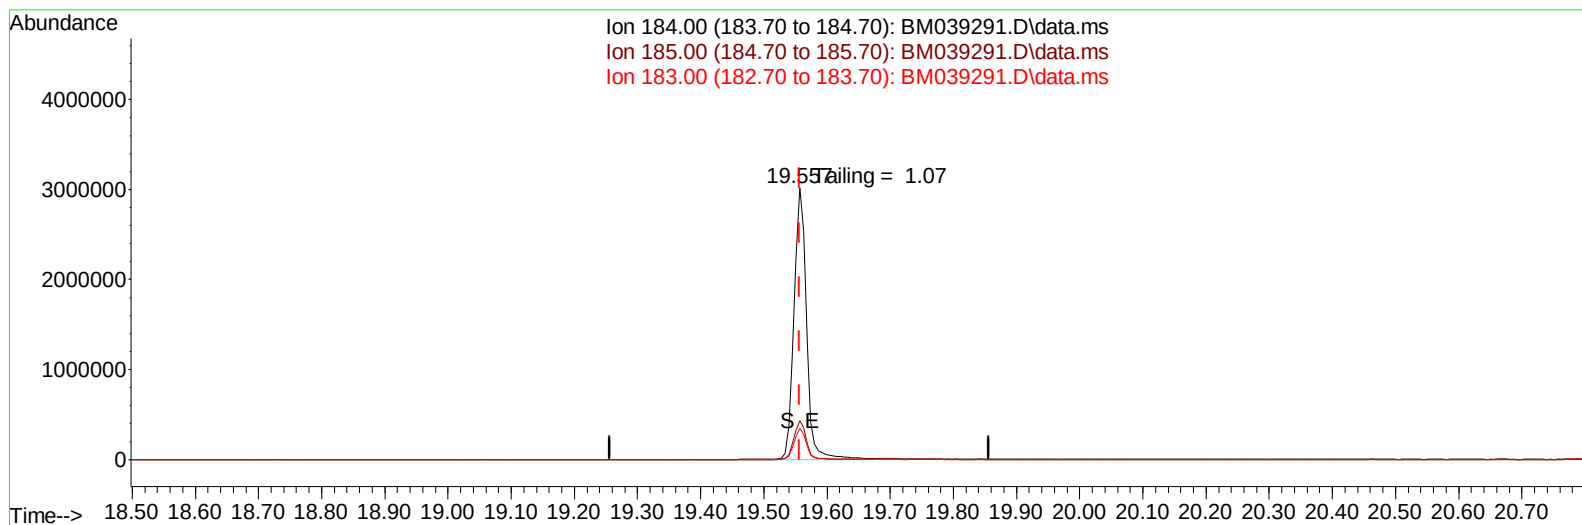

TIC: BM039291.D\data.ms

(77) Benzidine**19.557min (+ 0.000) 49425.08 ng****response 4192559**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.25
183.00	11.20	11.41
0.00	0.00	0.00