

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040423\
 Data File : BM039293.D
 Acq On : 04 Apr 2023 11:13
 Operator : CG/JU
 Sample : PB151768BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB151768BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM039293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.010	287	293	305	rVB	3191785	4352416	28.15%	4.848%
2	5.475	366	372	387	rBV	7413585	10930416	70.68%	12.176%
3	7.087	638	646	665	rBV	6834829	10834723	70.06%	12.069%
4	7.910	779	786	795	rBV	1318978	2050060	13.26%	2.284%
5	9.086	977	986	1000	rBV	4183810	6905013	44.65%	7.692%
6	10.722	1256	1264	1277	rBV	1628371	2751640	17.79%	3.065%
7	13.186	1675	1683	1702	rBV	9638574	13935760	90.12%	15.523%
8	14.557	1909	1916	1928	rBV	2264066	3304564	21.37%	3.681%
9	16.051	2163	2170	2185	rBV	6342258	9388015	60.71%	10.457%
10	17.309	2377	2384	2397	rBV	2419001	3563713	23.05%	3.970%
11	18.203	2531	2536	2545	rBV	132490	277225	1.79%	0.309%
12	19.480	2749	2753	2764	rBV2	98119	230177	1.49%	0.256%
13	19.933	2824	2830	2845	rBV	12335888	15463819	100.00%	17.225%
14	21.492	3090	3095	3106	rBV	2350103	3127779	20.23%	3.484%
15	23.903	3499	3505	3516	rVB2	1294578	2658142	17.19%	2.961%




Sum of corrected areas: 89773462

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040423\
Data File : BM039293.D
Acq On : 04 Apr 2023 11:13
Operator : CG/JU
Sample : PB151768BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151768BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

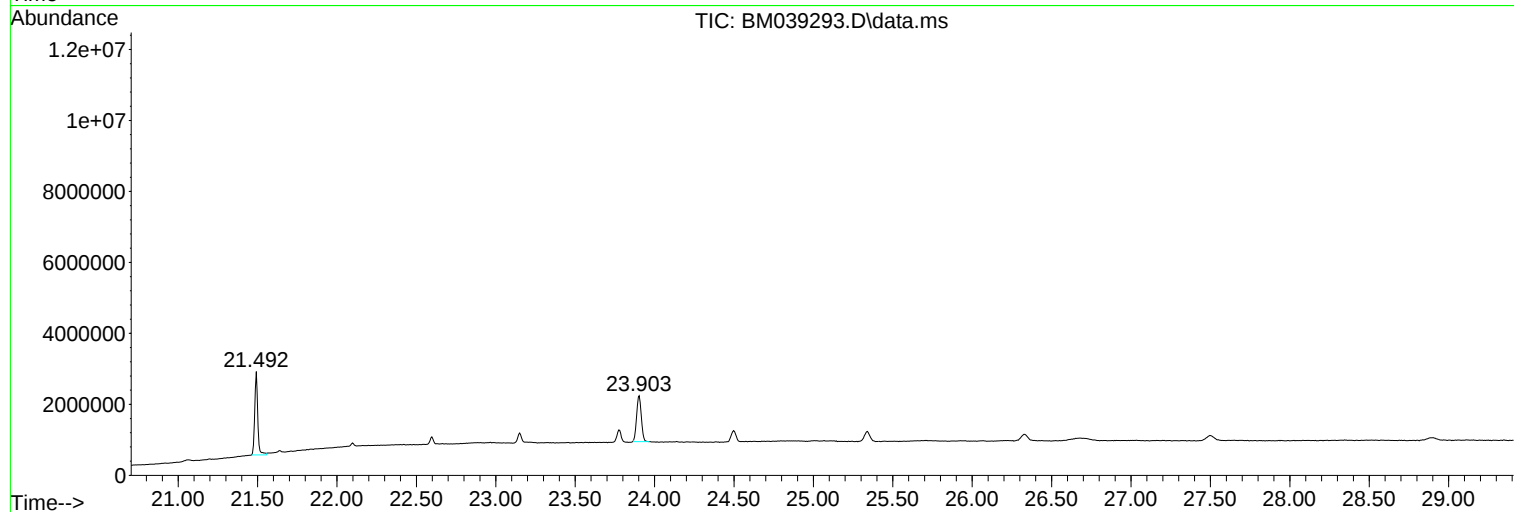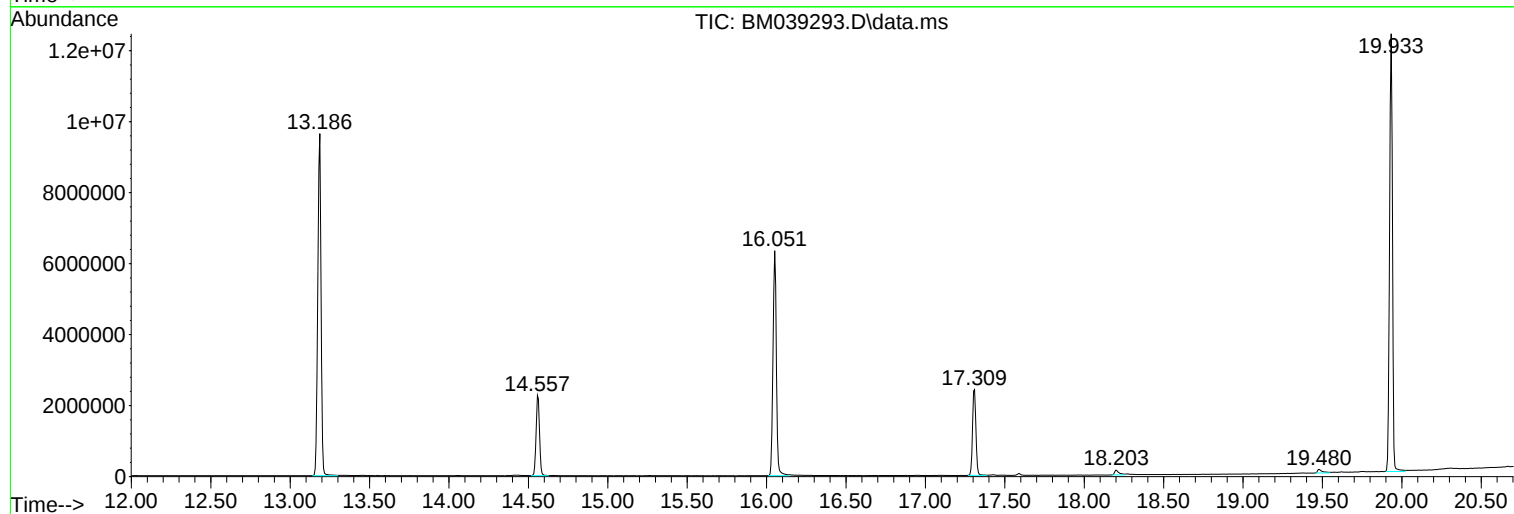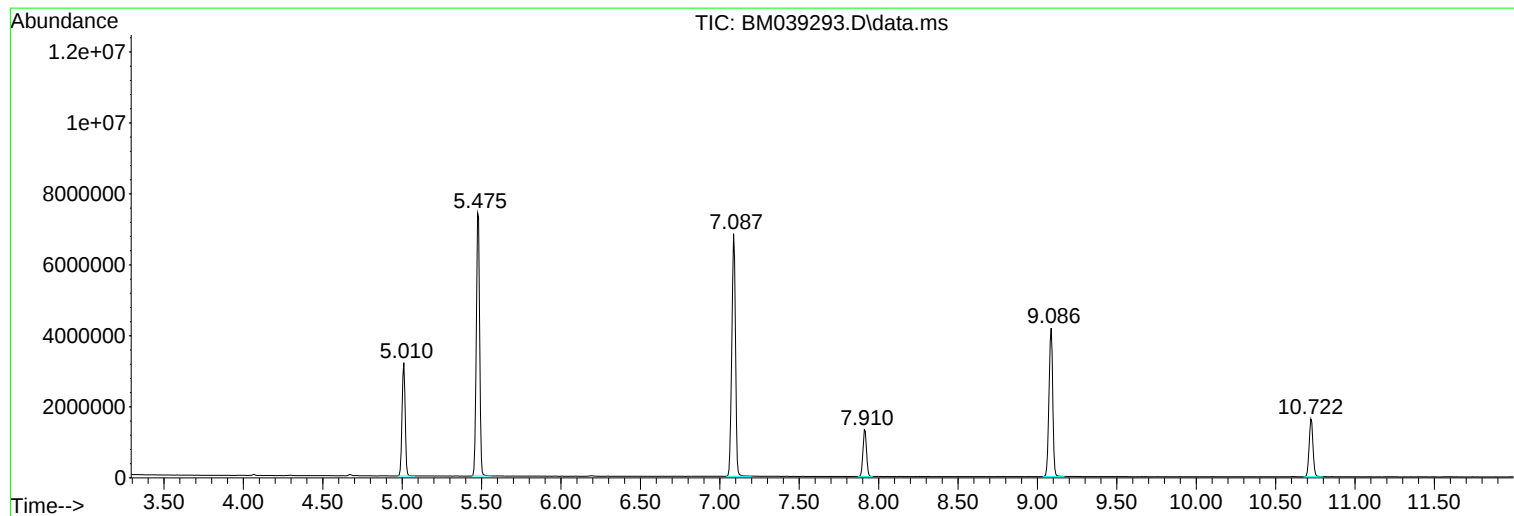

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040423\
Data File : BM039293.D
Acq On : 04 Apr 2023 11:13
Operator : CG/JU
Sample : PB151768BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151768BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.010	42.46 ng	4352420	1,4-Dichlorobenzene-d4	7.916

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	53		
3	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
5	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		

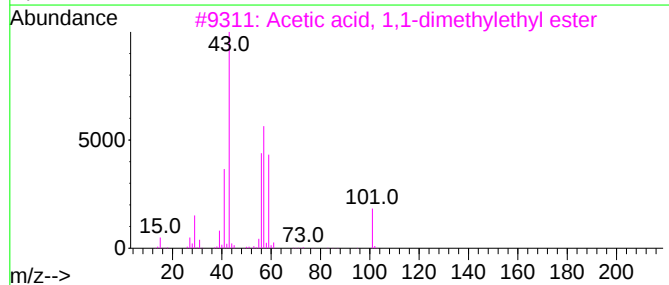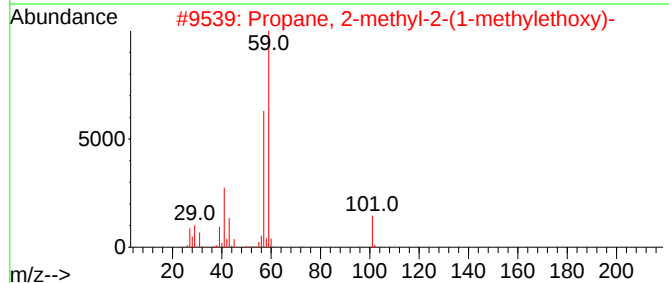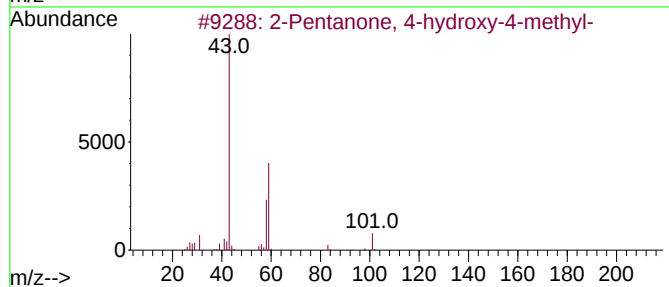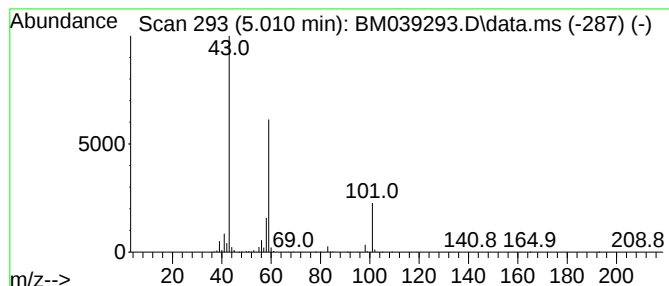

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040423\
Data File : BM039293.D
Acq On : 04 Apr 2023 11:13
Operator : CG/JU
Sample : PB151768BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151768BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.010	42.5	ng	4352420	1	7.916	2050060	20.0