


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040423\
Data File : BM039291.D
Acq On : 04 Apr 2023 09:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 31 17:03:41 2023

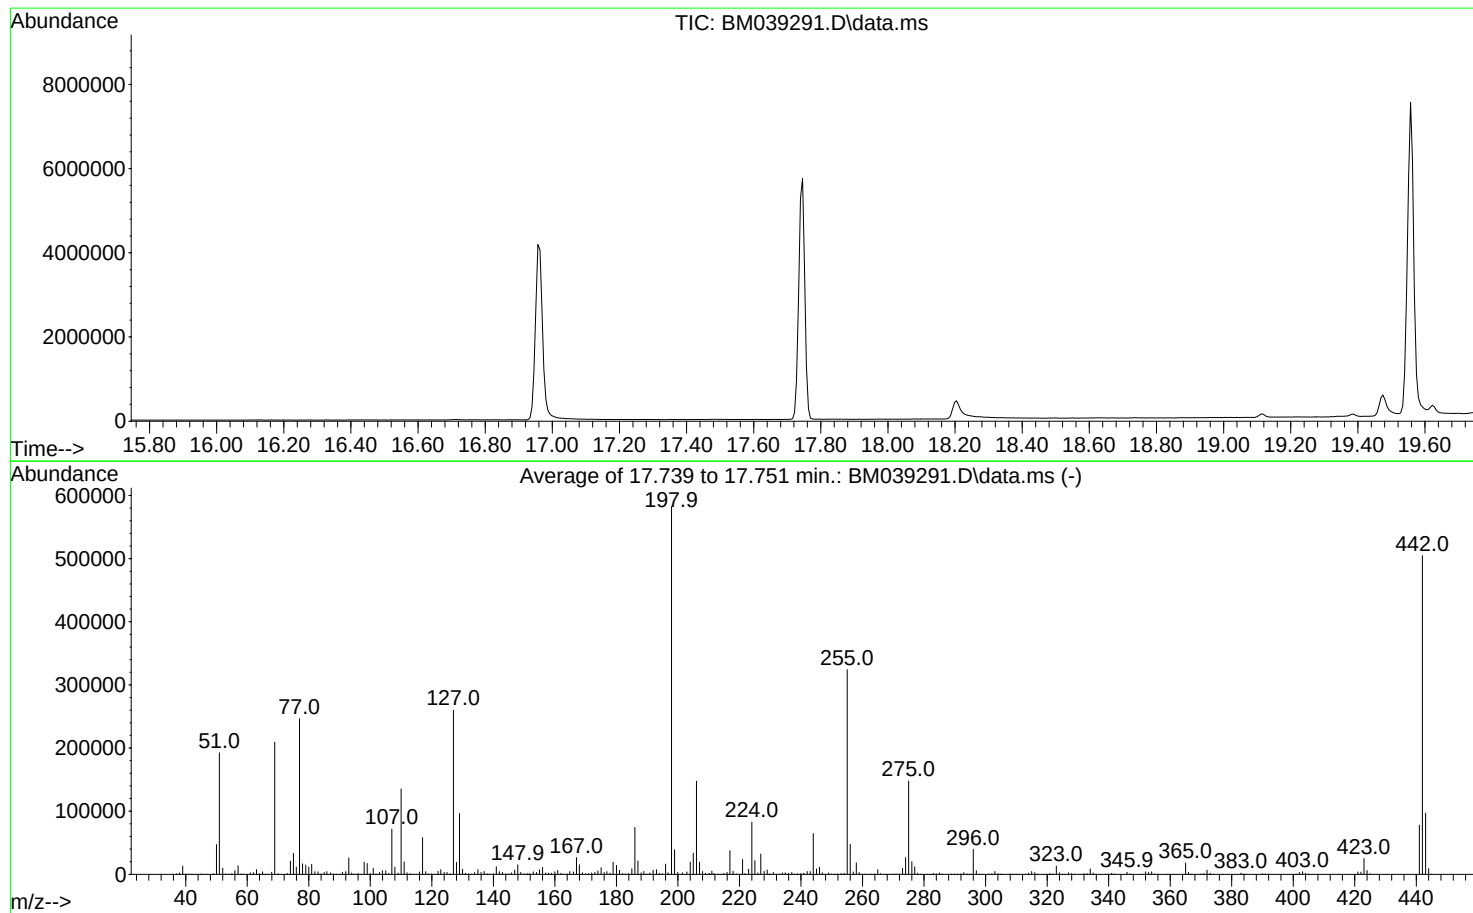




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	192570	PASS
68	69	0.00	2	1.5	3137	PASS
69	198	0.00	100	35.9	209214	PASS
70	69	0.00	2	0.4	933	PASS
127	198	10	80	44.6	259861	PASS
197	198	0.00	2	0.4	2518	PASS
198	198	100	100	100.0	582677	PASS
199	198	5	9	6.7	38877	PASS
275	198	10	60	25.3	147693	PASS
365	198	1	100	3.1	17862	PASS
441	198	0.01	100	13.4	77933	PASS
442	442	50	100	100.0	504832	PASS
443	442	15	24	19.2	96971	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040423\
Data File : BM039291.D
Acq On : 04 Apr 2023 09:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 04 17:43:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 17:03:41 2023
Response via : Initial Calibration

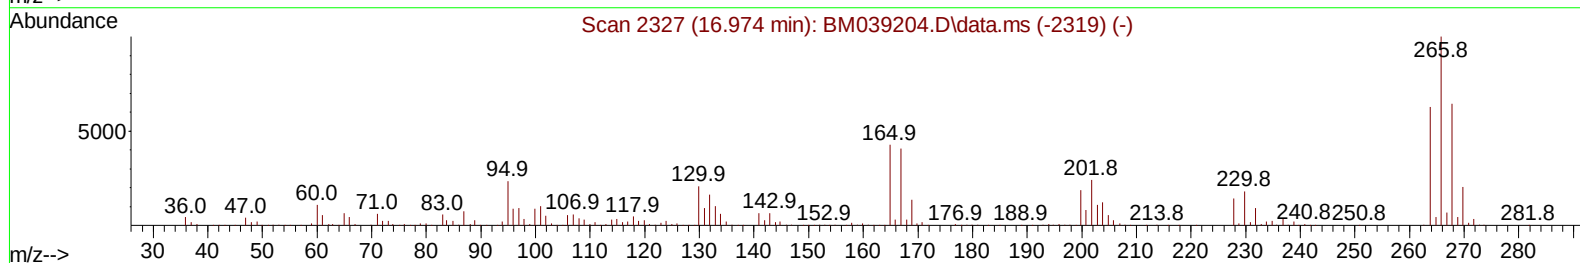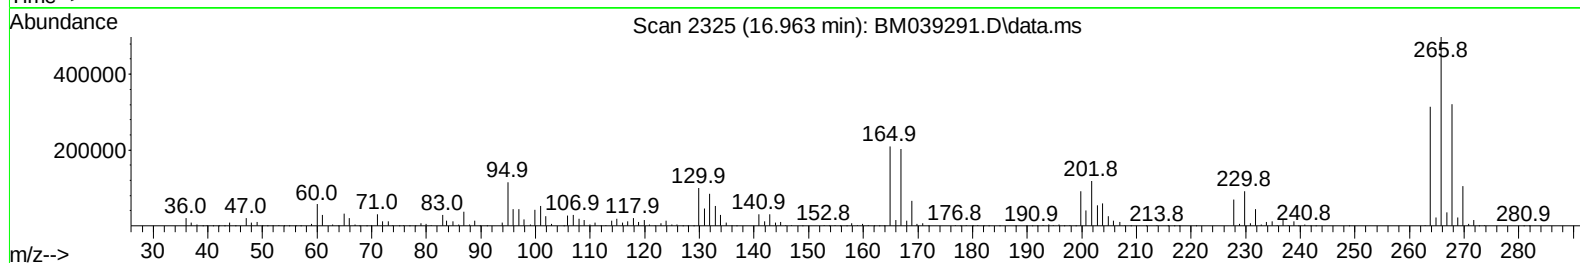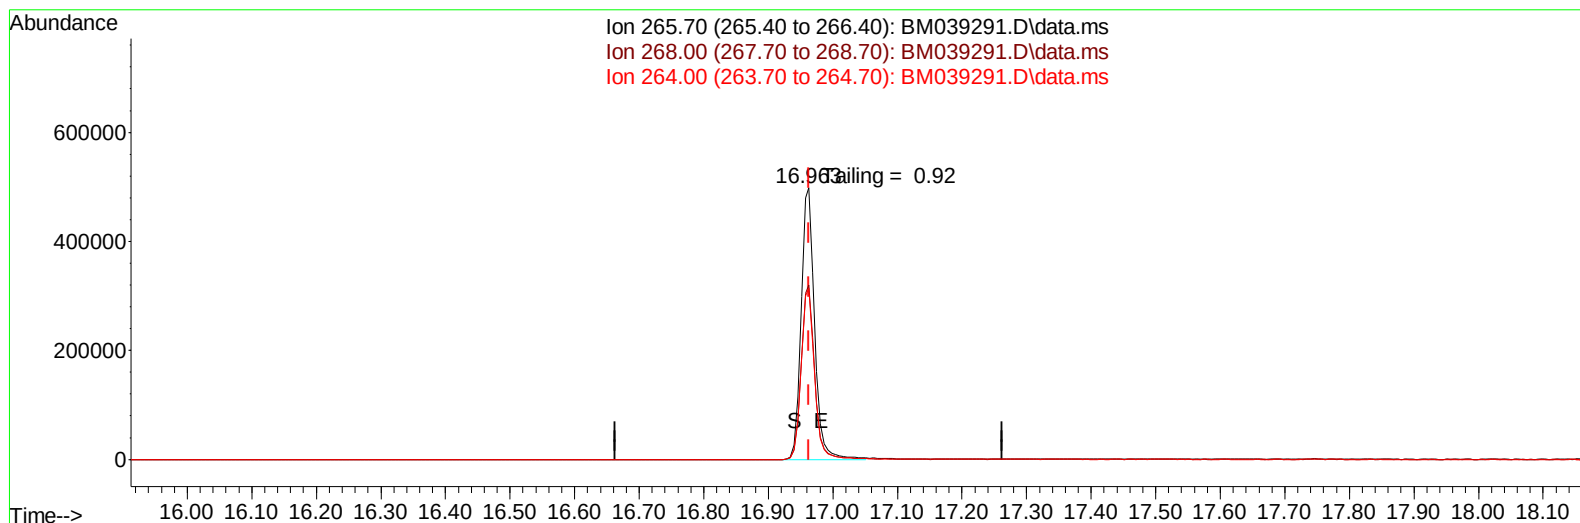

TIC: BM039291.D\data.ms

(70) Pentachlorophenol (C)

16.963min (+ 0.000) 612427.34 ng




response 747926

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.31
264.00	62.80	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040423\
Data File : BM039291.D
Acq On : 04 Apr 2023 09:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 04 17:43:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 17:03:41 2023
Response via : Initial Calibration

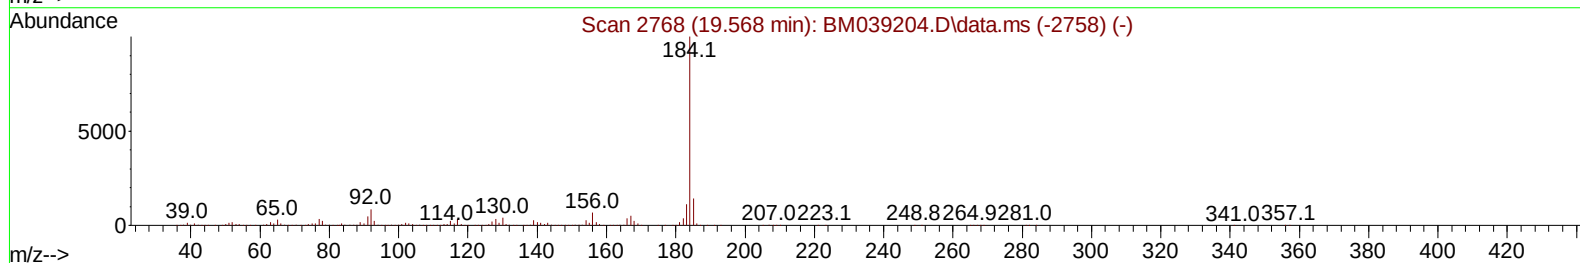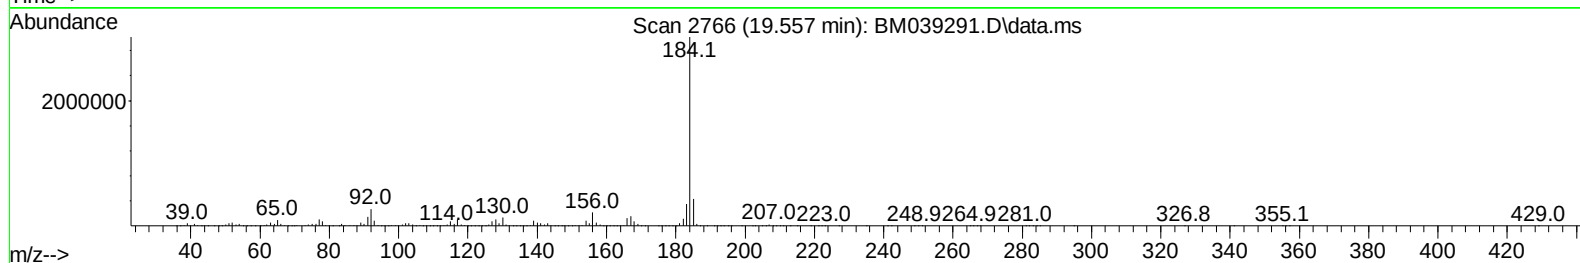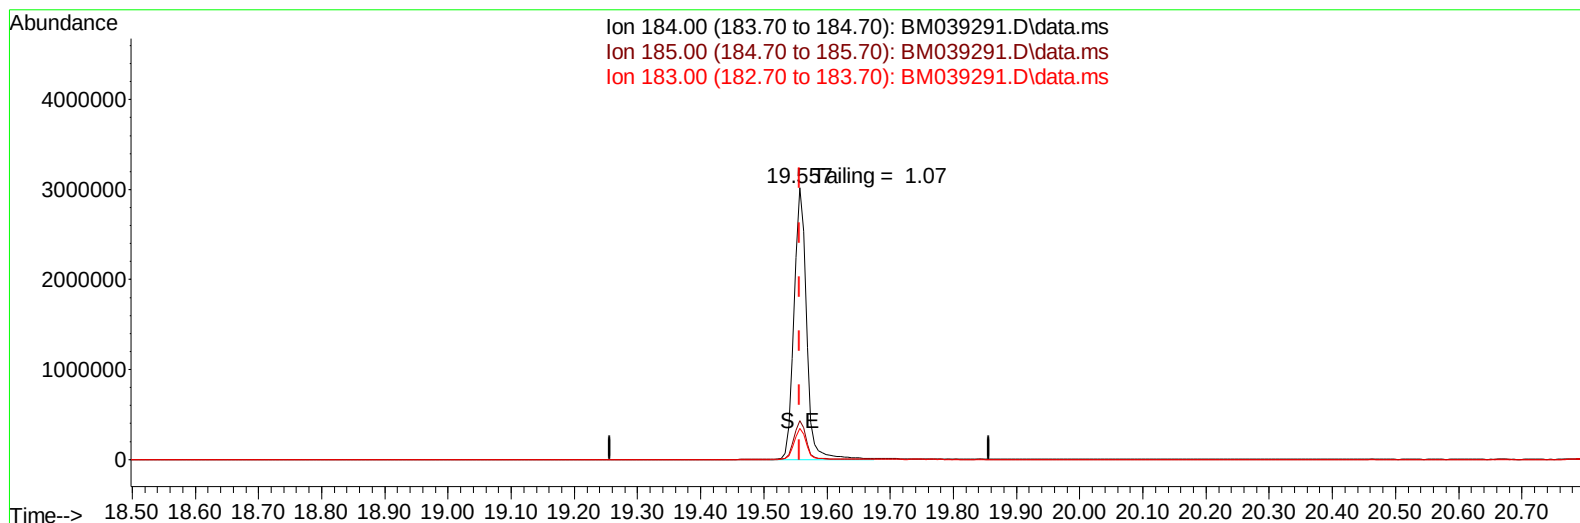

TIC: BM039291.D\data.ms

(77) Benzidine

19.557min (+ 0.000) 49425.08 ng

response 4192559

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.25
183.00	11.20	11.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/4/2023	BNA_M	<u>BM039291.D</u>
Compound Name	Response	Retention Time
DDT	2025683	20.786
DDD	42404	20.345
DDE	1959	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44363	2070046	2.14

Instrument :
BNA_M
ClientSampleId :
DFTPP