


Data Path : C:\Users\eUser\Desktop\Dhruv Practice\BF033125\
Data File : BF142174.D
Acq On : 31 Mar 2025 11:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

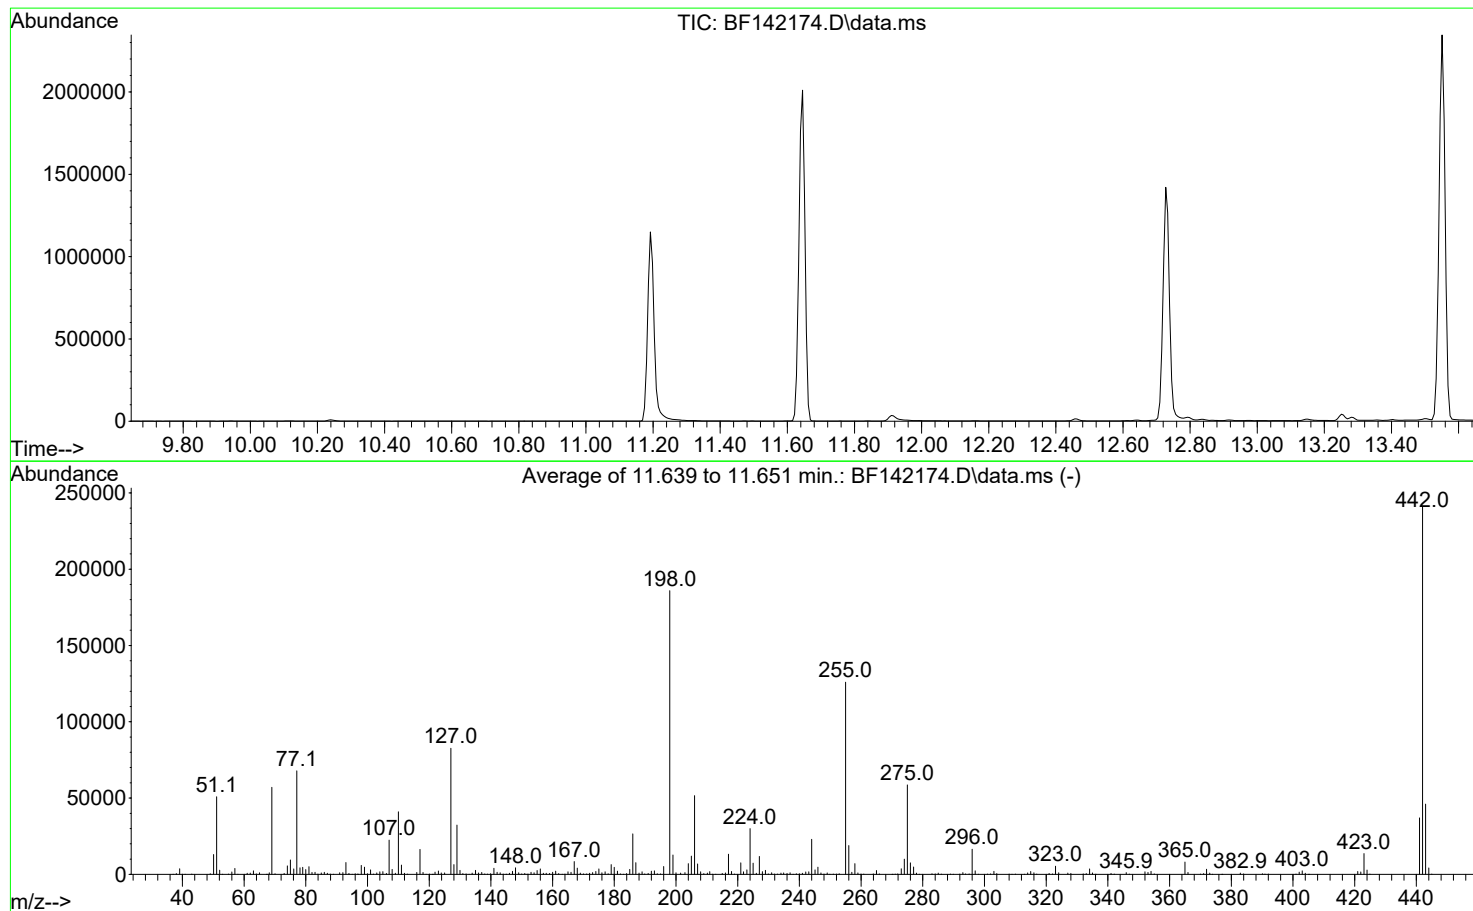

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	50853	PASS
68	69	0.00	2	1.8	1026	PASS
69	198	0.00	100	30.7	57003	PASS
70	69	0.00	2	0.7	402	PASS
127	198	10	80	44.4	82605	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	185877	PASS
199	198	5	9	6.8	12724	PASS
275	198	10	60	31.5	58629	PASS
365	198	1	100	4.3	8063	PASS
441	198	0.01	100	19.9	36995	PASS
442	442	50	100	100.0	241088	PASS
443	442	15	24	19.1	46021	PASS