
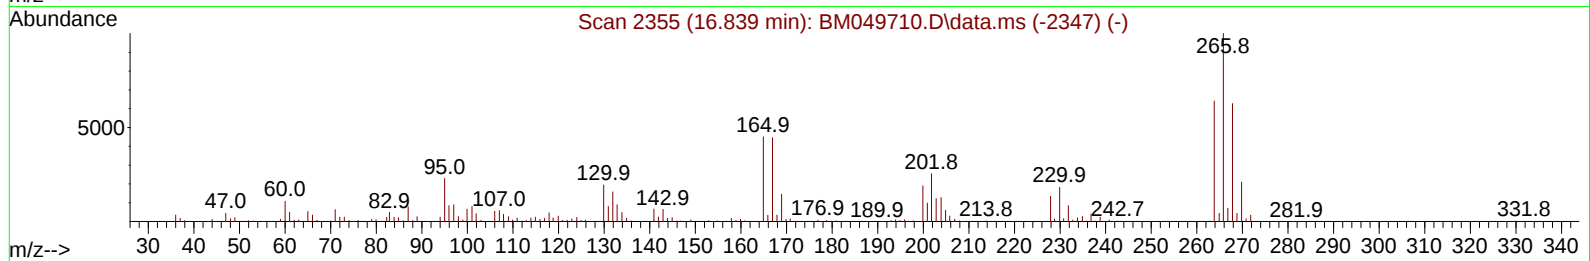
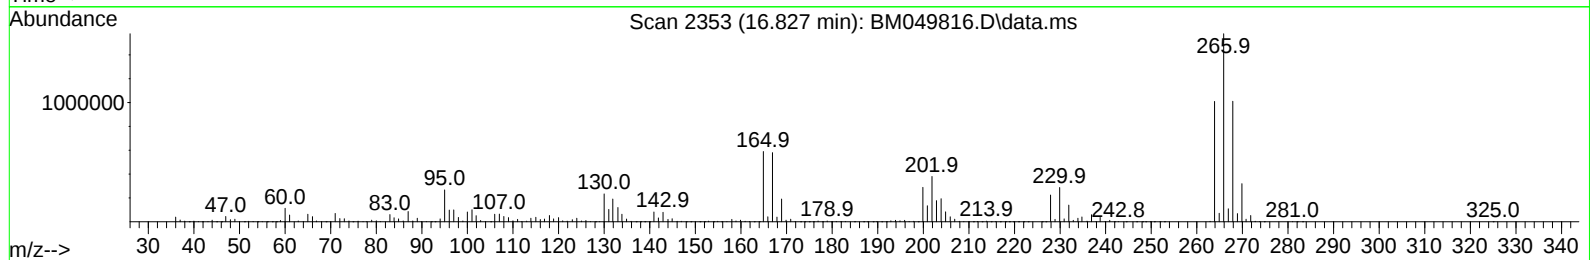


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040425\
Data File : BM049816.D
Acq On : 04 Apr 2025 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 12:21:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

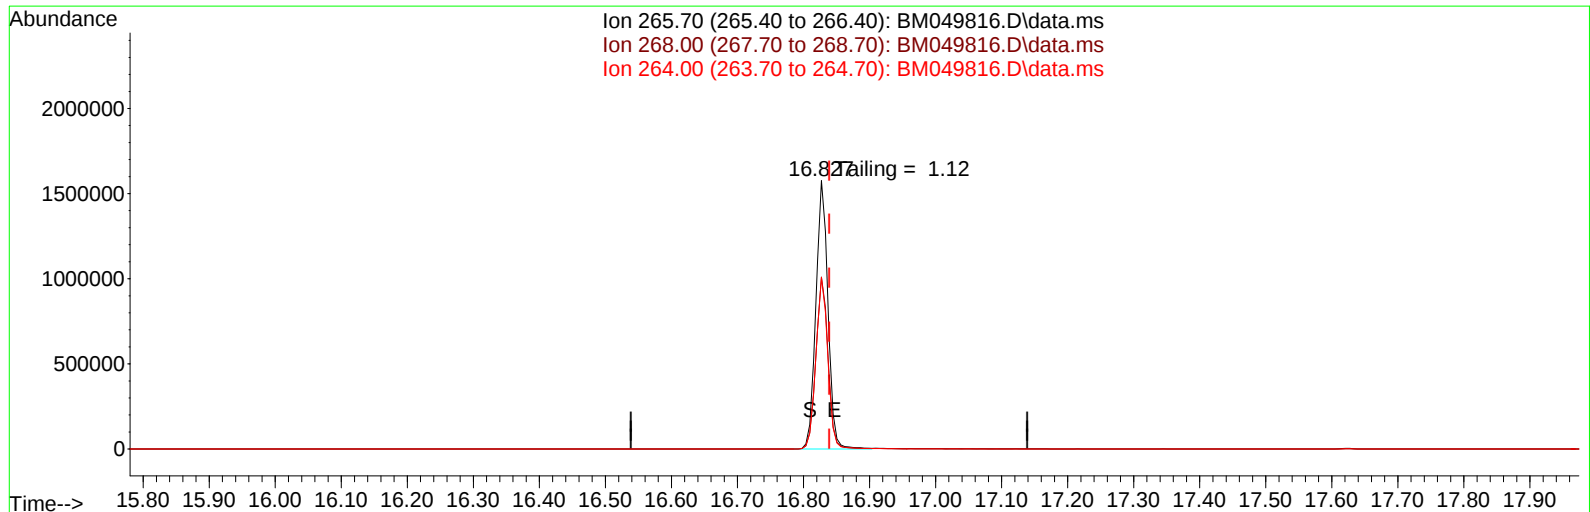

TIC: BM049816.D\data.ms

(70) Pentachlorophenol (C)




16.827min (-0.012) 278791.10 ng

response 2006266

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	64.09
264.00	64.10	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040425\
Data File : BM049816.D
Acq On : 04 Apr 2025 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 12:21:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

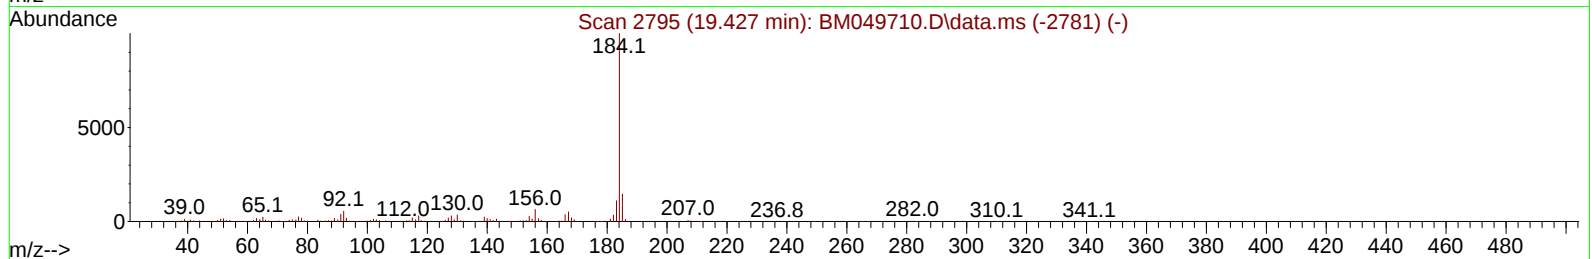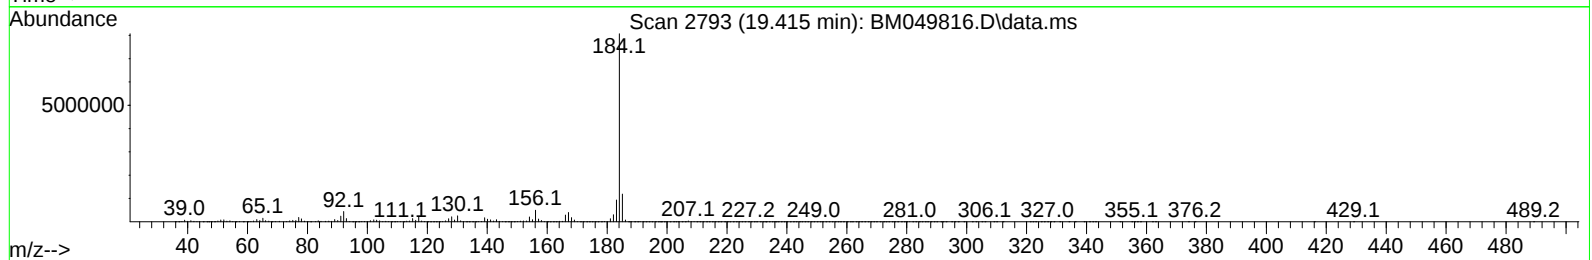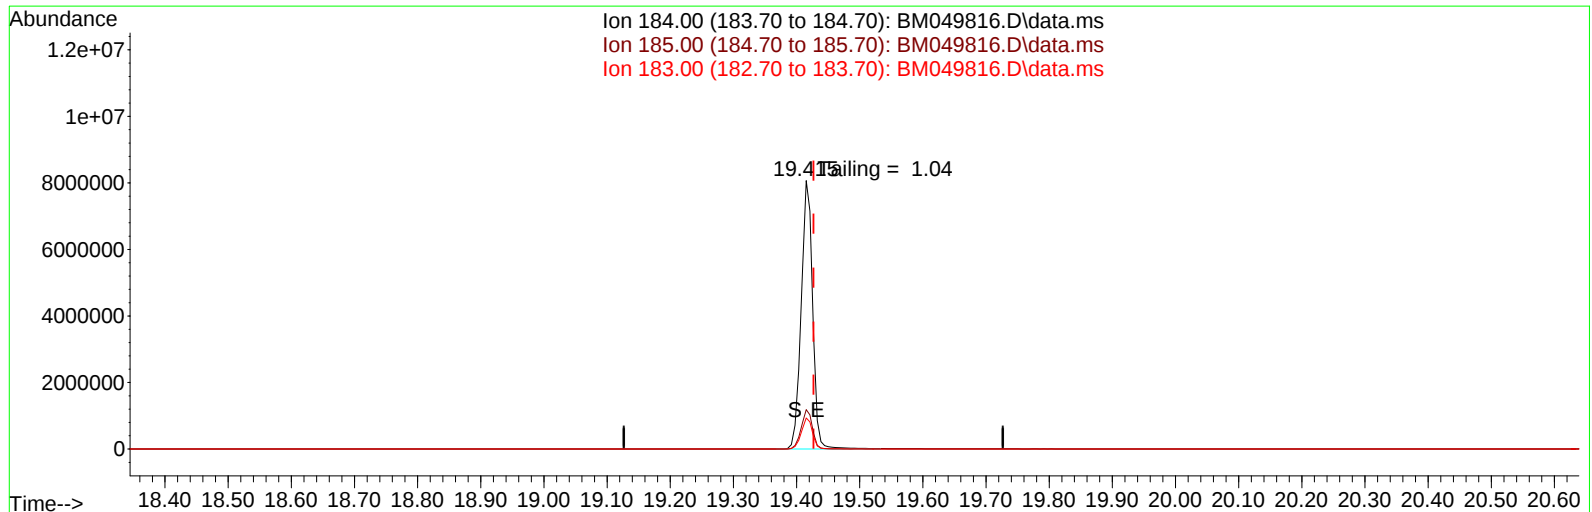

TIC: BM049816.D\data.ms

(77) Benzidine**19.415min (-0.012) 364848.31 ng****response 10256891**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.72
183.00	11.00	11.56
0.00	0.00	0.00