


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040425\
Data File : BM049816.D
Acq On : 04 Apr 2025 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 14:55:34 2025

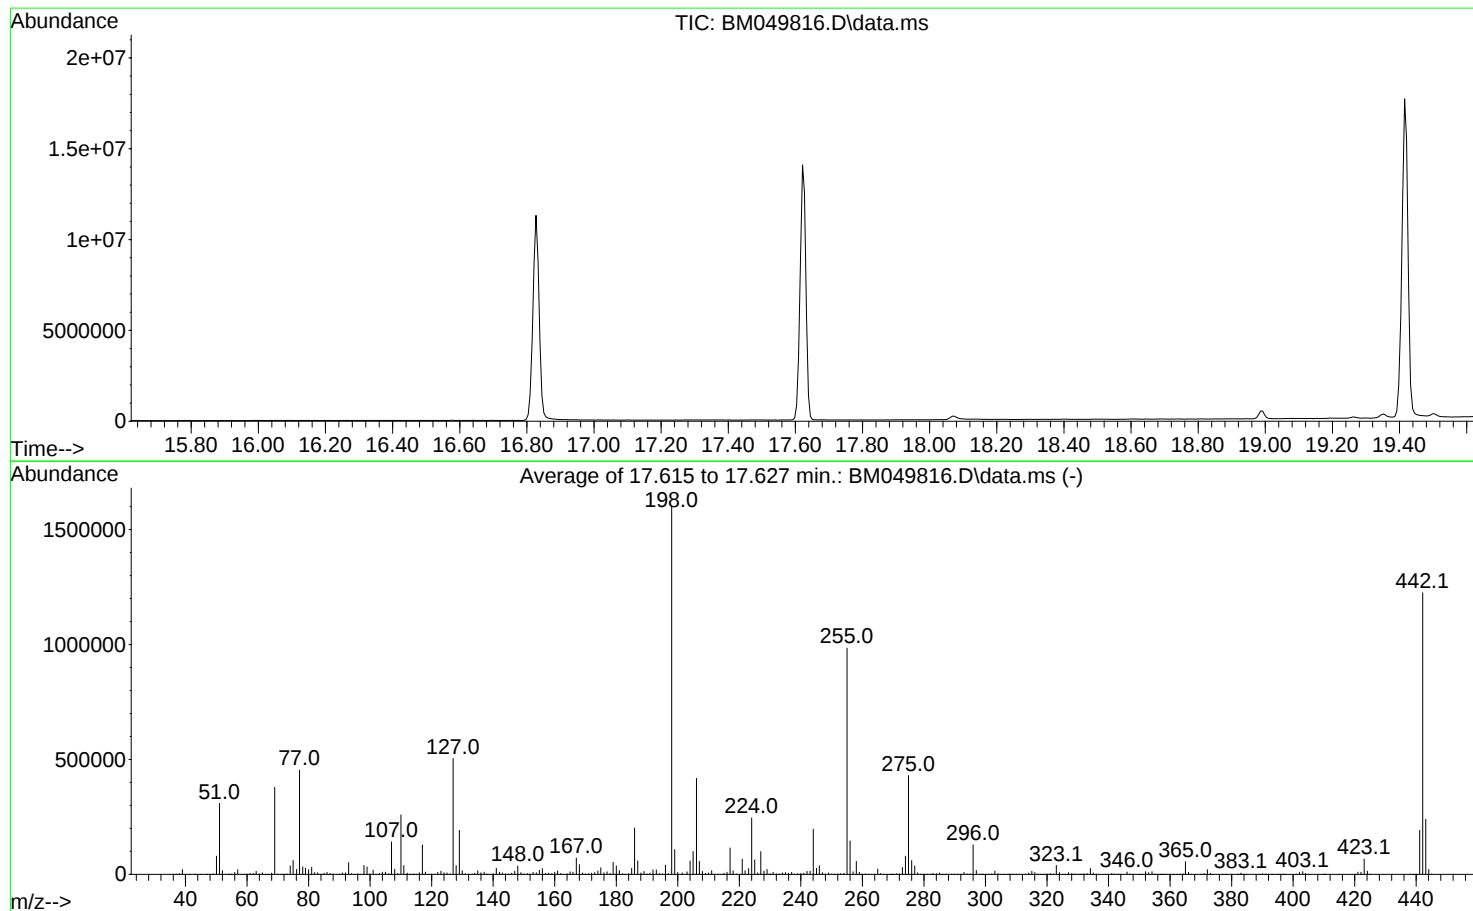




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.3	308941	PASS
68	69	0.00	2	1.4	5486	PASS
69	198	0.00	100	23.7	379111	PASS
70	69	0.00	2	0.4	1513	PASS
127	198	10	80	31.5	503957	PASS
197	198	0.00	2	0.2	3827	PASS
198	198	100	100	100.0	1600512	PASS
199	198	5	9	6.7	107885	PASS
275	198	10	60	26.9	429739	PASS
365	198	1	100	3.4	55160	PASS
441	198	0.01	100	12.0	191573	PASS
442	442	50	100	100.0	1225131	PASS
443	442	15	24	19.5	239296	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040425\
Data File : BM049816.D
Acq On : 04 Apr 2025 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 04 12:21:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

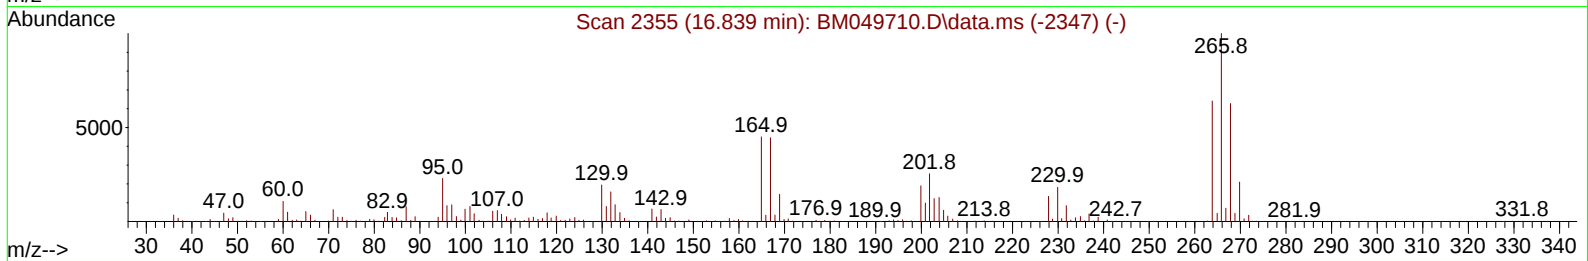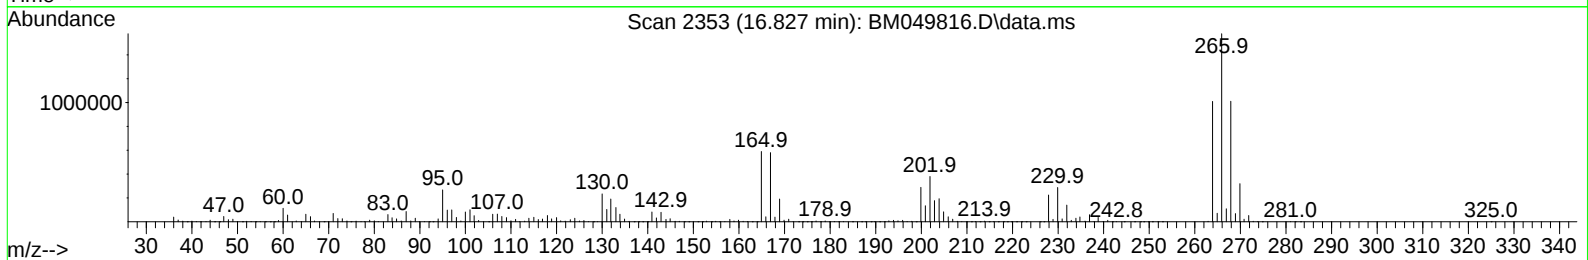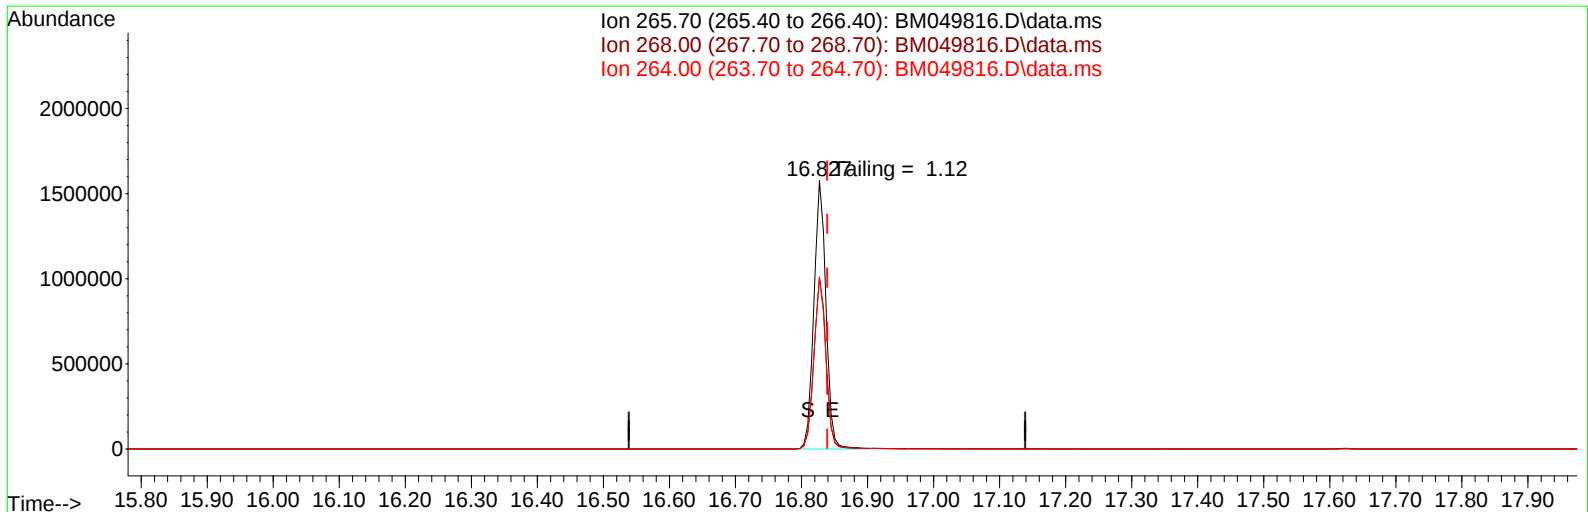

TIC: BM049816.D\data.ms

(70) Pentachlorophenol (C)

16.827min (-0.012) 278791.10 ng




response 2006266

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	64.09
264.00	64.10	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040425\
Data File : BM049816.D
Acq On : 04 Apr 2025 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 04 12:21:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

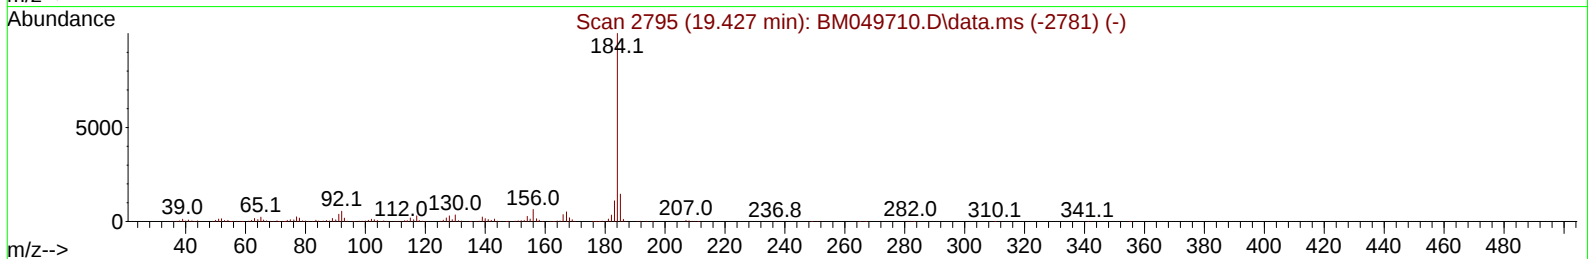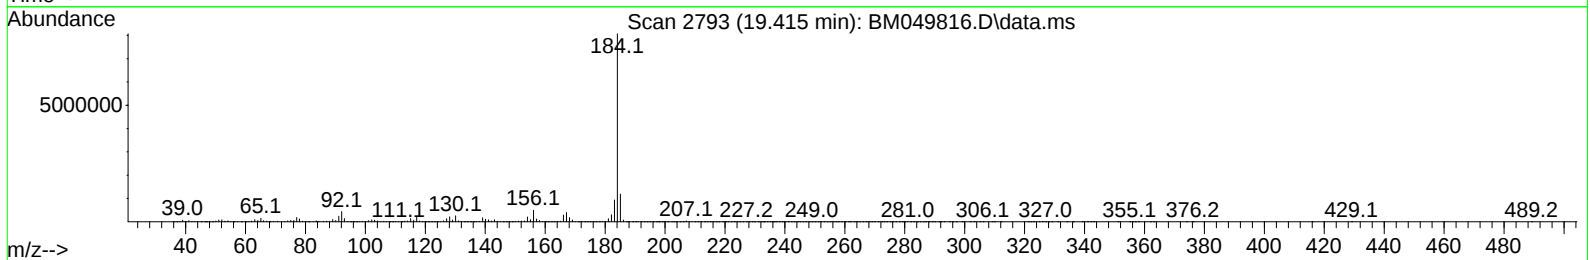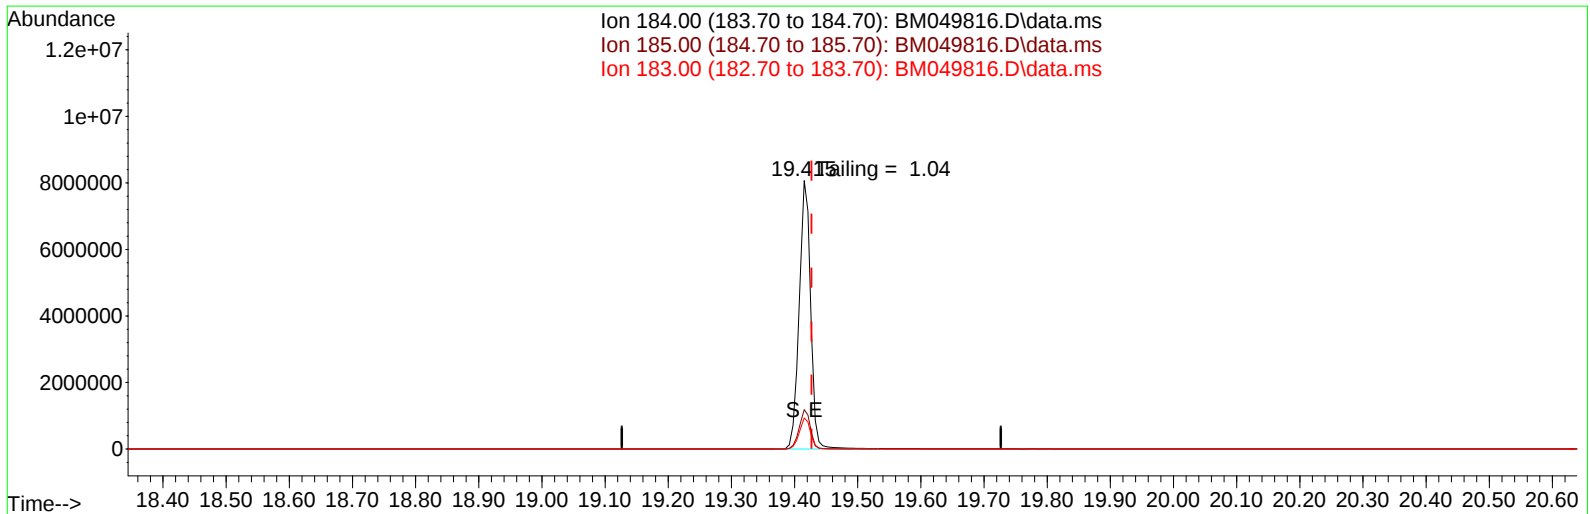

TIC: BM049816.D\data.ms

(77) Benzidine

19.415min (-0.012) 364848.31 ng

response 10256891

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.72
183.00	11.00	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/4/2025	BNA_M	<u>BM049816.D</u>
Compound Name	Response	Retention Time
DDT	5266388	20.65
DDD	53491	20.262
DDE	2681	19.709
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
56172	5322560	1.06

Instrument :
BNA_M
ClientSampleId :
DFTPP