


Data Path : Z:\HPCHEM1\BNA M\Data\BM040516\
 Data File : BM004882.D
 Acq On : 05 Apr 2016 16:22
 Operator : UM/SJ
 Sample : DFTPP45
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP45

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
 Title : SVOA CALIBRATION
 Last Update : Wed Apr 06 01:34:45 2016

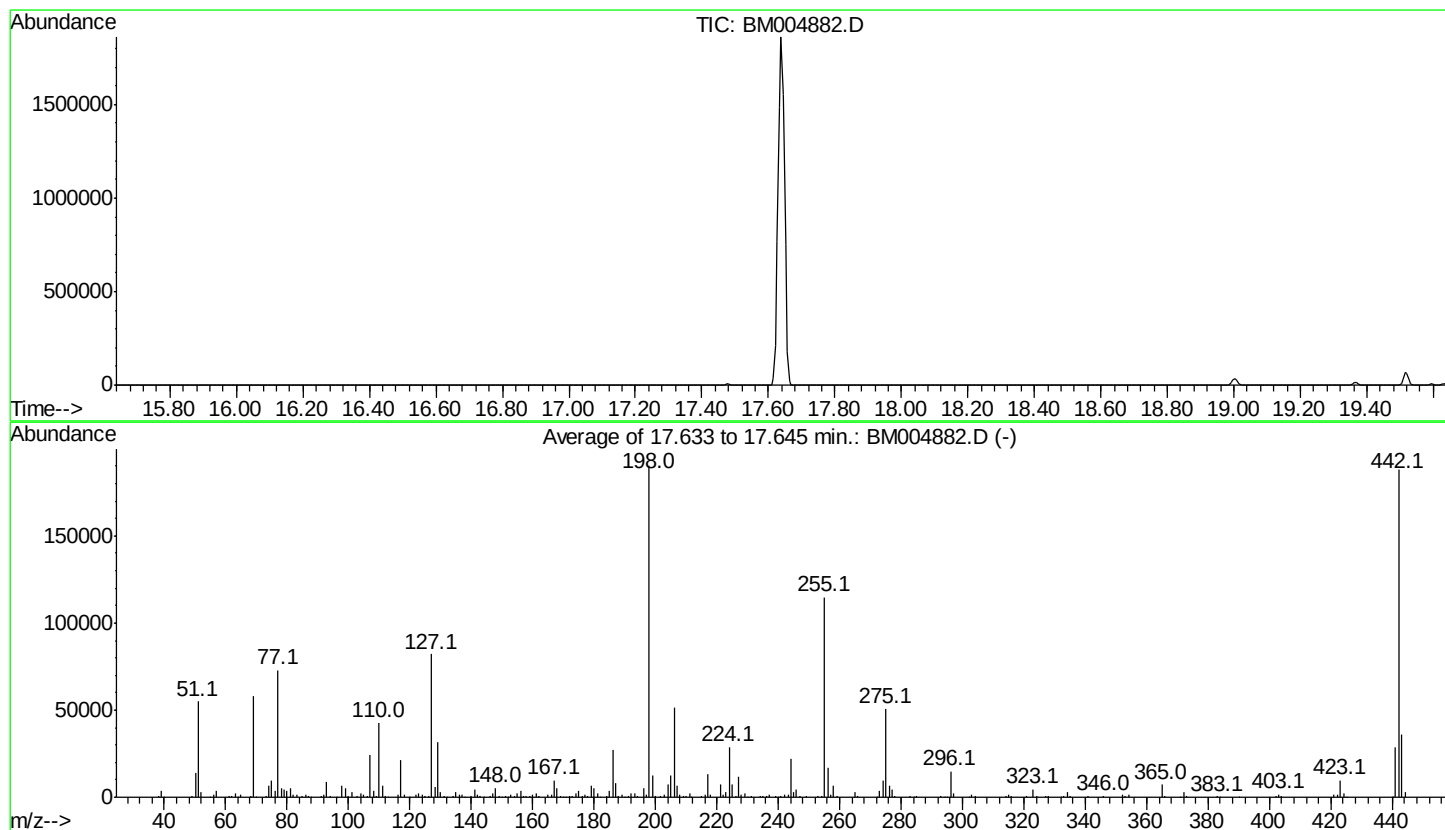

AutoFind: Scans 2541, 2542, 2543; Background Corrected with Scan 2535

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	54944	PASS
68	69	0.00	2	1.6	945	PASS
69	198	0.00	100	30.6	58178	PASS
70	69	0.00	2	0.2	115	PASS
127	198	10	80	43.2	82192	PASS
197	198	0.00	2	0.7	1271	PASS
198	198	100	100	100.0	190336	PASS
199	198	5	9	6.7	12726	PASS
275	198	10	60	26.7	50752	PASS
365	198	1	100	3.7	7074	PASS
441	443	0.01	100	79.6	28714	PASS
442	198	50	100	99.0	188480	PASS
443	442	15	24	19.1	36061	PASS

Scan 2535 (17.598 min): BM004882.D
DFTPP45

m/z	Abundance
44.00	398.0
207.00	360.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

m/z	Abundance
38.00	602.0
39.10	3698.0
44.00	305.0
49.00	423.0
50.10	14266.0
51.10	56944.0
52.10	2964.0
56.00	1611.0
57.00	3743.0
61.00	741.0
62.00	784.0
63.10	2319.0
64.00	300.0
65.00	1259.0
68.10	1019.0
69.00	59496.0
73.10	485.0
74.10	6231.0
75.00	9810.0
76.10	3459.0
77.10	73616.0
78.10	5121.0
79.00	4748.0
80.00	3428.0
81.00	4855.0
82.00	1271.0
83.10	1229.0
85.00	1090.0
86.00	1569.0
87.10	719.0
91.00	1198.0
92.00	1289.0
93.00	8787.0
94.00	615.0
96.00	381.0
98.00	6418.0
99.00	5748.0
100.00	526.0
101.00	2992.0
103.00	878.0
104.00	1936.0
105.00	1595.0
106.00	629.0
107.00	23976.0
108.00	3620.0
109.10	642.0
110.00	42984.0
111.00	6696.0
112.00	719.0
116.00	1312.0
117.00	20576.0
118.10	1616.0
120.00	342.0
122.00	1543.0
123.00	2306.0
124.00	1202.0
125.00	1107.0
126.20	556.0
127.10	80160.0
128.10	6168.0
129.00	31008.0
130.00	2754.0
131.00	560.0
134.00	953.0
135.00	2450.0
136.00	1269.0
137.10	1539.0
138.00	354.0
140.00	401.0
141.00	4322.0
142.00	1462.0
143.00	889.0
146.00	723.0
147.00	2236.0
148.00	5271.0
149.00	1062.0
150.00	363.0
151.00	518.0
153.00	1393.0
154.00	1061.0
155.00	2442.0
156.00	3858.0
157.10	617.0
158.00	788.0
159.00	625.0
160.00	1260.0
161.00	1932.0
162.00	662.0
165.00	1533.0
166.00	1301.0
167.00	9330.0
168.00	5517.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

169.00	807.0
170.90	386.0
172.00	756.0
173.00	1063.0
174.00	1936.0
175.10	3605.0
176.00	926.0
177.00	1551.0
178.00	548.0
179.00	6410.0
180.00	4768.0
181.00	2071.0
184.00	537.0
185.10	3109.0
186.10	25832.0
187.10	7354.0
188.00	888.0
189.00	1468.0
190.00	300.0
191.00	728.0
192.00	2105.0
193.10	2222.0
194.10	566.0
196.10	4778.0
197.10	1104.0
198.00	176512.0
199.00	12323.0
200.00	974.0
201.50	715.0
203.00	1263.0
204.10	6697.0
205.10	10873.0
206.10	48040.0
207.10	6452.0
208.00	1597.0
209.00	558.0
210.10	797.0
211.10	1859.0
215.00	586.0
216.00	1030.0
217.00	12578.0
218.00	1464.0
221.10	7185.0
221.90	1723.0
223.00	2813.0
224.10	25936.0
225.10	6691.0
226.10	786.0
227.10	10809.0
228.00	1578.0
229.00	2389.0
229.90	343.0
231.10	911.0
234.00	774.0
235.00	829.0
236.00	554.0
237.10	1199.0
239.00	445.0
240.00	345.0
241.00	725.0
242.00	1355.0
243.10	1543.0
244.10	19528.0
245.10	2760.0
246.00	3913.0
247.10	742.0
249.00	674.0
253.00	472.0
254.20	819.0
255.10	100608.0
256.10	14774.0
257.10	1227.0
258.00	6146.0
259.00	1045.0
265.00	2611.0
266.00	327.0
273.00	3023.0
274.10	8036.0
275.10	43456.0
276.10	6001.0
277.00	4085.0
278.00	729.0
283.00	355.0
285.00	571.0
293.00	969.0
295.00	310.0
296.00	12523.0
297.00	1623.0
303.00	1214.0
304.00	397.0
314.10	678.0
315.00	1398.0
316.00	770.0
321.10	379.0
323.10	3790.0
324.10	763.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

327.00	713.0
328.00	411.0
332.10	324.0
333.10	417.0
334.10	2483.0
335.00	781.0
341.00	427.0
346.00	893.0
352.10	1134.0
353.10	935.0
354.10	1275.0
365.00	5587.0
366.00	839.0
372.10	2010.0
373.10	477.0
383.00	566.0
402.00	905.0
403.10	1133.0
404.00	385.0
421.00	1222.0
422.10	1031.0
423.10	7356.0
424.10	2313.0
425.00	311.0
441.10	20864.0
442.10	138048.0
443.10	27032.0
444.10	2524.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

m/z	Abundance
38.00	610.0
39.10	3931.0
49.10	467.0
50.10	15391.0
51.10	60088.0
52.10	3173.0
55.00	309.0
56.00	1950.0
57.00	4240.0
61.00	867.0
62.00	1002.0
63.00	2568.0
64.00	383.0
65.10	1211.0
68.10	1002.0
69.00	64888.0
70.00	345.0
73.00	469.0
74.10	7280.0
75.00	10848.0
76.10	3633.0
77.10	81920.0
78.10	5810.0
79.00	5184.0
80.00	4169.0
81.00	5575.0
82.00	1380.0
83.00	1219.0
85.00	1191.0
86.00	1681.0
87.00	731.0
88.00	321.0
91.00	1192.0
92.00	1407.0
93.00	9869.0
94.00	742.0
96.00	465.0
98.00	7831.0
99.00	5964.0
100.00	442.0
101.00	3449.0
103.00	1082.0
104.00	1962.0
105.00	2114.0
106.00	644.0
107.10	27496.0
108.10	4178.0
109.10	837.0
110.00	46784.0
111.00	7382.0
112.00	857.0
113.00	333.0
116.00	1517.0
117.00	24264.0
118.00	1800.0
122.00	1797.0
123.00	2784.0
124.00	1334.0
125.00	1220.0
126.20	559.0
127.10	93368.0
128.00	6766.0
129.00	36632.0
130.00	3148.0
131.10	559.0
134.00	1026.0
135.00	3157.0
136.10	1331.0
137.10	1605.0
138.00	309.0
140.00	427.0
141.00	5157.0
142.00	1692.0
143.00	1202.0
144.10	303.0
146.00	944.0
147.00	2530.0
148.00	6155.0
149.00	1225.0
150.00	411.0
151.10	583.0
151.90	407.0
153.00	1556.0
154.00	1199.0
155.00	2784.0
156.10	4323.0
157.10	772.0
158.00	885.0
159.00	813.0
160.00	1676.0
161.00	2506.0
162.00	586.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

165.00	1987.0
166.00	1582.0
167.10	10995.0
168.00	5859.0
169.00	911.0
170.00	324.0
171.00	421.0
172.00	882.0
173.00	1292.0
174.10	2207.0
175.10	4047.0
176.00	1037.0
177.00	2112.0
178.00	629.0
179.00	7704.0
180.00	5371.0
181.00	2672.0
182.10	407.0
184.00	718.0
185.10	4179.0
186.10	30624.0
187.10	9286.0
188.00	893.0
189.00	2009.0
190.00	374.0
191.00	939.0
192.00	2591.0
193.10	2838.0
194.10	615.0
196.00	5990.0
197.10	1518.0
198.00	216000.0
199.00	14395.0
200.00	1184.0
201.50	821.0
203.00	1515.0
204.10	8342.0
205.10	13830.0
206.10	58992.0
207.10	8069.0
208.10	2127.0
209.10	779.0
210.20	1004.0
211.10	2192.0
211.80	408.0
215.10	639.0
216.10	1374.0
217.00	15181.0
218.00	2084.0
221.10	8531.0
221.90	2078.0
223.10	3589.0
224.10	32872.0
225.10	8610.0
226.10	1000.0
227.10	13857.0
228.00	1936.0
229.00	2683.0
230.00	302.0
231.00	1288.0
234.00	819.0
235.00	1070.0
236.00	639.0
237.10	1216.0
239.00	513.0
240.00	375.0
241.00	768.0
242.10	1687.0
243.10	1927.0
244.10	25488.0
245.10	3030.0
246.00	5390.0
247.00	1083.0
249.00	867.0
253.00	674.0
254.20	1370.0
255.10	132032.0
256.10	19296.0
257.00	1484.0
258.10	7744.0
259.00	1327.0
265.10	2991.0
266.00	468.0
272.00	345.0
273.00	3770.0
274.10	11019.0
275.10	58648.0
276.10	7712.0
277.00	5335.0
278.00	943.0
283.10	575.0
284.10	436.0
285.00	1024.0
293.00	1199.0
294.00	319.0
295.00	340.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

296.10	16904.0
297.10	2267.0
302.00	339.0
303.10	1994.0
304.00	522.0
314.00	817.0
315.00	1838.0
316.00	931.0
321.00	554.0
323.10	5244.0
324.10	1034.0
327.00	1029.0
328.00	570.0
332.00	355.0
333.10	507.0
334.10	3532.0
335.10	1015.0
341.10	662.0
346.00	1203.0
352.10	1627.0
353.00	1194.0
354.10	1887.0
365.00	8241.0
366.00	1207.0
371.00	303.0
372.10	3090.0
373.10	779.0
383.10	728.0
384.00	302.0
390.00	376.0
402.00	1229.0
403.10	1776.0
404.00	612.0
421.00	1609.0
422.10	1629.0
423.10	11145.0
424.10	2585.0
425.10	353.0
439.90	303.0
441.10	32944.0
442.10	216576.0
443.10	42624.0
444.10	3857.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

m/z	Abundance
38.00	490.0
39.10	3060.0
40.00	310.0
44.00	361.0
49.10	361.0
50.10	11899.0
51.10	47800.0
52.10	2160.0
56.00	1335.0
57.00	3045.0
61.00	628.0
62.00	599.0
63.00	2187.0
65.10	1000.0
68.00	814.0
69.00	50152.0
73.00	388.0
74.10	5590.0
75.00	8601.0
76.10	3003.0
77.10	63120.0
78.10	4373.0
79.00	3989.0
80.00	3116.0
81.00	4260.0
82.00	1114.0
83.00	961.0
85.00	1046.0
86.00	1162.0
87.00	598.0
91.00	976.0
92.00	1096.0
93.00	7338.0
94.10	534.0
98.00	5667.0
99.00	4815.0
100.00	490.0
101.00	2459.0
103.00	773.0
104.00	1725.0
105.00	1567.0
106.00	563.0
107.00	21336.0
108.00	3306.0
109.00	558.0
110.00	38080.0
111.00	5750.0
112.00	715.0
116.10	1171.0
117.00	18096.0
118.00	1397.0
122.00	1325.0
123.00	2140.0
124.00	906.0
125.00	842.0
126.20	474.0
127.10	73048.0
128.00	5658.0
129.00	27736.0
130.00	2275.0
131.00	426.0
132.10	345.0
134.00	754.0
135.00	2286.0
136.00	932.0
137.00	1338.0
140.00	397.0
141.00	3950.0
142.00	1168.0
143.00	923.0
146.10	709.0
147.00	2014.0
148.00	4772.0
149.00	1039.0
150.00	302.0
151.10	435.0
153.00	1225.0
154.00	857.0
155.00	2213.0
156.10	3470.0
157.10	554.0
158.00	717.0
159.10	557.0
160.00	1380.0
161.00	2022.0
162.00	591.0
165.00	1638.0
166.00	1301.0
167.00	8726.0
168.00	4632.0
169.00	720.0
171.00	362.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

172.00	702.0
173.00	981.0
174.00	1838.0
175.10	3164.0
176.10	870.0
177.00	1536.0
178.00	552.0
179.00	6427.0
180.10	4468.0
181.00	2078.0
182.00	346.0
184.00	434.0
185.10	3244.0
186.10	24776.0
187.10	7262.0
188.10	678.0
189.00	1568.0
191.00	651.0
192.00	2070.0
193.10	2516.0
194.00	440.0
196.00	4936.0
197.10	1191.0
198.00	178496.0
199.00	11460.0
200.00	860.0
201.60	650.0
203.00	1202.0
204.10	6670.0
205.10	12055.0
206.10	48248.0
207.10	6385.0
208.10	1606.0
209.00	601.0
210.20	670.0
211.10	1773.0
215.00	590.0
216.00	1077.0
217.00	13060.0
218.00	1593.0
221.10	6973.0
221.90	1556.0
223.00	2918.0
224.10	27576.0
225.10	7187.0
226.10	764.0
227.00	11090.0
228.00	1585.0
229.00	2222.0
231.10	947.0
234.00	730.0
235.00	887.0
236.10	568.0
237.00	988.0
239.00	514.0
240.00	359.0
241.00	694.0
242.00	1485.0
243.10	1607.0
244.10	21056.0
245.10	2529.0
246.00	4415.0
247.00	881.0
249.10	642.0
253.00	553.0
254.10	1159.0
255.10	111424.0
256.10	16330.0
257.10	1295.0
258.00	6595.0
259.00	917.0
265.00	2651.0
266.00	389.0
272.10	362.0
273.00	3426.0
274.00	9550.0
275.10	50152.0
276.10	6696.0
277.00	4252.0
278.00	731.0
283.00	478.0
284.10	356.0
285.10	787.0
293.00	941.0
295.00	370.0
296.00	15408.0
297.10	2039.0
303.10	1790.0
304.00	434.0
314.10	857.0
315.00	1685.0
316.10	976.0
321.00	507.0
323.10	4881.0
324.10	941.0
327.00	1016.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

328.00	502.0
331.90	358.0
333.10	526.0
334.10	3279.0
335.10	769.0
341.00	571.0
346.00	1165.0
352.00	1572.0
353.00	1086.0
354.10	1572.0
365.00	7394.0
366.00	1004.0
371.10	445.0
372.10	2712.0
373.10	724.0
383.00	850.0
390.00	387.0
402.00	1086.0
403.00	1669.0
404.00	626.0
421.00	1463.0
422.10	1636.0
423.10	10777.0
424.10	2391.0
440.10	356.0
441.10	32336.0
442.10	210816.0
443.10	38528.0
444.10	3337.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45