
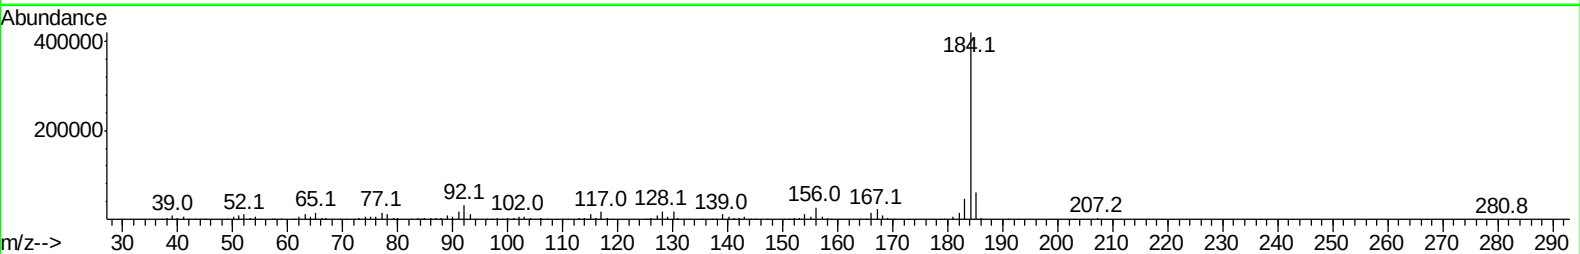


```
Data Path : Z:\HPCHEM1\BNA M\DATA\BM040517\  
Data File : BM009530.D  
Acq On    : 04 Apr 2017  15:27  
Operator  : SJ/MA  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Apr 05 05:27:20 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 12:10:26 2017
Response via : Initial Calibration

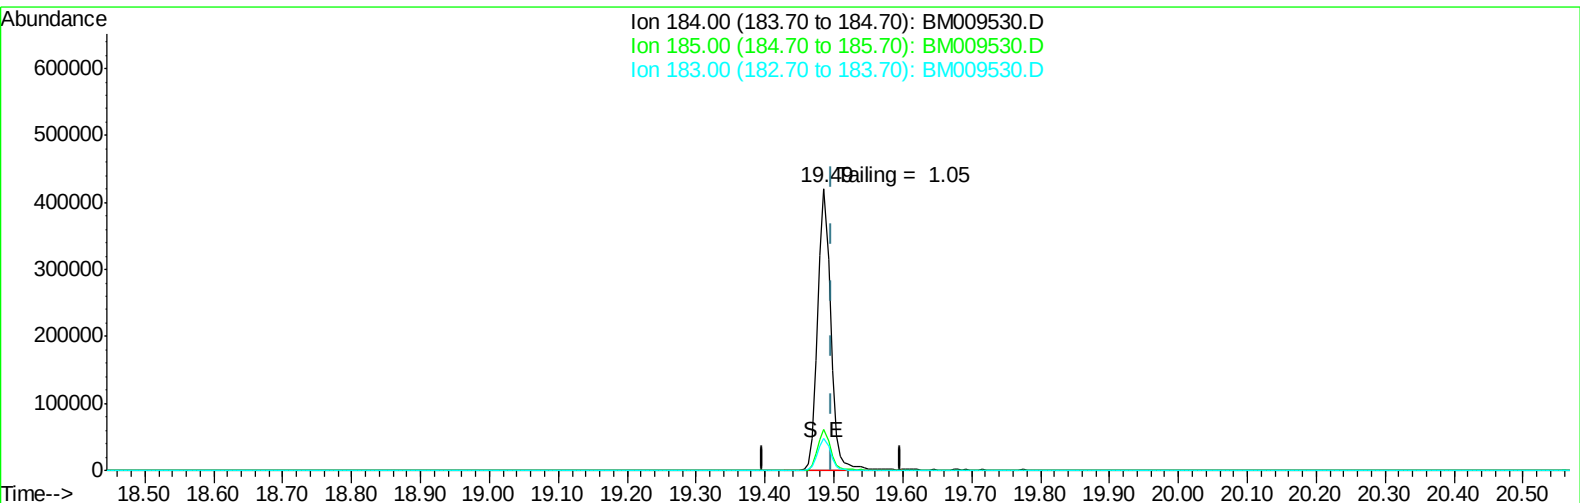

TIC: BM009530.D




(76) Benzidine

19.486min (-0.012) 26756.65ng

response 547839

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040517\
Data File : BM009530.D
Acq On : 04 Apr 2017 15:27
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 05:27:20 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 12:10:26 2017
Response via : Initial Calibration

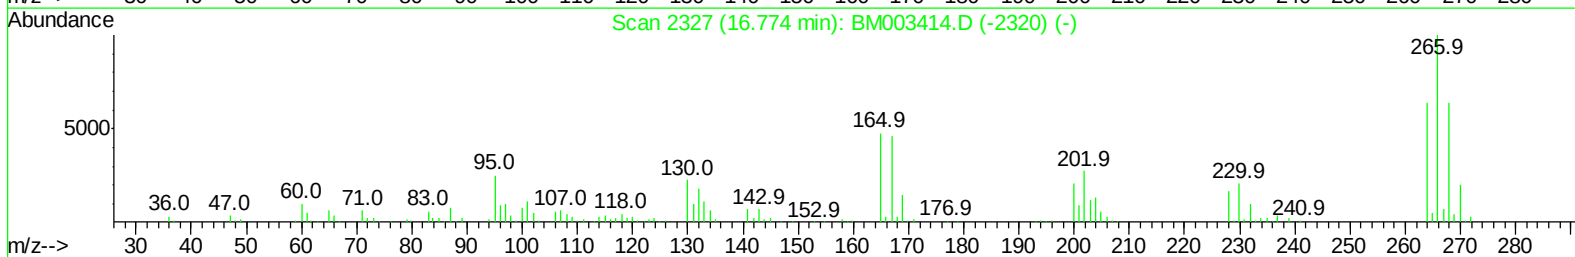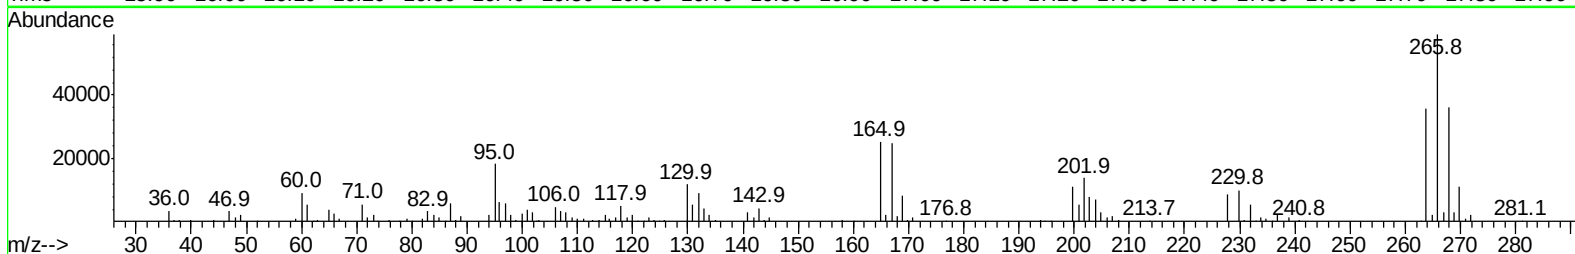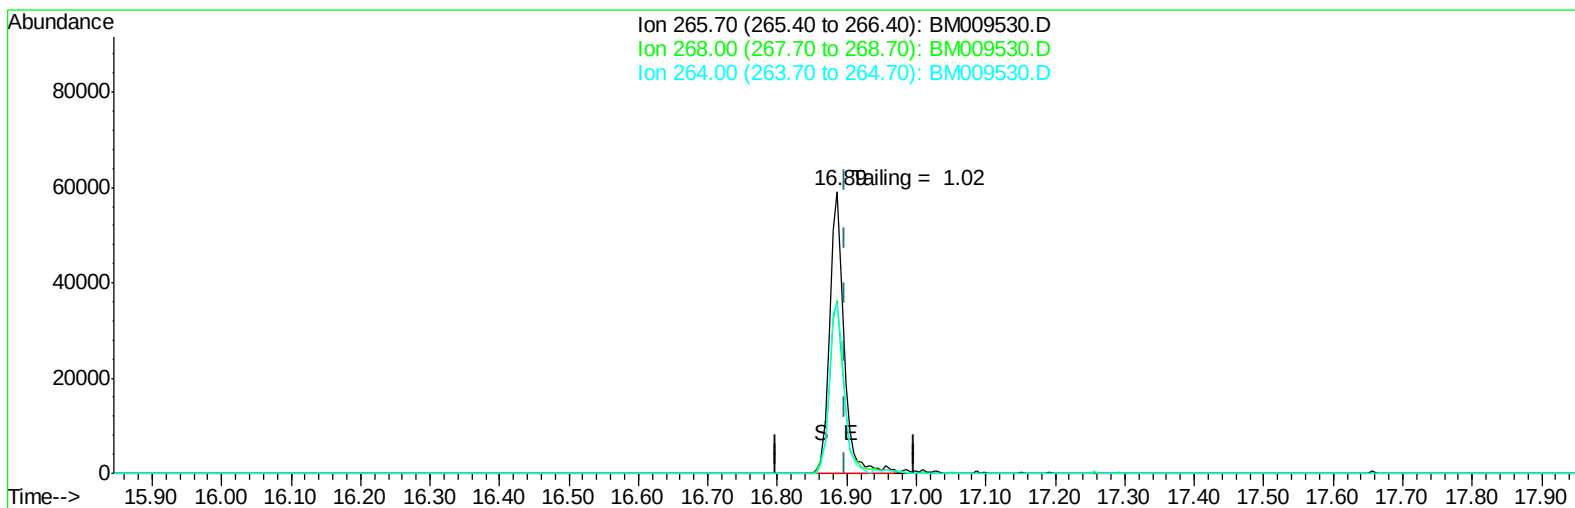

TIC: BM009530.D

(69) Pentachlorophenol (C)

16.886min (-0.012) 0.00ng

response 84503

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.35
264.00	61.20	60.56
0.00	0.00	0.00