

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
 Data File : BM019754.D
 Acq On : 05 Apr 2019 18:09
 Operator : JU/SJ
 Sample : K2217-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF613

Quant Time: Apr 06 00:23:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 06 00:13:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	167061	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	786544	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	460180	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	1002409	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	829480	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	747674	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	20813	4.88	ng/uL	0.00
5) Phenol-d5	6.75	99	310504	20.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	195015	19.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	243942	21.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	257878	23.09	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	119218	21.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	141848	22.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	247936	21.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	323572	22.87	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	752640	20.27	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	1004907	21.64	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	90900	15.62	ng/ul	0.01
58) Fluorene-d10	15.22	176	682823	21.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	71883	10.84	ng/ul	0.00
71) Anthracene-d10	17.08	188	1040423	21.63	ng/ul	0.00
79) Pyrene-d10	19.39	212	1037711	27.08	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	796268	20.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	148672	3.991	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
Data File : BM019754.D
Acq On : 05 Apr 2019 18:09
Operator : JU/SJ
Sample : K2217-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF613

Quant Time: Apr 06 00:23:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 06 00:13:11 2019
Response via : Initial Calibration

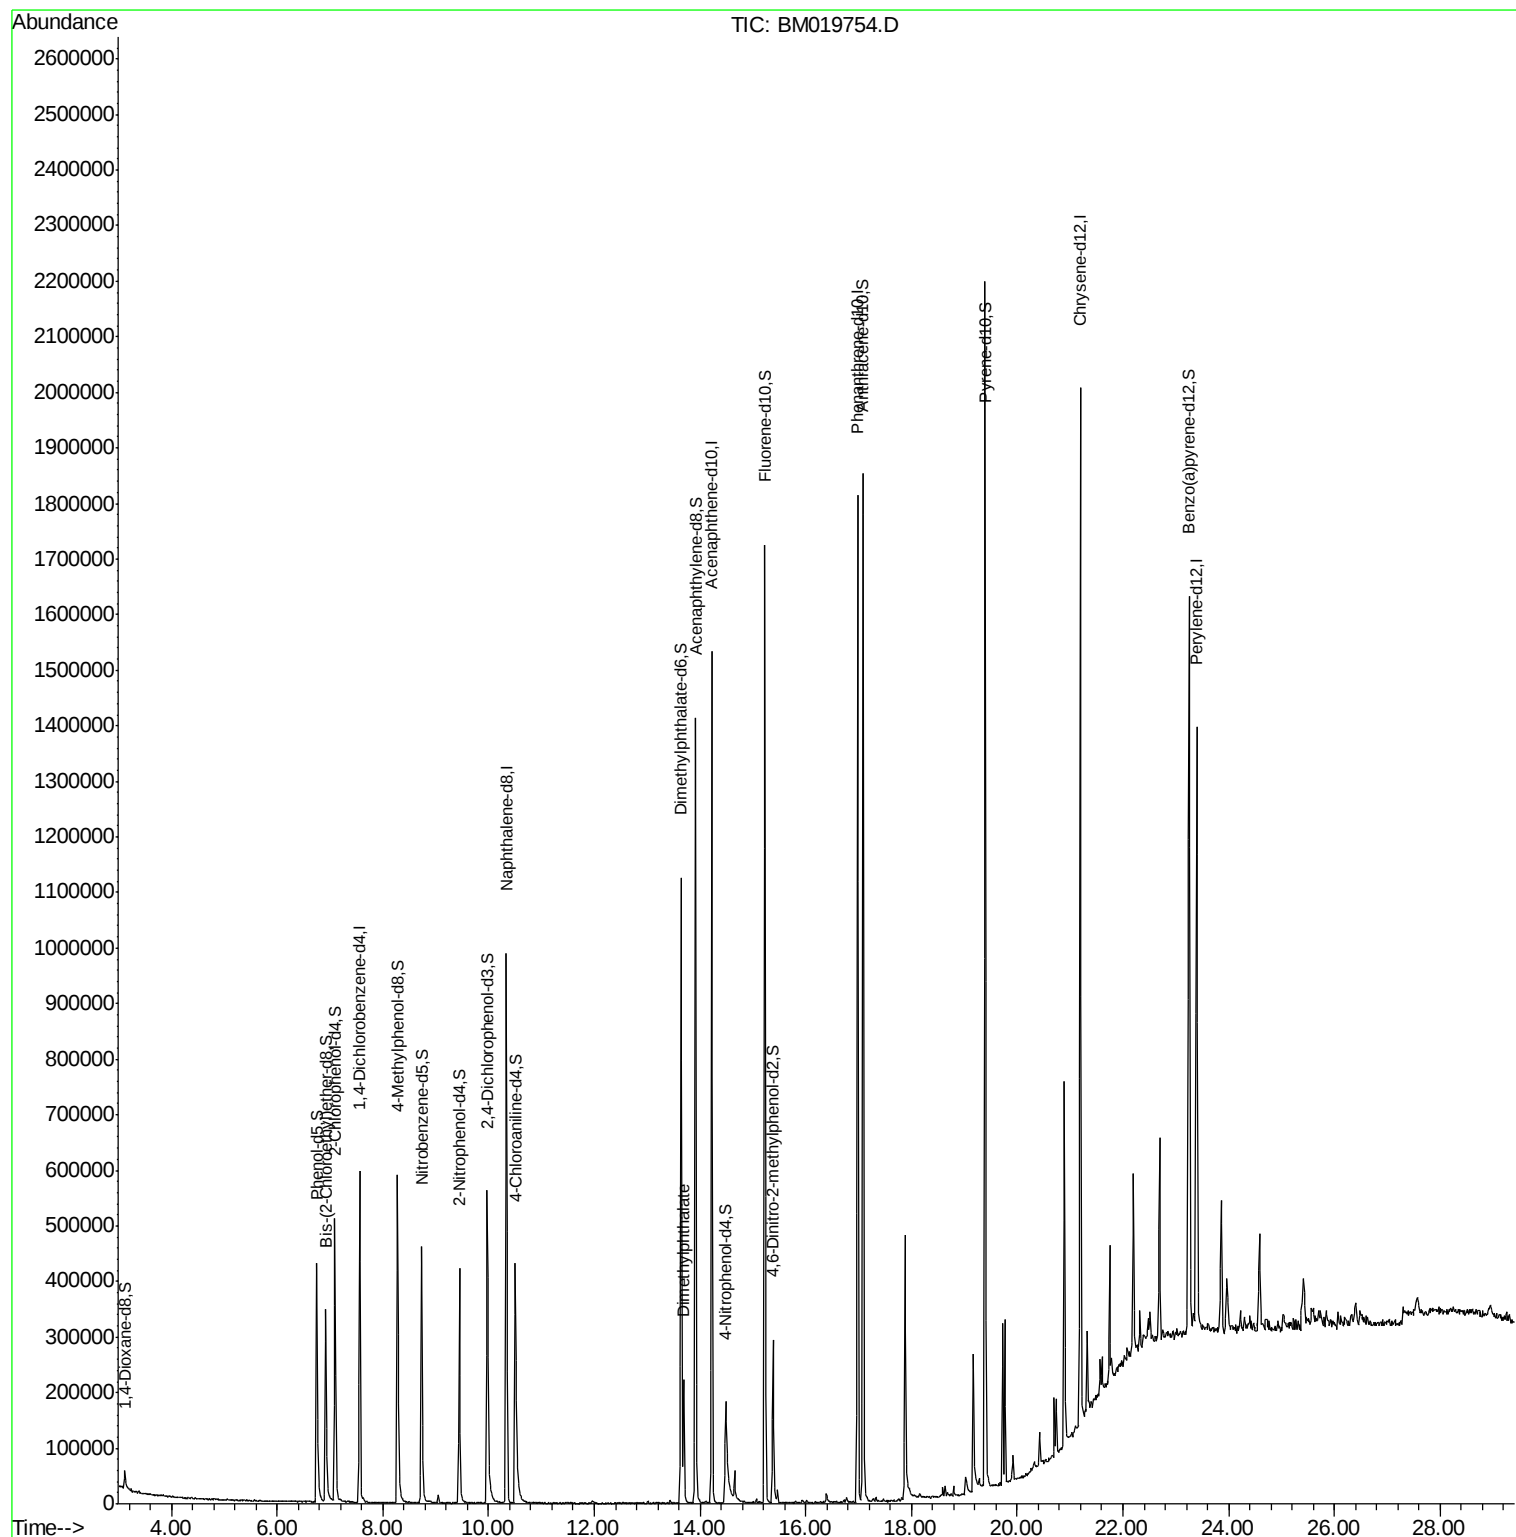

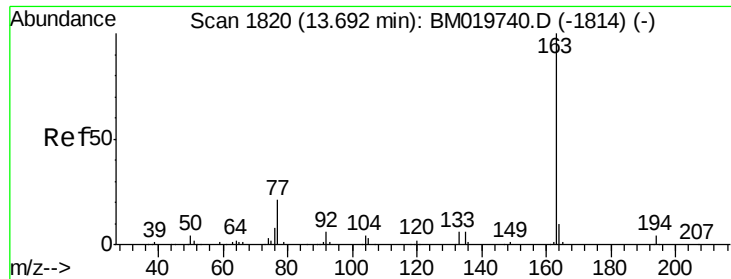

#45

Dimethylphthalate

Concen: 3.991 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. 0.00 min

Lab File: BM019754.D

Acq: 05 Apr 2019 18:09

Instrument :

BNA_M

ClientSampleId :

BF613



Tgt Ion:163 Resp: 148672

Ion Ratio Lower Upper

163 100

194 3.8 4.0 6.0#

164 10.1 8.4 12.6

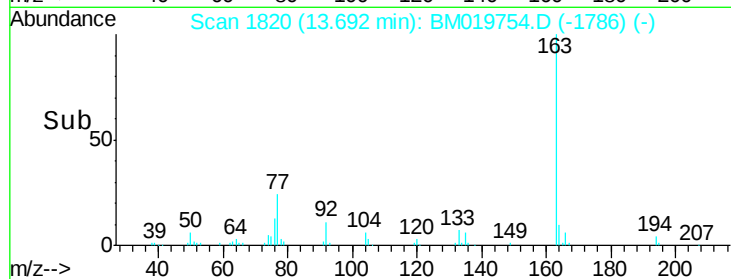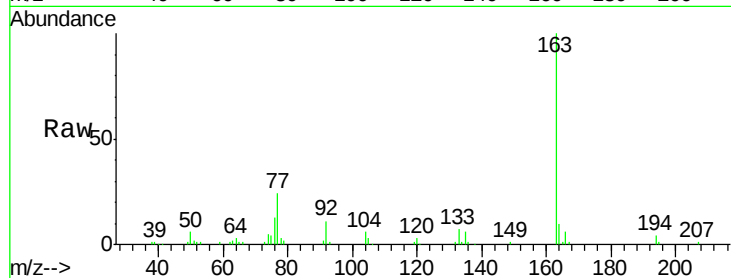

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

120000

100000

80000

60000

40000

20000

0

13.69

13.70

13.80

Time-->