

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
 Data File : BM019742.D
 Acq On : 05 Apr 2019 10:17
 Operator : JU/SJ
 Sample : K2188-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF652

Quant Time: Apr 06 00:21:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 06 00:13:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	175786	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	794663	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	477559	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	1047049	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	839470	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	792817	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	21324	4.75	ng/uL	0.00
5) Phenol-d5	6.75	99	263811	16.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	165280	15.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	206607	17.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	206930	17.61	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	102102	18.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	117701	18.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	209285	17.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	232451	16.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	761162	19.75	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	864772	17.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	84933	14.06	ng/ul	0.00
58) Fluorene-d10	15.23	176	650450	19.59	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	99630	14.39	ng/ul	0.00
71) Anthracene-d10	17.09	188	956727	19.04	ng/ul	0.00
79) Pyrene-d10	19.39	212	924574	23.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	691509	16.45	ng/ul	0.00


Target Compounds					Qvalue	
45) Dimethylphthalate	13.69	163	136372	3.527	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
Data File : BM019742.D
Acq On : 05 Apr 2019 10:17
Operator : JU/SJ
Sample : K2188-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BF652

Quant Time: Apr 06 00:21:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 06 00:13:11 2019
Response via : Initial Calibration

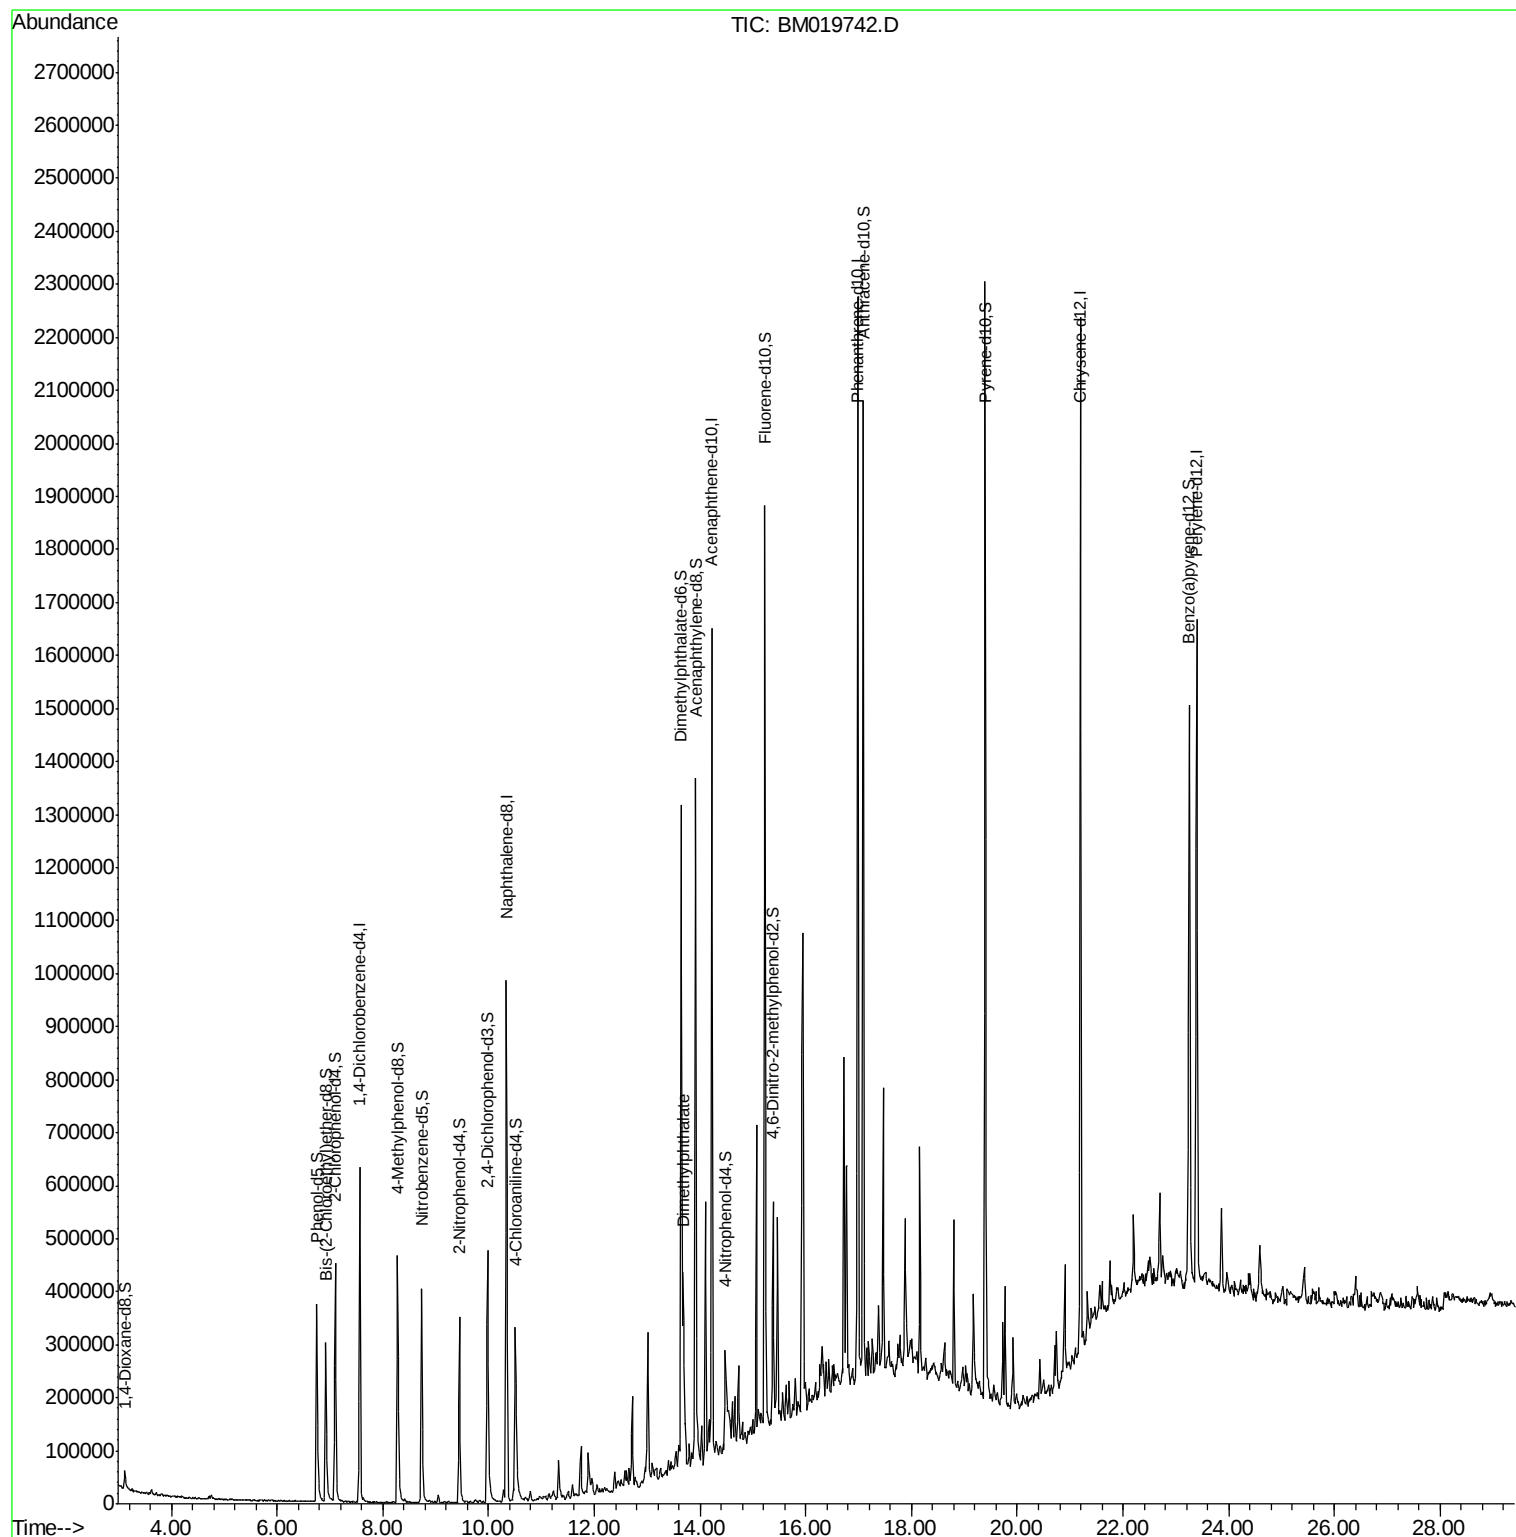

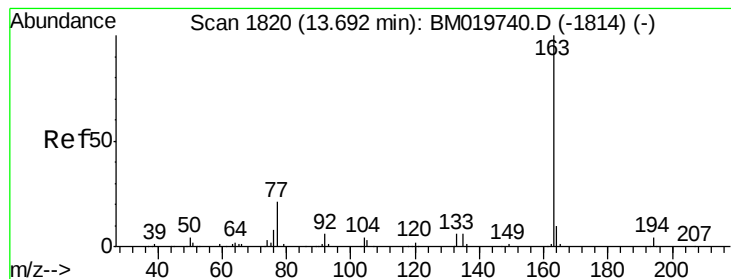

#45

Dimethylphthalate

Concen: 3.527 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.00 min

Lab File: BM019742.D

Acq: 05 Apr 2019 10:17

Instrument :

BNA_M

ClientSampleId :

BF652


Tgt Ion:163 Resp: 136372

Ion Ratio Lower Upper

163 100

194 4.1 4.0 6.0

164 10.0 8.4 12.6

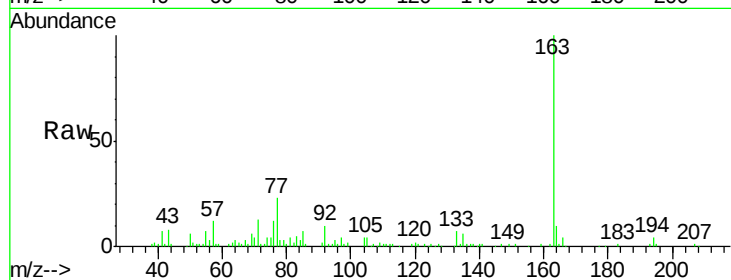

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

