

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
 Data File : BM019771.D
 Acq On : 06 Apr 2019 04:23
 Operator : JU/SJ
 Sample : K2217-14
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF604

Quant Time: Apr 06 05:25:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 06 00:13:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	152626	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	715390	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	429792	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	975307	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	927525	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	870337	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	22661	5.81	ng/uL	0.00
5) Phenol-d5	6.75	99	237307	17.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	156399	17.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	195597	18.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	184429	18.08	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	96631	18.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	112247	19.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	190006	17.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	263313	20.46	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	704211	20.31	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	826047	19.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	81675	15.02	ng/ul	0.00
58) Fluorene-d10	15.22	176	601256	20.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	87277	13.53	ng/ul	0.00
71) Anthracene-d10	17.08	188	926066	19.79	ng/ul	0.00
79) Pyrene-d10	19.39	212	1022306	23.86	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	853411	18.50	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	106996	3.075	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
Data File : BM019771.D
Acq On : 06 Apr 2019 04:23
Operator : JU/SJ
Sample : K2217-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF604

Quant Time: Apr 06 05:25:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 06 00:13:11 2019
Response via : Initial Calibration

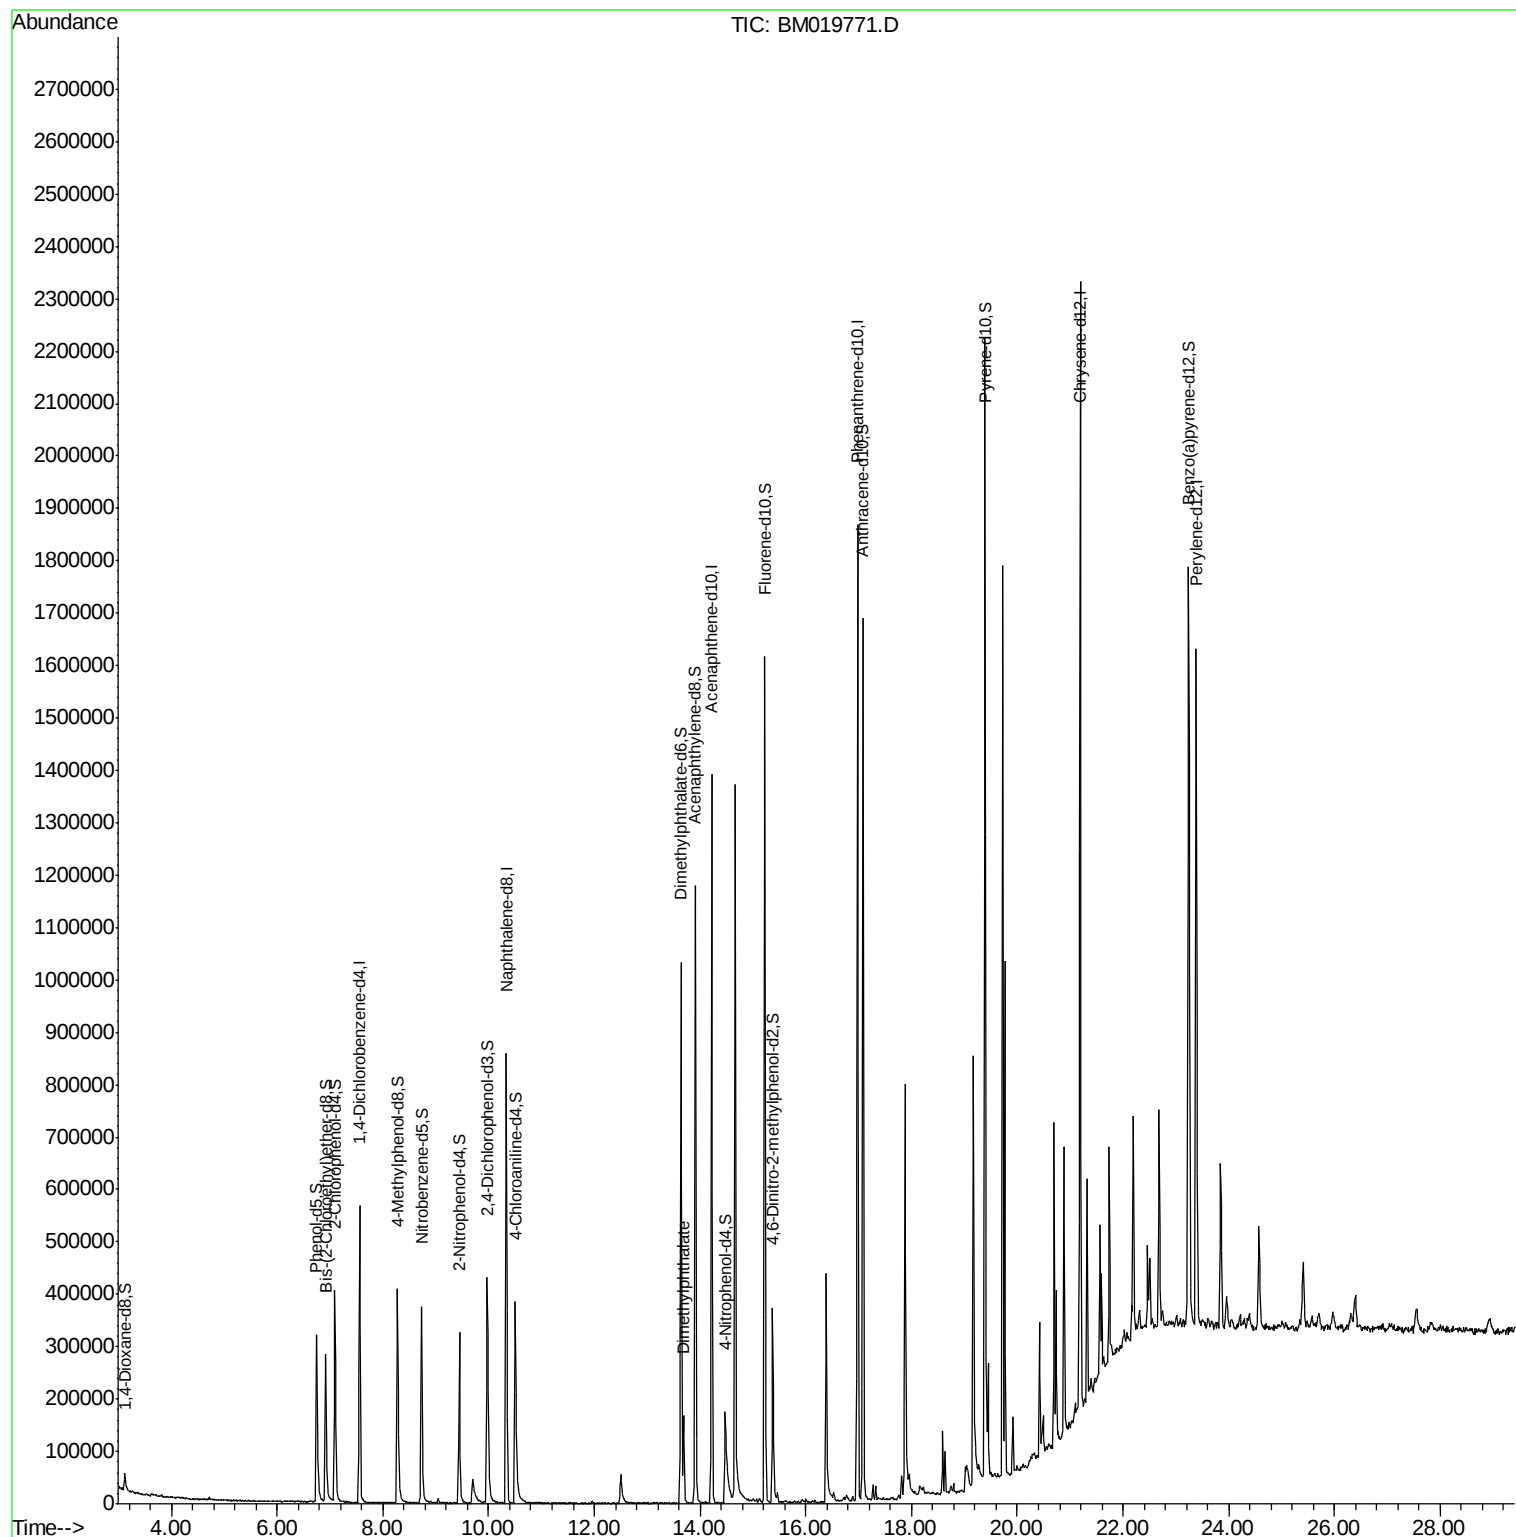

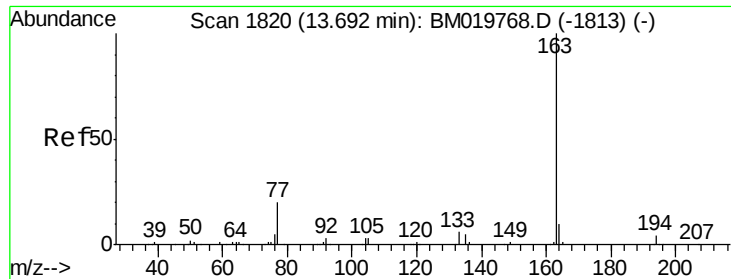

#45

Dimethylphthalate

Concen: 3.075 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.00 min

Lab File: BM019771.D

Acq: 06 Apr 2019 04:23

Instrument :

BNA_M

ClientSampleId :

BF604


Tgt Ion:163 Resp: 106996

Ion Ratio Lower Upper

163 100

194 4.7 4.0 6.0

164 10.0 8.4 12.6

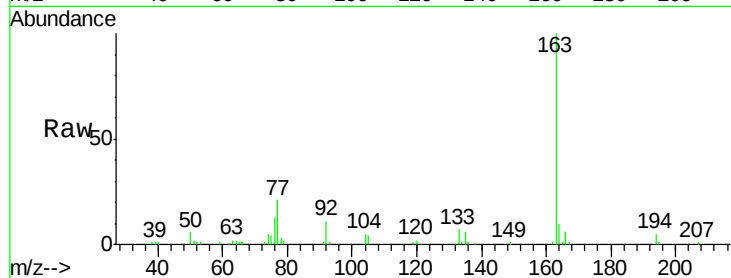

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

