

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
 Data File : BM019777.D
 Acq On : 06 Apr 2019 07:59
 Operator : JU/SJ
 Sample : K2217-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF615

Manual Integrations
 APPROVED

Sohil
 4/8/2019 6:11:54 PM

Quant Time: Apr 08 03:25:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 06 00:13:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	164448	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	787181	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	484956	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	1091819	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	1103553	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	997259	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	17153	4.08	ng/uL	0.00
5) Phenol-d5	6.75	99	215756	14.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	137962	14.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	169268	15.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	172770	15.72	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	83125	14.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	98094	15.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	172897	14.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	217466	15.36	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	617659	15.78	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	736884	15.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	70432m	11.48	ng/ul	0.01
58) Fluorene-d10	15.22	176	532633	15.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	69498	9.63	ng/ul	0.00
71) Anthracene-d10	17.08	188	808935	15.44	ng/ul	0.00
79) Pyrene-d10	19.39	212	861634	16.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	710866	13.45	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	108615	2.766	ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
Data File : BM019777.D
Acq On : 06 Apr 2019 07:59
Operator : JU/SJ
Sample : K2217-04
Misc :
ALS Vial : 37 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF615

Quant Time: Apr 08 03:25:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 06 00:13:11 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/8/2019 6:11:54 PM

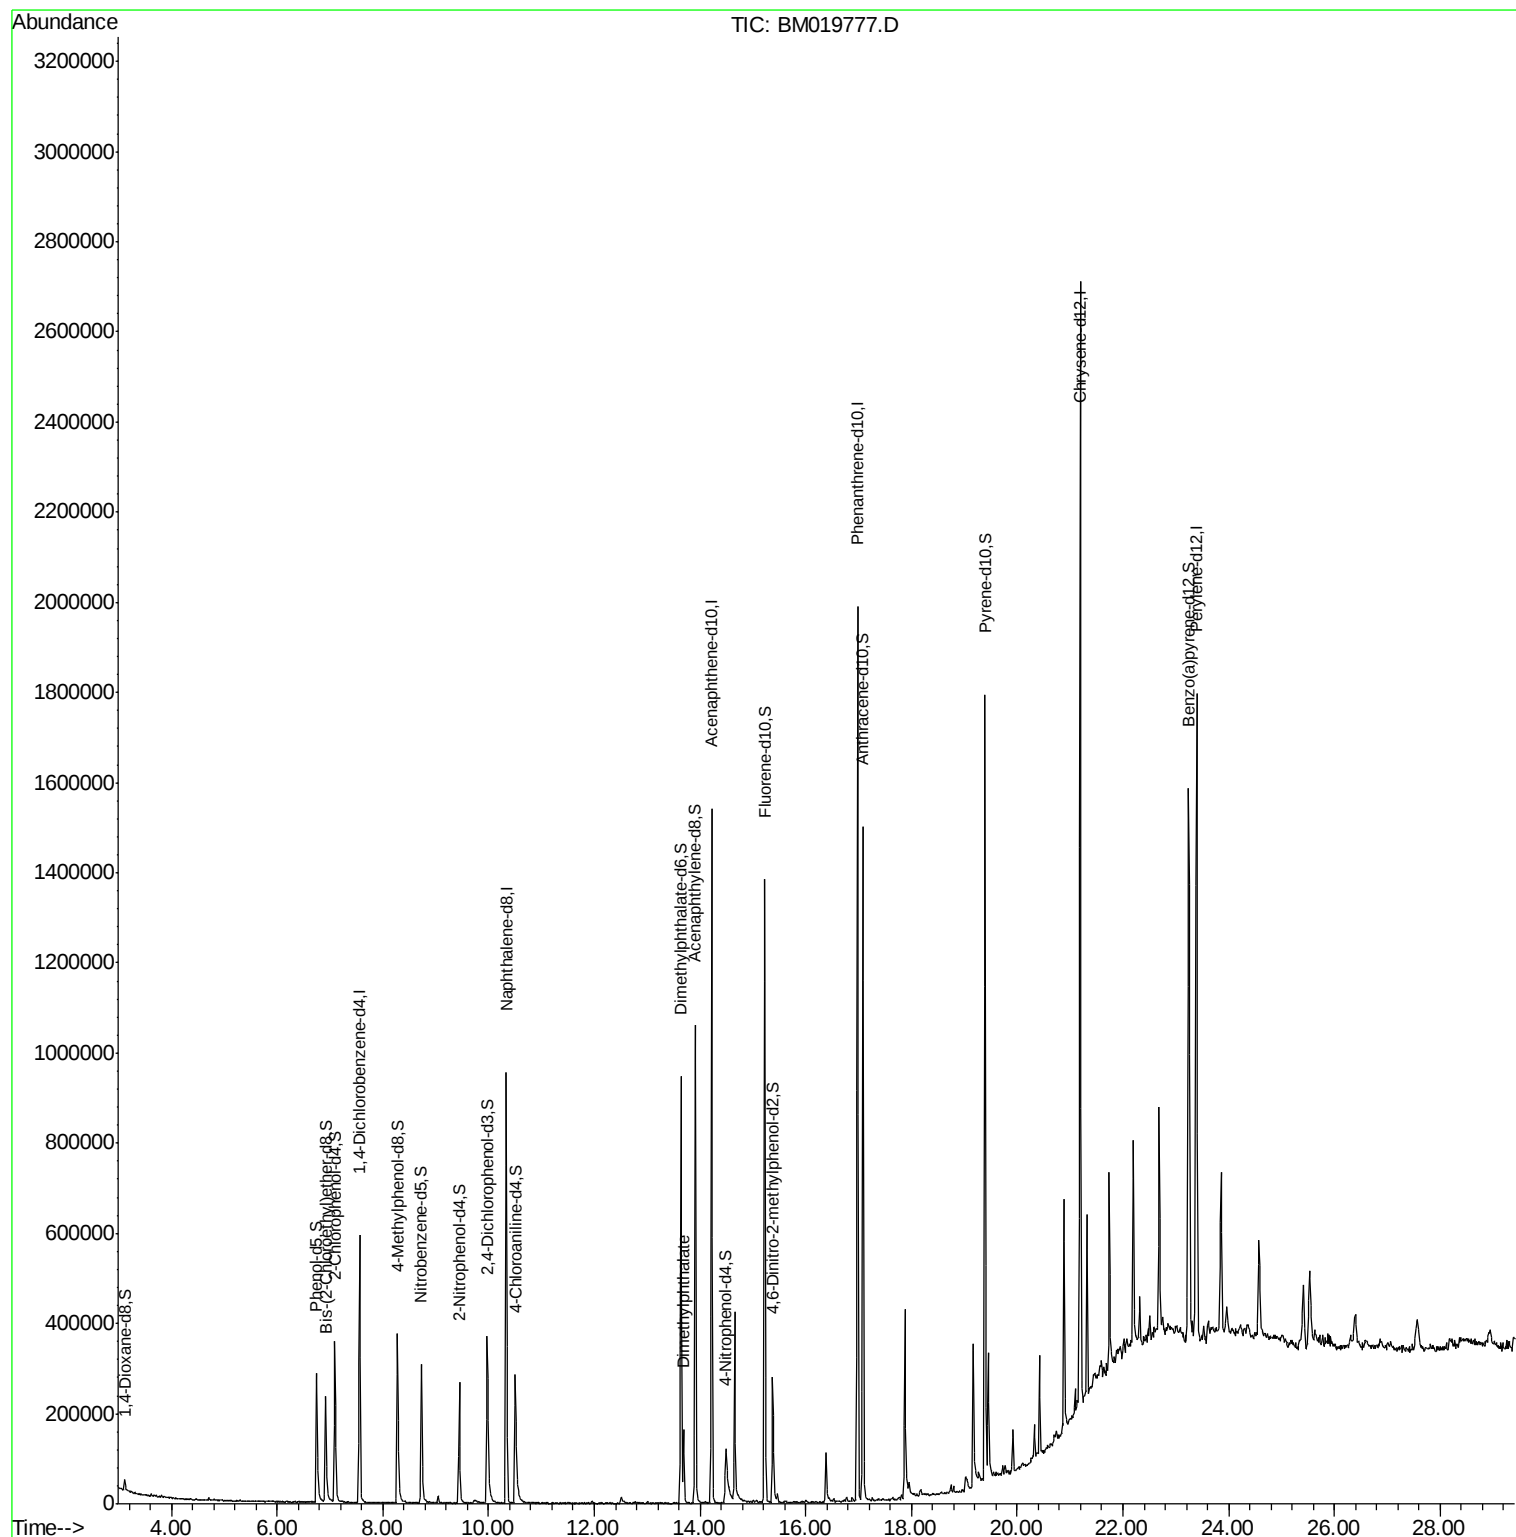

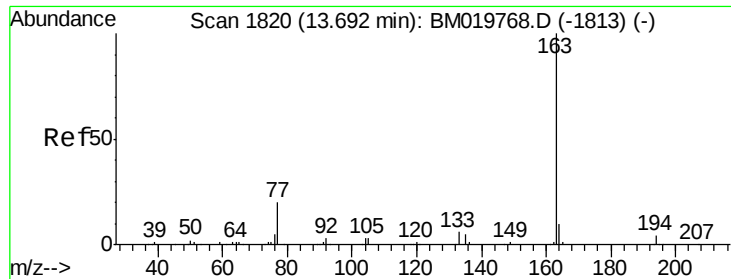

#45
 Dimethylphthalate
 Concen: 2.766 ng/ul
 RT: 13.69 min Scan# 1820
 Delta R.T. 0.00 min
 Lab File: BM019777.D
 Acq: 06 Apr 2019 07:59

Instrument :
 BNA_M
 ClientSampleId :
 BF615

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	3.6	4.0	6.0#
164	10.1	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/8/2019 6:11:54 PM

