

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
 Data File : BM019782.D
 Acq On : 06 Apr 2019 10:59
 Operator : JU/SJ
 Sample : K2217-10
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF630

Manual Integrations
 APPROVED

Sohil
 4/8/2019 6:12:04 PM

Quant Time: Apr 08 03:40:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 06 00:13:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	154089	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	691111	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	424694	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	995892	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	962536	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	869035	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	21526	5.47	ng/uL	0.00
5) Phenol-d5	6.75	99	318346	23.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	184223	20.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	249835	24.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	266599	25.88	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	119079	24.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	139994	25.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	252395	24.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	342859	27.58	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	822327	24.00	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	1091266	25.47	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	116822m	21.75	ng/ul	0.00
58) Fluorene-d10	15.22	176	754602	25.56	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	88474	13.43	ng/ul	0.00
71) Anthracene-d10	17.08	188	1229814	25.73	ng/ul	0.00
79) Pyrene-d10	19.39	212	1317760	29.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	1097535	23.82	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	166966	4.856	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
Data File : BM019782.D
Acq On : 06 Apr 2019 10:59
Operator : JU/SJ
Sample : K2217-10
Misc :
ALS Vial : 42 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
BF630

Manual Integrations
APPROVED

Sohil
4/8/2019 6:12:04 PM

Quant Time: Apr 08 03:40:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 06 00:13:11 2019
Response via : Initial Calibration

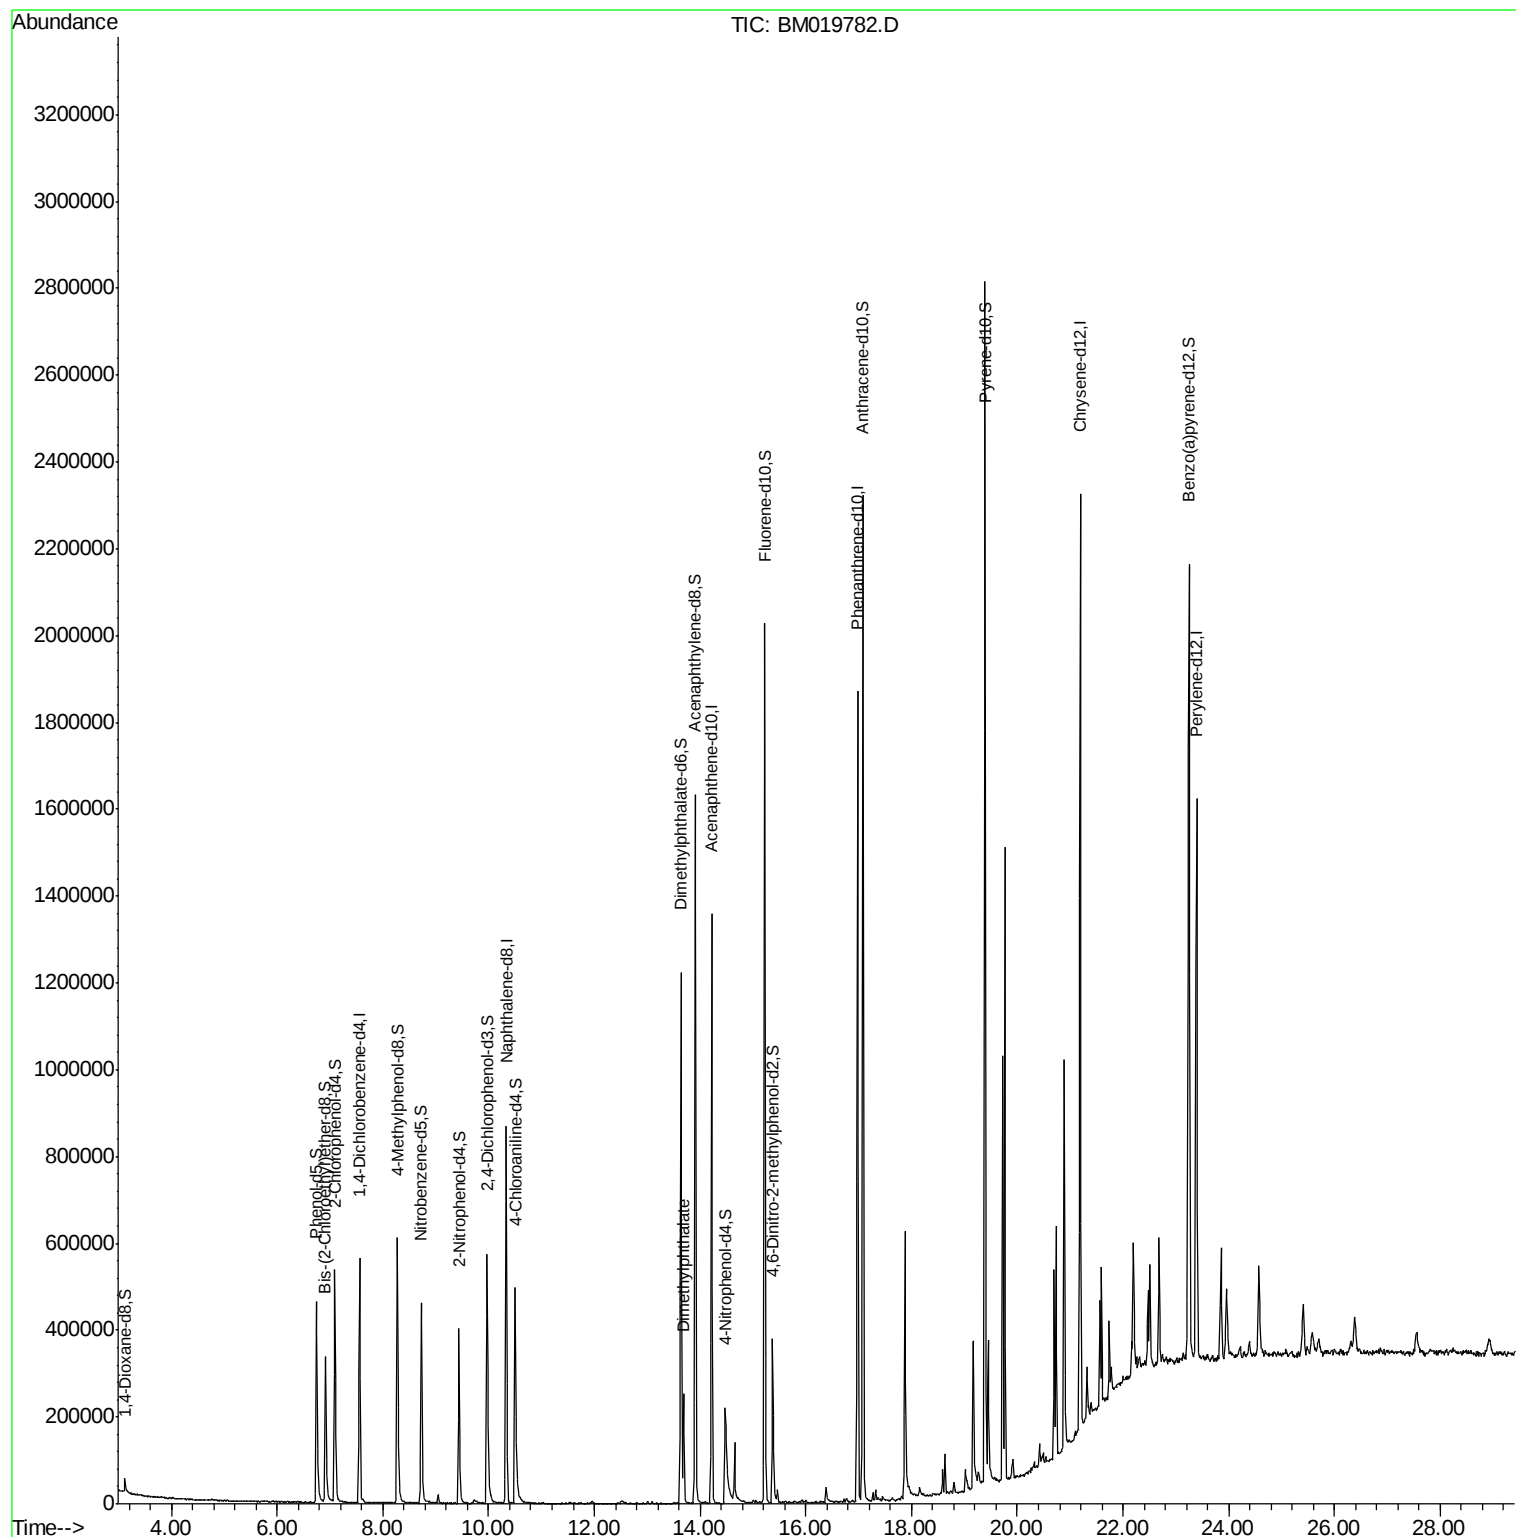

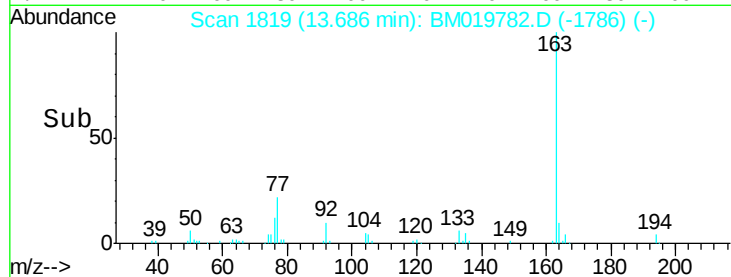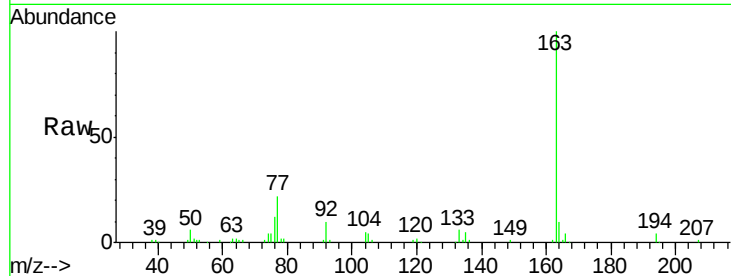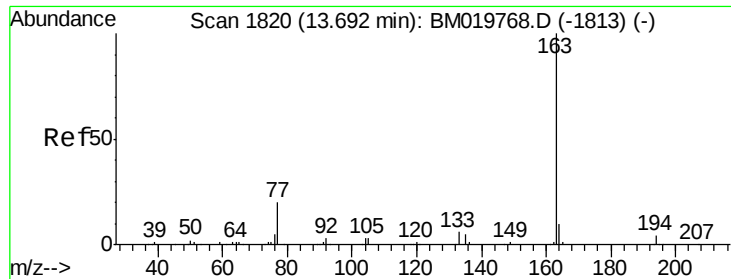

#45

Dimethylphthalate

Concen: 4.856 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BM019782.D

Acq: 06 Apr 2019 10:59

Instrument :

BNA_M

ClientSampleId :

BF630

Tgt	Ion	Ratio	Resp	Lower	Upper
163	100		166966		
194	4.0		4.0	6.0	
164	9.7		8.4	12.6	

Manual Integrations
APPROVED

Sohil
4/8/2019 6:12:04 PM

