

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040519\
 Data File : BM019767.D
 Acq On : 06 Apr 2019 01:59
 Operator : JU/SJ
 Sample : K2269-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BR6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	20	22	28	rVB	17529	24965	0.56%	0.059%
2	4.904	320	326	341	rBV	433130	678396	15.14%	1.592%
3	6.751	635	640	655	rBV	107256	227305	5.07%	0.533%
4	6.916	662	668	692	rBV	423621	795439	17.75%	1.867%
5	7.092	692	698	714	rVB	522227	901776	20.12%	2.116%
6	7.445	753	758	766	rVB	33187	51014	1.14%	0.120%
7	7.557	771	777	781	rVV	602260	1002562	22.37%	2.353%
8	7.592	781	783	795	rVB	298245	421485	9.40%	0.989%
9	7.904	827	836	848	rBV	342061	568271	12.68%	1.334%
10	8.275	894	899	918	rBV	374155	719813	16.06%	1.689%
11	8.728	970	976	996	rBV	583002	1065433	23.77%	2.500%
12	9.051	1027	1031	1037	rVB	25148	35686	0.80%	0.084%
13	9.439	1090	1097	1113	rBV	519134	933751	20.83%	2.191%
14	9.975	1181	1188	1210	rBV	583131	1391371	31.05%	3.265%
15	10.116	1210	1212	1215	rVV3	9548	11724	0.26%	0.028%
16	10.145	1215	1217	1221	rVV2	5020	6364	0.14%	0.015%
17	10.204	1221	1227	1235	rVB	90685	151737	3.39%	0.356%
18	10.339	1242	1250	1259	rBV	910689	1547357	34.53%	3.631%
19	10.551	1280	1286	1293	rBV5	13893	39541	0.88%	0.093%
20	10.722	1310	1315	1323	rVB3	19800	34650	0.77%	0.081%
21	11.539	1448	1454	1459	rBV	28877	41913	0.94%	0.098%
22	11.969	1522	1527	1536	rVB2	6215	15111	0.34%	0.035%
23	13.016	1701	1705	1710	rBV3	3091	4877	0.11%	0.011%
24	13.574	1795	1800	1802	rVB	5168	5963	0.13%	0.014%
25	13.645	1805	1812	1829	rBV	1516281	2193996	48.95%	5.149%
26	13.910	1851	1857	1872	rBV	1884206	2808336	62.66%	6.590%
27	14.221	1903	1910	1925	rBV2	1511667	2219791	49.53%	5.209%
28	14.515	1955	1960	1968	rBV5	24010	75057	1.67%	0.176%
29	15.221	2074	2080	2093	rBV	2344672	3467476	77.37%	8.137%
30	15.380	2101	2107	2118	rBV	561590	905075	20.19%	2.124%
31	15.468	2118	2122	2130	rVB2	30171	46724	1.04%	0.110%
32	16.015	2211	2215	2218	rBV3	6415	8824	0.20%	0.021%
33	16.774	2340	2344	2351	rVB2	6347	9425	0.21%	0.022%
34	16.980	2373	2379	2390	rBV2	1937349	2617099	58.39%	6.142%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040519\
Data File : BM019767.D
Acq On : 06 Apr 2019 01:59
Operator : JU/SJ
Sample : K2269-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BR6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Title : SVOA CALIBRATION

35	17.080	2390	2396	2415	rVB	2764984	4048650	90.34%	9.501%
36	17.880	2526	2532	2537	rBV3	10830	18863	0.42%	0.044%
37	19.027	2723	2727	2732	rBV2	23042	30386	0.68%	0.071%
38	19.174	2747	2752	2755	rBV5	8756	14579	0.33%	0.034%
39	19.274	2766	2769	2777	rVB	18817	24901	0.56%	0.058%
40	19.392	2783	2789	2798	rBV	3488998	4481729	100.00%	10.517%
41	21.192	3090	3095	3106	rBV	1873918	2553386	56.97%	5.992%
42	21.750	3187	3190	3193	rVB2	54894	61217	1.37%	0.144%
43	22.197	3263	3266	3271	rVB2	91544	110315	2.46%	0.259%
44	22.686	3346	3349	3354	rVB	134950	171501	3.83%	0.402%
45	23.250	3438	3445	3456	rVB	2033284	3612765	80.61%	8.478%
46	23.391	3462	3469	3483	rVB	1190686	2285715	51.00%	5.364%
47	23.856	3545	3548	3554	rVB2	111581	170431	3.80%	0.400%


Sum of corrected areas: 42612745

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040519\
Data File : BM019767.D
Acq On : 06 Apr 2019 01:59
Operator : JU/SJ
Sample : K2269-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BR6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

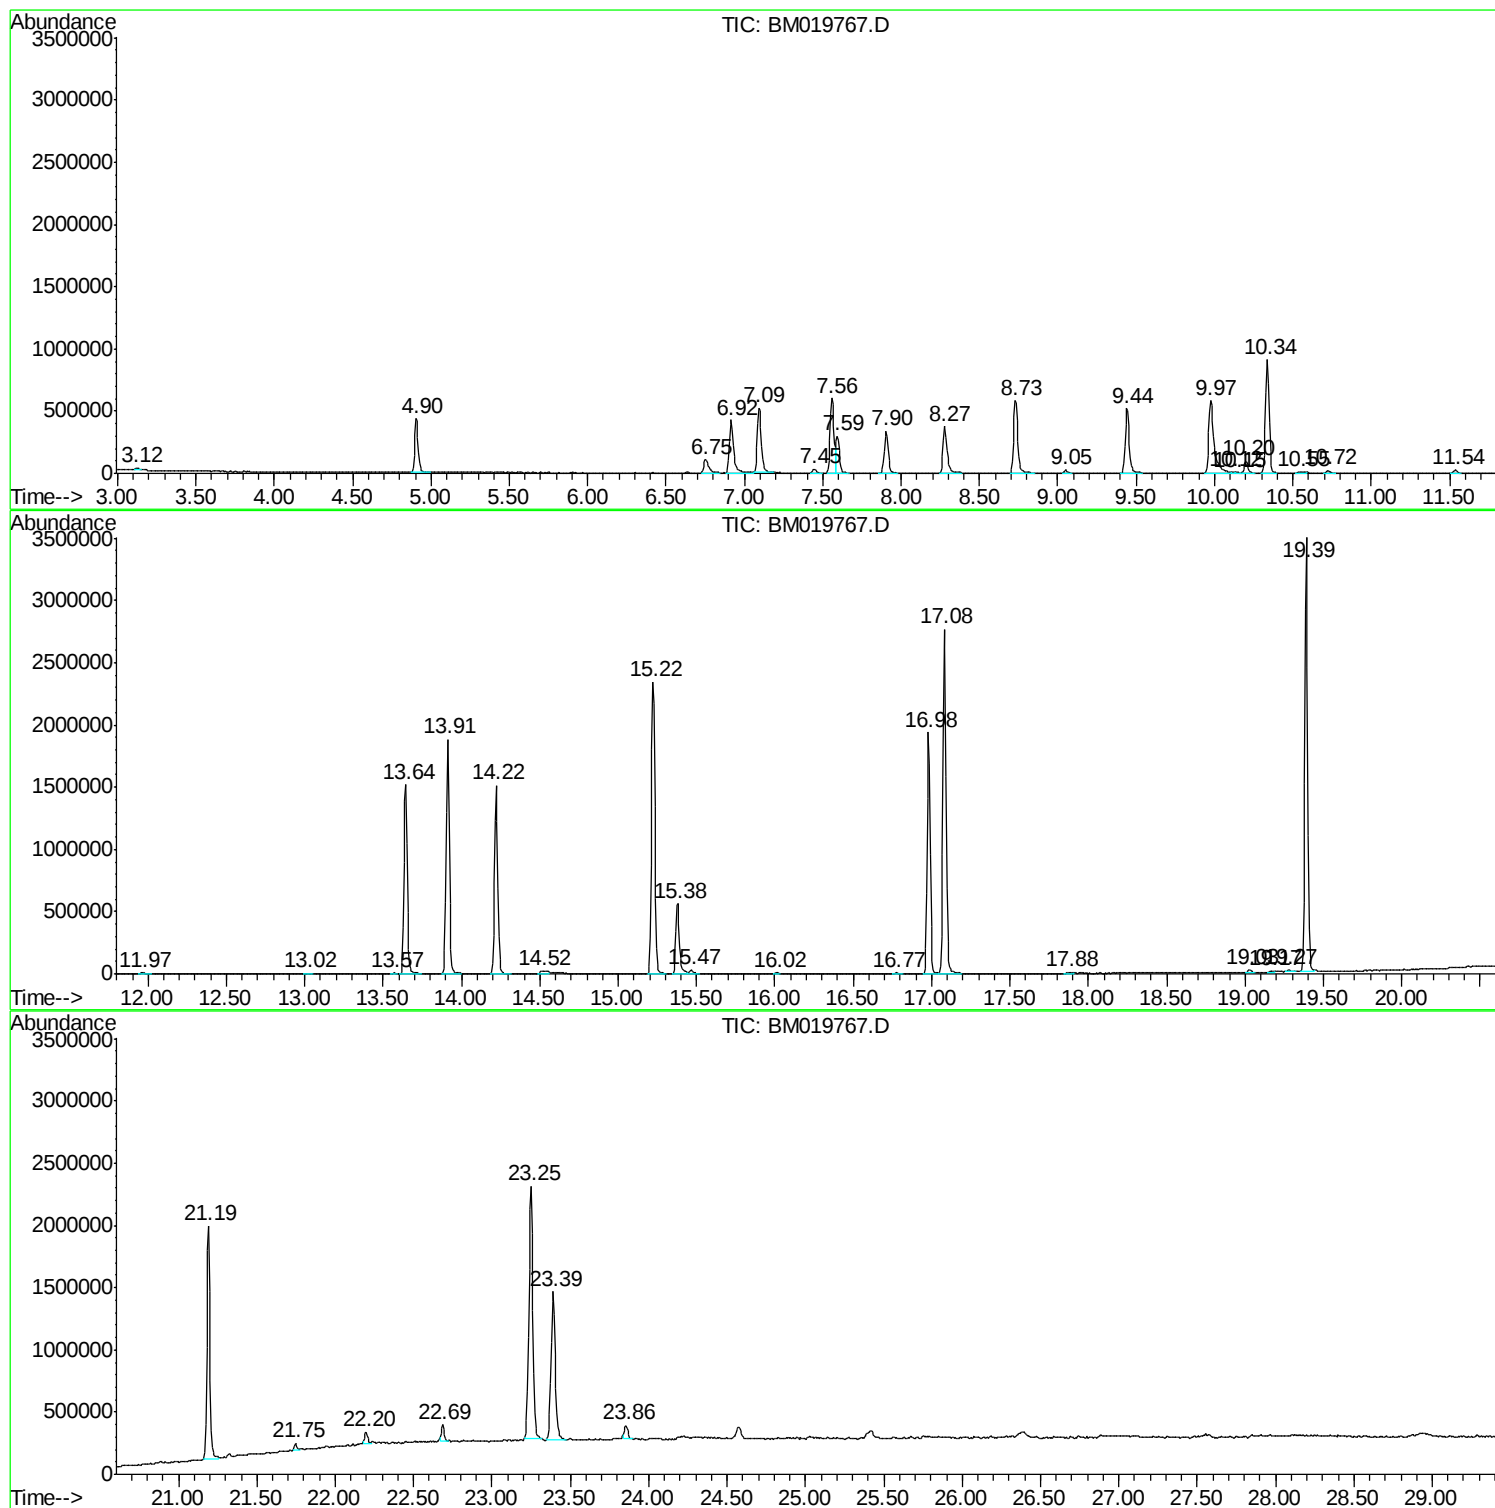

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
Data File : BM019767.D
Acq On : 06 Apr 2019 01:59
Operator : JU/SJ
Sample : K2269-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BR6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040519\
Data File : BM019767.D
Acq On : 06 Apr 2019 01:59
Operator : JU/SJ
Sample : K2269-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BR6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc