


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040521\
Data File : BM029346.D
Acq On : 05 Apr 2021 17:45
Operator : CG/JU
Sample : M1818-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Manual Integrations
APPROVED

mohammad
4/6/2021 3:23:30 PM

Quant Time: Apr 05 18:18:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 05 15:51:17 2021
Response via : Initial Calibration

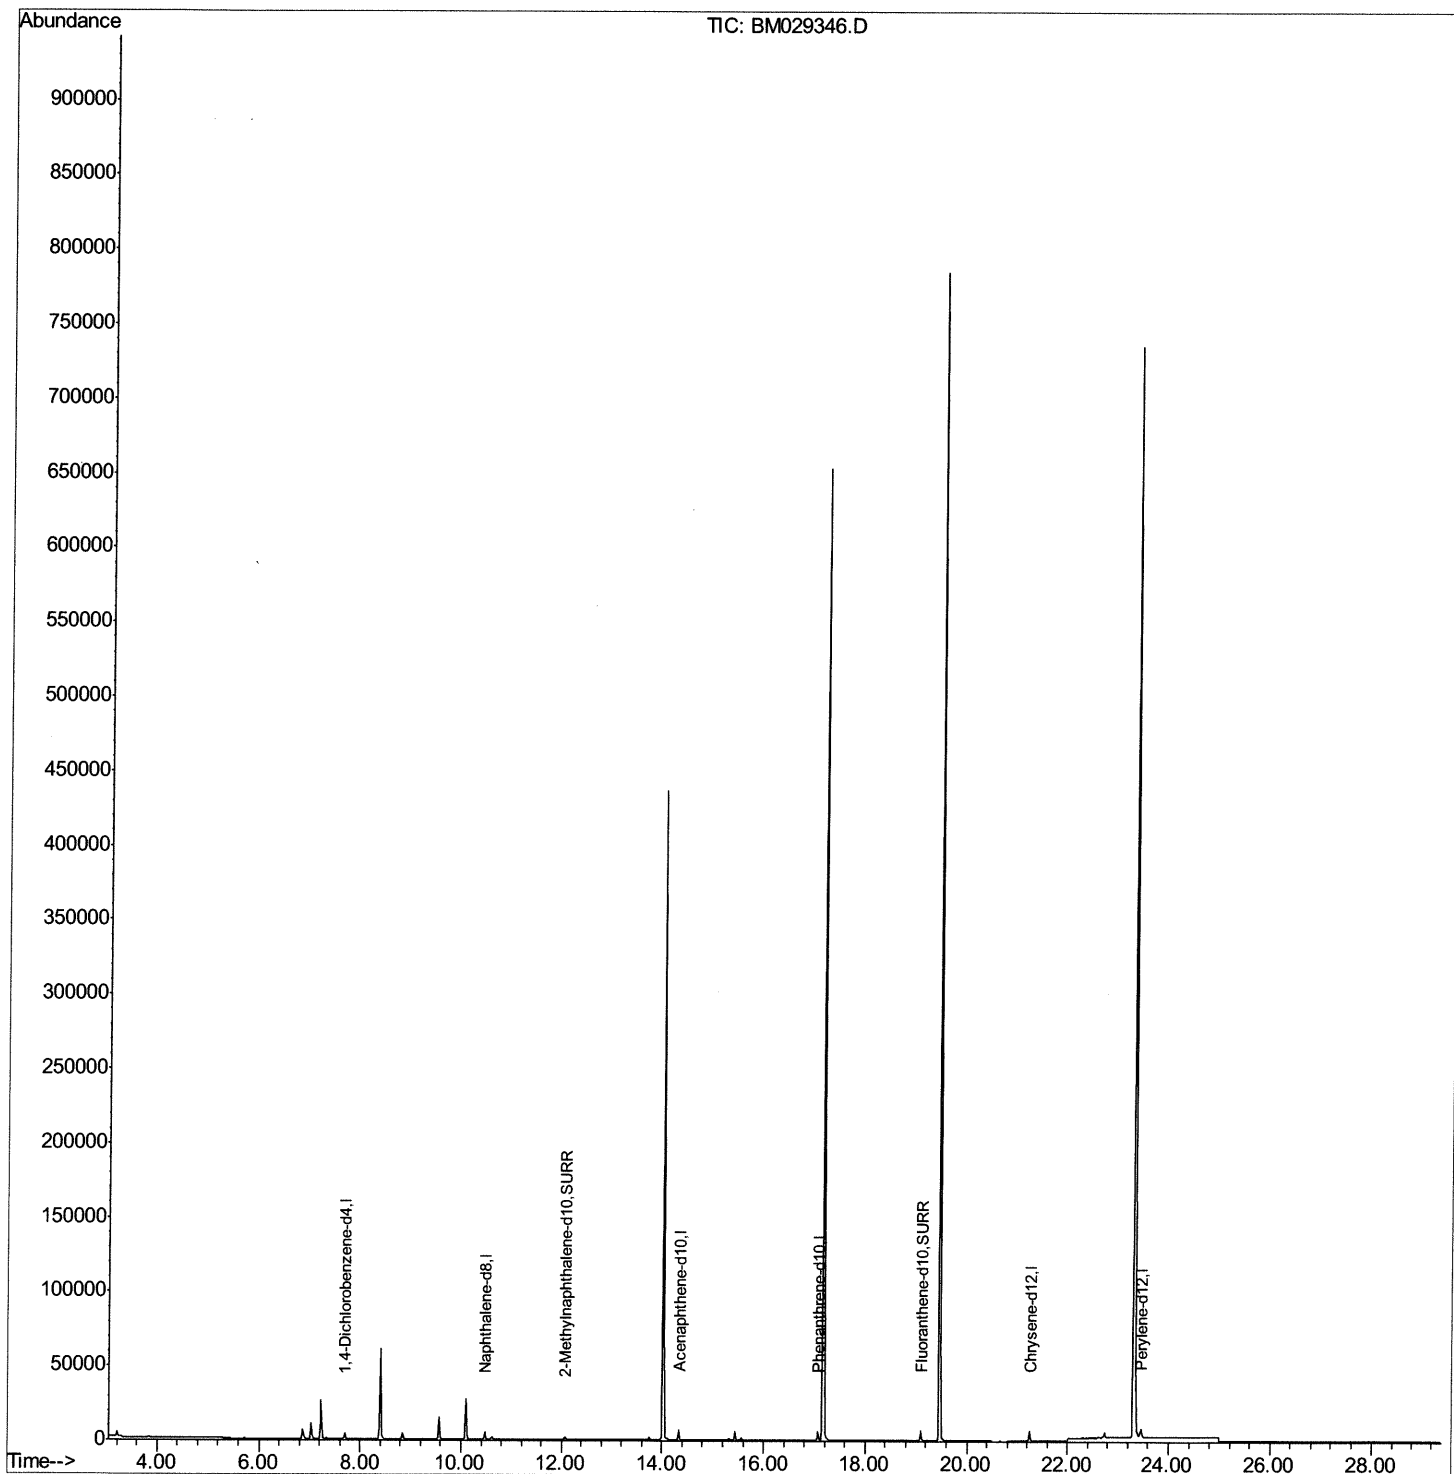

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040521\
 Data File : BM029346.D
 Acq On : 05 Apr 2021 17:45
 Operator : CG/JU
 Sample : M1818-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA0

Manual Integrations
 APPROVED

mohammad
 4/6/2021 3:23:30 PM

Quant Time: Apr 05 18:16:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 05 15:51:17 2021
 Response via : Initial Calibration

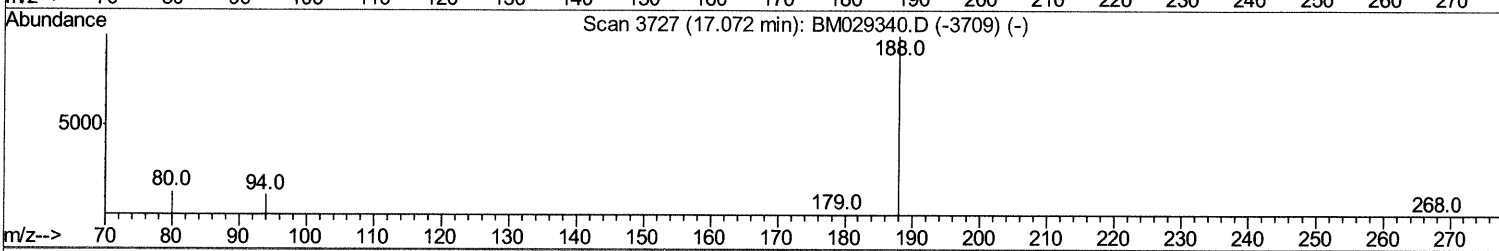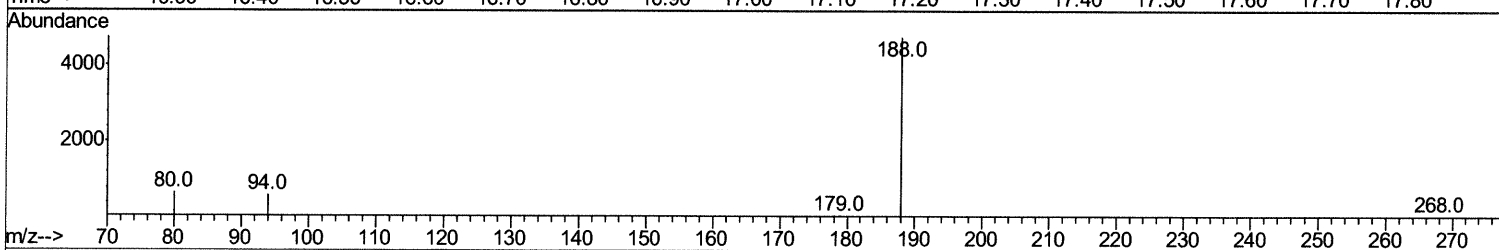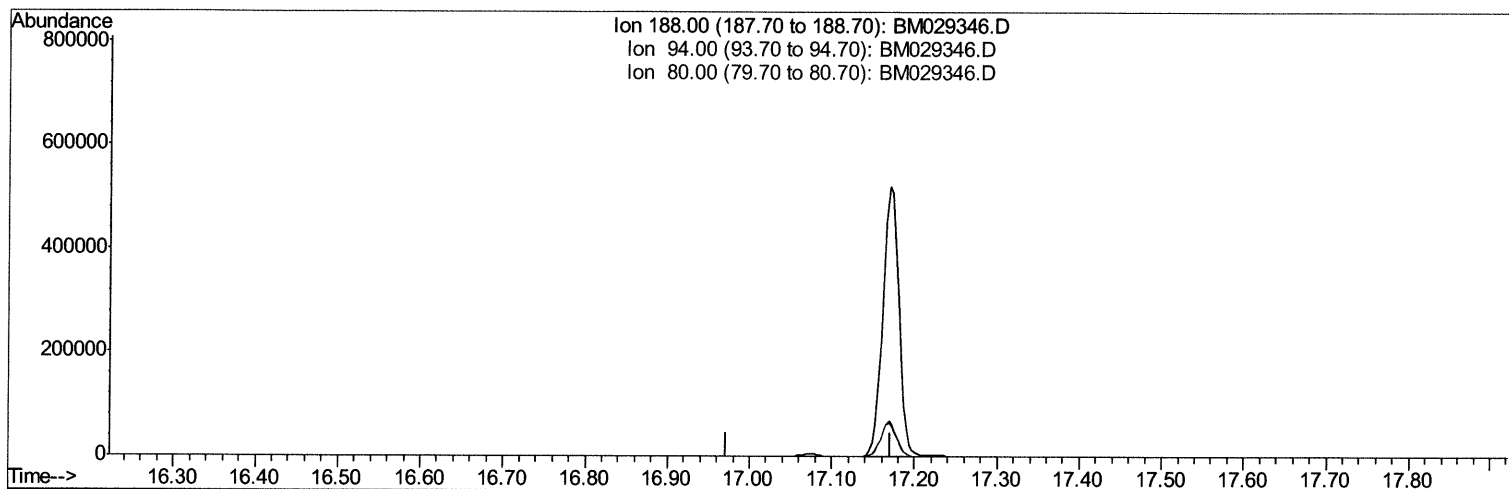

TIC: BM029346.D

(10) Phenanthrene-d10 (I)

17.072min (-17.072) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.30	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040521\
Data File : BM029346.D
Acq On : 05 Apr 2021 17:45
Operator : CG/JU
Sample : M1818-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Manual Integrations
APPROVED

mohammad
4/6/2021 3:23:30 PM

Quant Time: Apr 05 18:16:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 05 15:51:17 2021
Response via : Initial Calibration

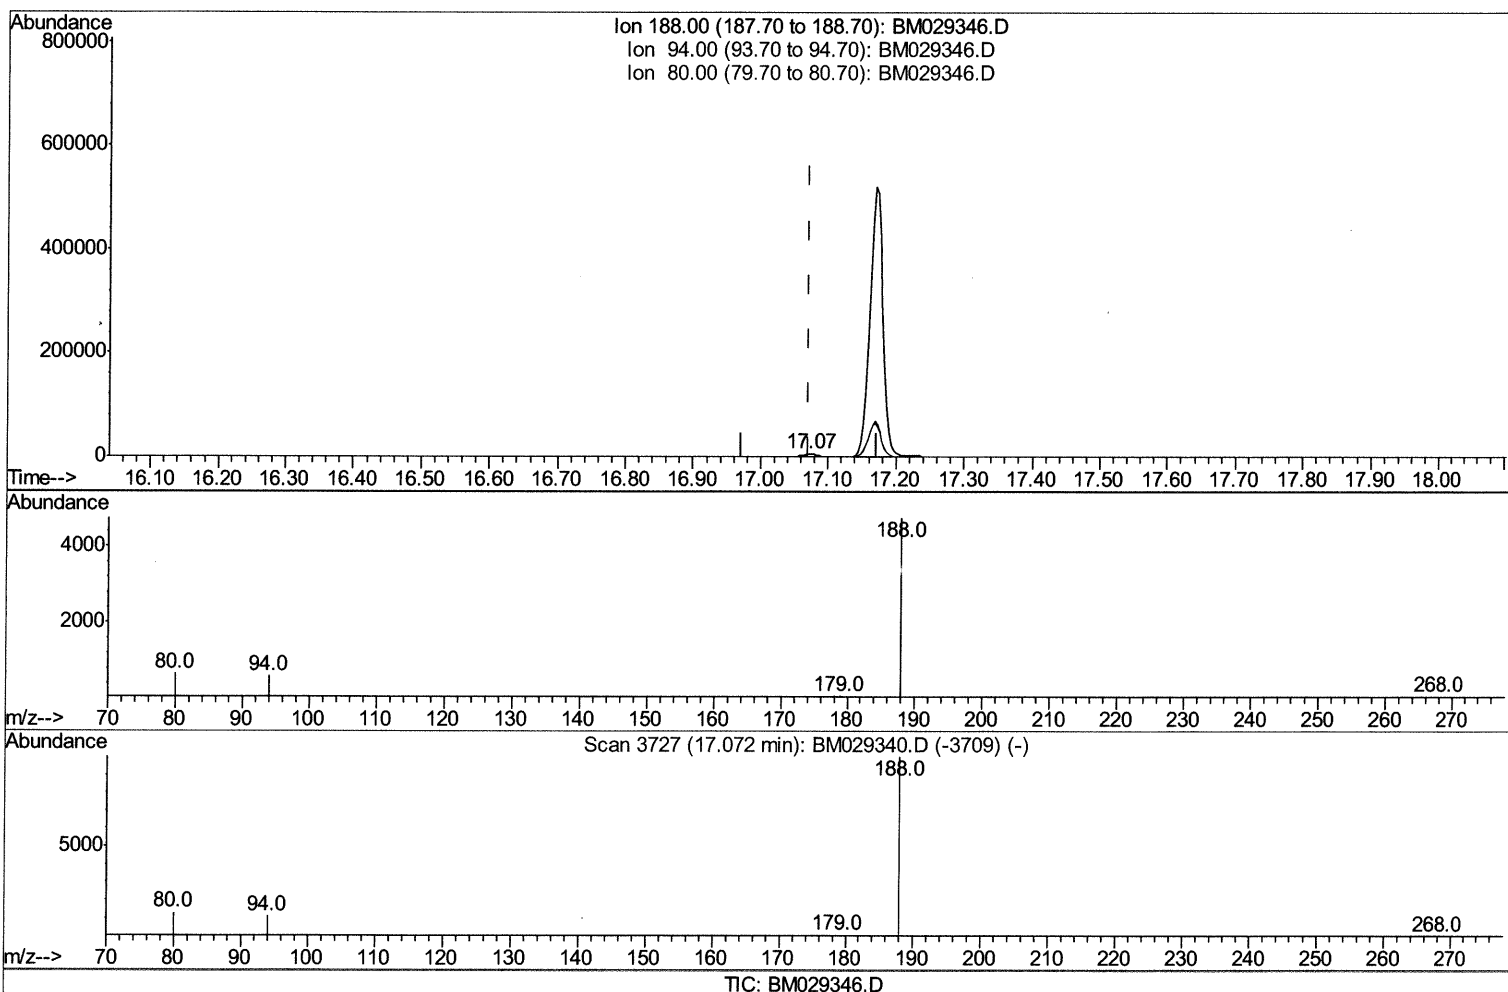

(10) Phenanthrene-d10 (I)

17.072min (0.000) 0.40ng/ul m 04/07/21 JU

response 6729

Ion	Exp%	Act%
188.00	100	100
94.00	12.30	12.51
80.00	13.70	13.78
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040521\
 Data File : BM029346.D
 Acq On : 05 Apr 2021 17:45
 Operator : CG/JU
 Sample : M1818-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA0

Manual Integrations
 APPROVED

mohammad
 4/6/2021 3:23:30 PM

Quant Time: Apr 05 18:18:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 05 15:51:17 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	1790	0.40	ng/ul	0.00
2) Naphthalene-d8	10.48	136	6021	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.33	164	3532	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	6729m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.25	240	6527	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	8292	0.40	ng/ul	0.00

04/07/2021

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.07	152	3036	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.10	212	7154	0.42	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed