


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040521\
Data File : BM029347.D
Acq On : 05 Apr 2021 18:22
Operator : CG/JU
Sample : M1818-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

mohammad
4/6/2021 3:23:32 PM

Quant Time: Apr 06 03:37:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 05 15:51:17 2021
Response via : Initial Calibration

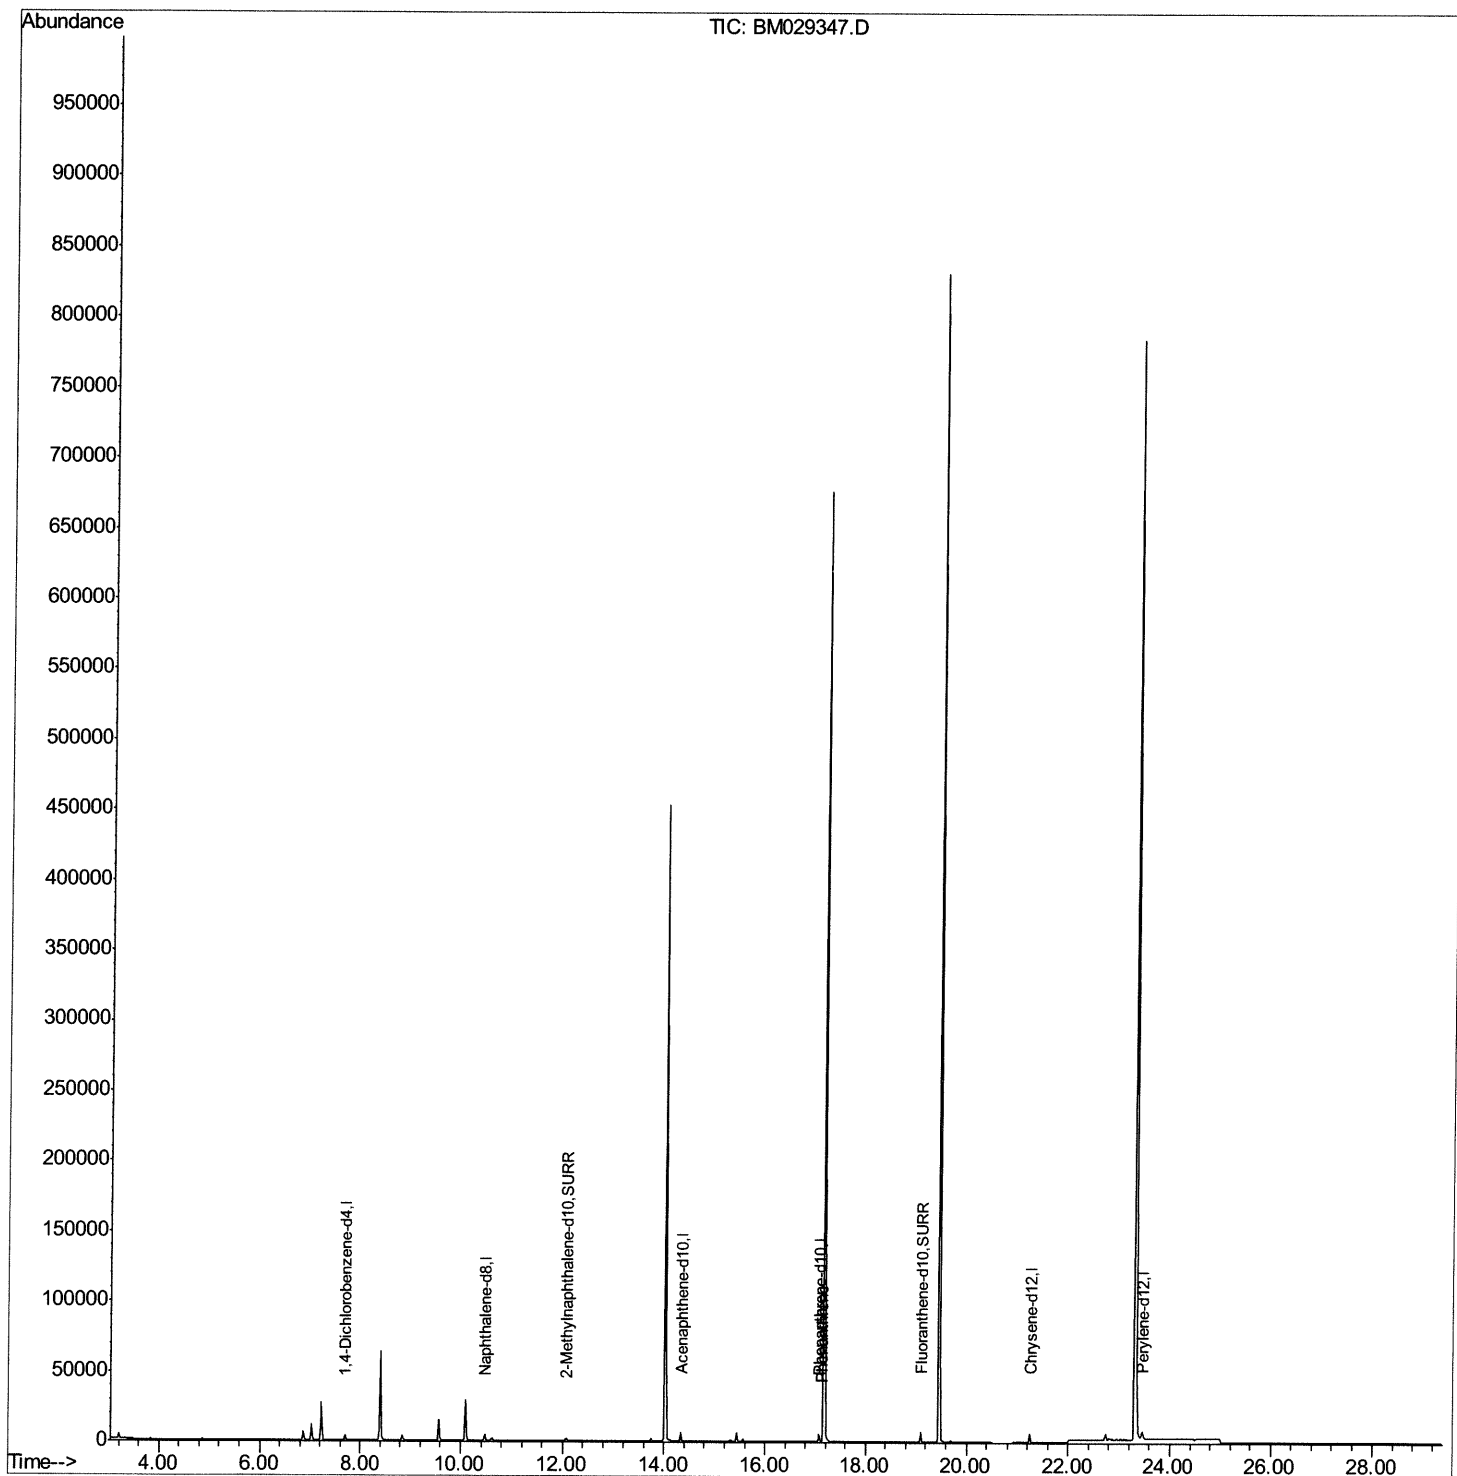

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040521\
 Data File : BM029347.D
 Acq On : 05 Apr 2021 18:22
 Operator : CG/JU
 Sample : M1818-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 C0AA1

Manual Integrations
APPROVED

mohammad
 4/6/2021 3:23:32 PM

Quant Time: Apr 06 03:31:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 05 15:51:17 2021
 Response via : Initial Calibration

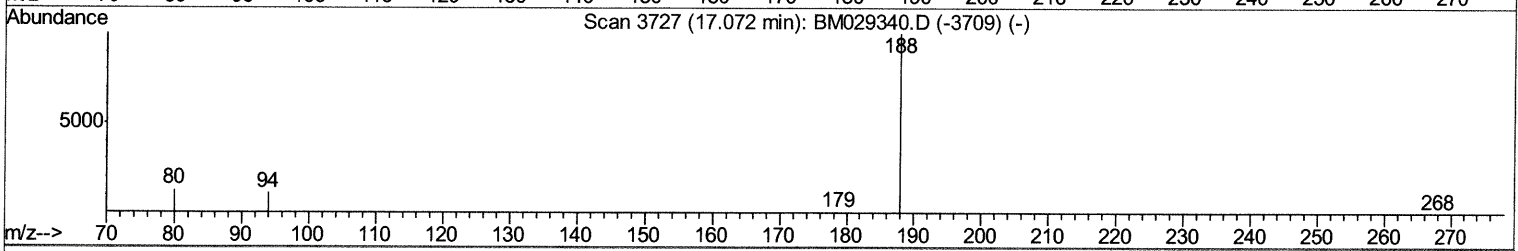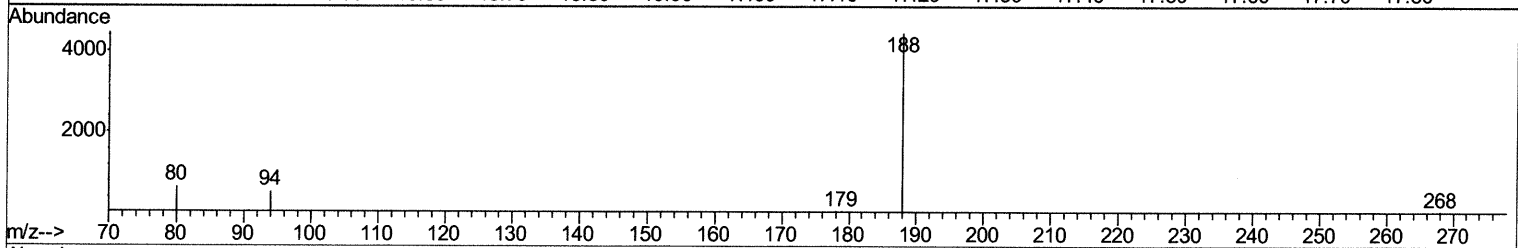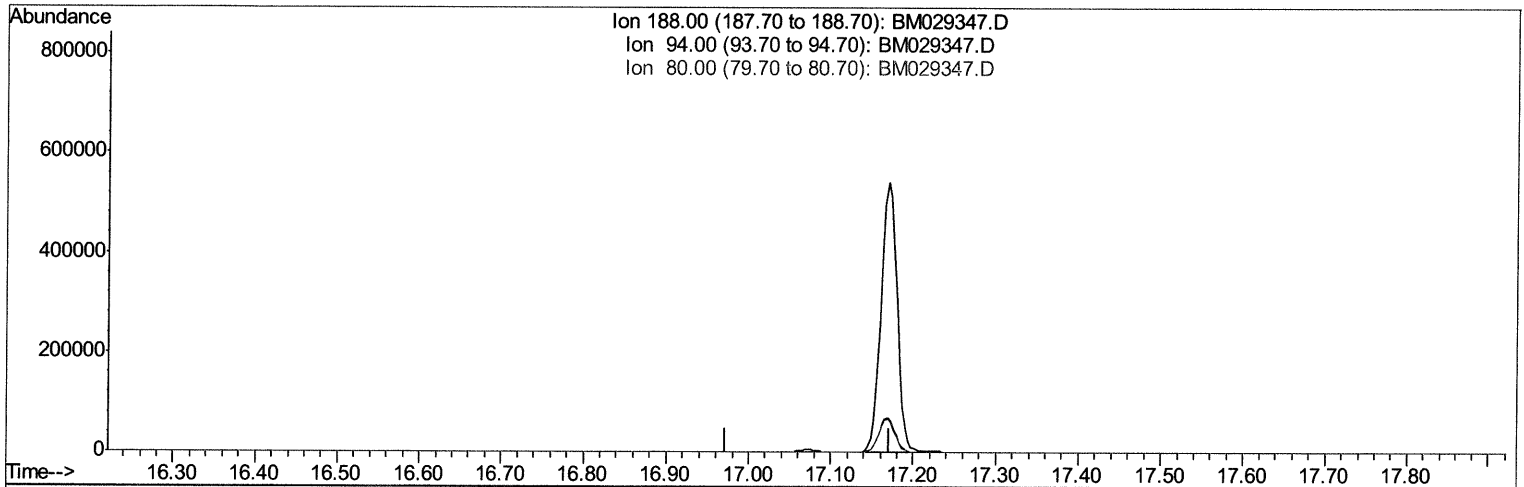

TIC: BM029347.D

(10) Phenanthrene-d10 (I)

17.072min (-17.072) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.30	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040521\
 Data File : BM029347.D
 Acq On : 05 Apr 2021 18:22
 Operator : CG/JU
 Sample : M1818-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

mohammad
 4/6/2021 3:23:32 PM

Quant Time: Apr 06 03:31:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 05 15:51:17 2021
 Response via : Initial Calibration

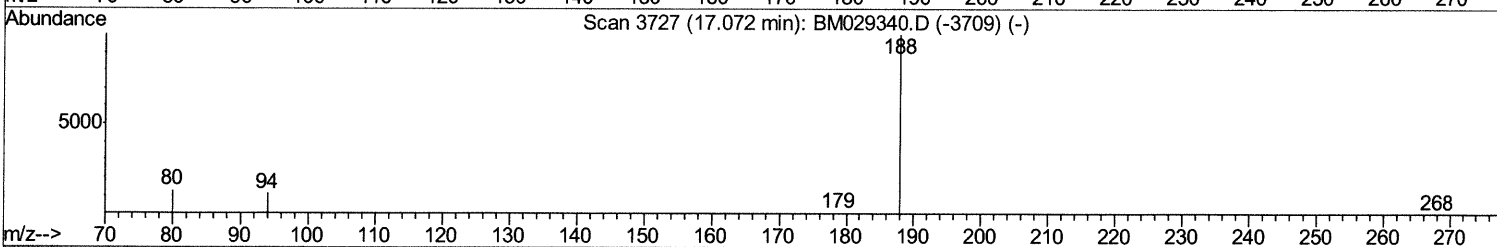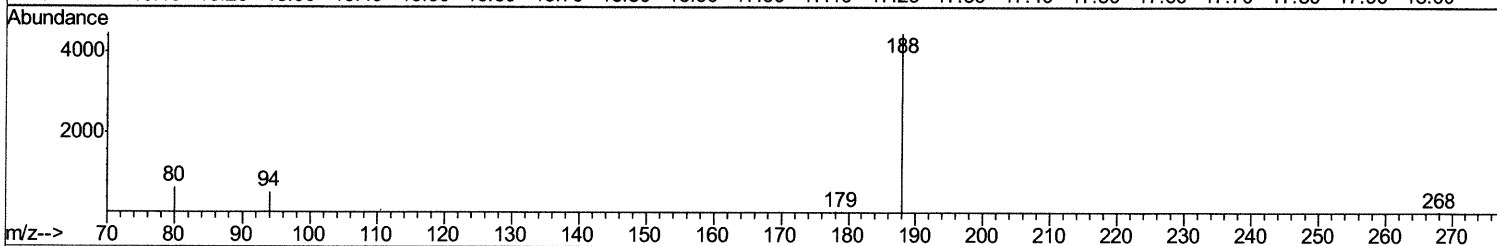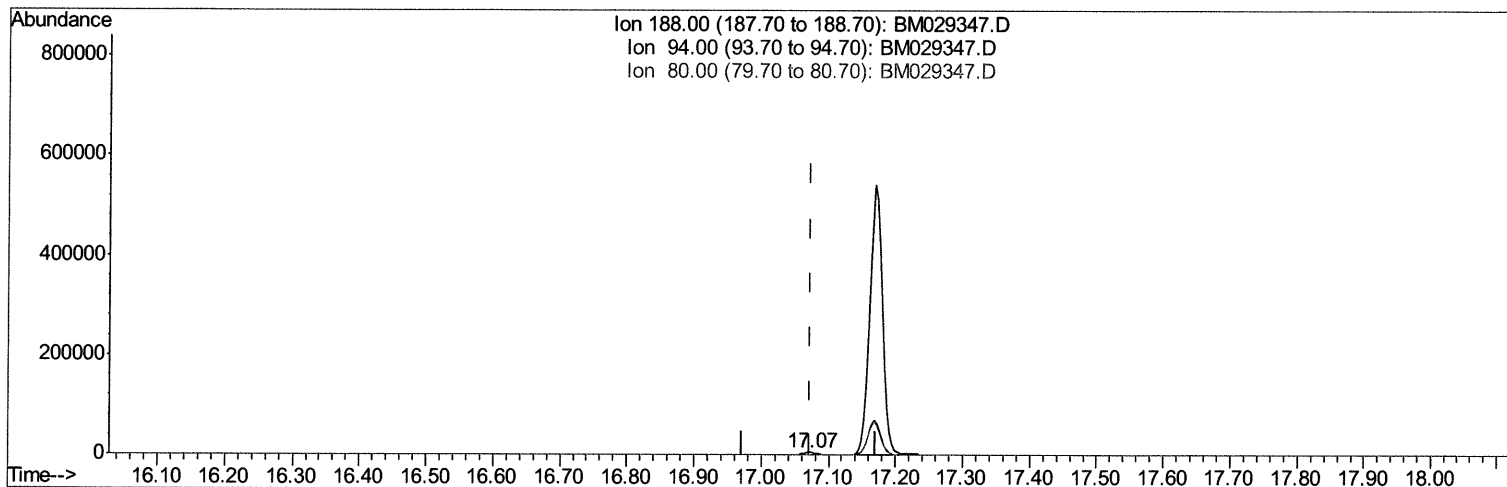

TIC: BM029347.D

(10) Phenanthrene-d10 (I)

17.072min (-0.000) 0.40ng/ul m 04/07/2021

response 6115

Ion	Exp%	Act%
188.00	100	100
94.00	12.30	12.15
80.00	13.70	14.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040521\
 Data File : BM029347.D
 Acq On : 05 Apr 2021 18:22
 Operator : CG/JU
 Sample : M1818-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

mohammad
 4/6/2021 3:23:32 PM

Quant Time: Apr 06 03:37:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 05 15:51:17 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	1661	0.40	ng/ul	0.00
2) Naphthalene-d8	10.48	136	5567	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.33	164	3288	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	6115m>	0.40	ng/ul>	0.0004167/2150
16) Chrysene-d12	21.25	240	6202	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	7838	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.07	152	3167	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.10	212	7588	0.49	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.11	178	383	0.021	ng/ul#	Ovalue 57

(#) = qualifier out of range (m) = manual integration (+) = signals summed