

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040616\
 Data File : BM004902.D
 Acq On : 06 Apr 2016 13:24
 Operator : UM/SJ
 Sample : PB89480BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.981	725	730	740	rBV	184226	280211	16.71%	1.827%
2	7.151	753	759	769	rBV	159701	241941	14.42%	1.577%
3	7.351	787	793	801	rBV	189235	295446	17.61%	1.926%
4	7.822	867	873	881	rBB	204499	326790	19.48%	2.131%
5	8.516	986	991	1001	rBV	233766	370303	22.08%	2.414%
6	8.975	1063	1069	1082	rBB	179037	284389	16.95%	1.854%
7	9.692	1185	1191	1199	rBB	142853	229292	13.67%	1.495%
8	10.227	1276	1282	1296	rBV	222229	365954	21.82%	2.386%
9	10.610	1340	1347	1357	rBV	312652	515252	30.72%	3.359%
10	10.745	1364	1370	1386	rBV	242508	405490	24.17%	2.644%
11	13.863	1894	1900	1910	rVB	497838	687173	40.97%	4.480%
12	14.151	1942	1949	1956	rBV	517670	776367	46.29%	5.062%
13	14.457	1995	2001	2010	rBV2	486485	750742	44.76%	4.895%
14	14.651	2028	2034	2047	rBV	207593	291954	17.41%	1.904%
15	15.451	2164	2170	2179	rVB	719498	1036517	61.80%	6.758%
16	15.568	2184	2190	2198	rBV	204377	278350	16.59%	1.815%
17	17.198	2461	2467	2476	rBV2	672031	981216	58.50%	6.397%
18	17.298	2478	2484	2498	rVB	828024	1177955	70.23%	7.680%
19	19.597	2868	2875	2889	rBV	1065574	1508433	89.93%	9.835%
20	21.386	3174	3179	3189	rBV	1093113	1392209	83.00%	9.077%
21	23.533	3536	3544	3557	rBV2	876149	1677346	100.00%	10.936%
22	23.680	3561	3569	3583	rVB2	707309	1409063	84.01%	9.187%
23	24.203	3654	3658	3664	rVB	13755	24930	1.49%	0.163%
24	24.974	3784	3789	3796	rVB3	15182	30233	1.80%	0.197%


Sum of corrected areas: 15337556

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040616\
Data File : BM004902.D
Acq On : 06 Apr 2016 13:24
Operator : UM/SJ
Sample : PB89480BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK80

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

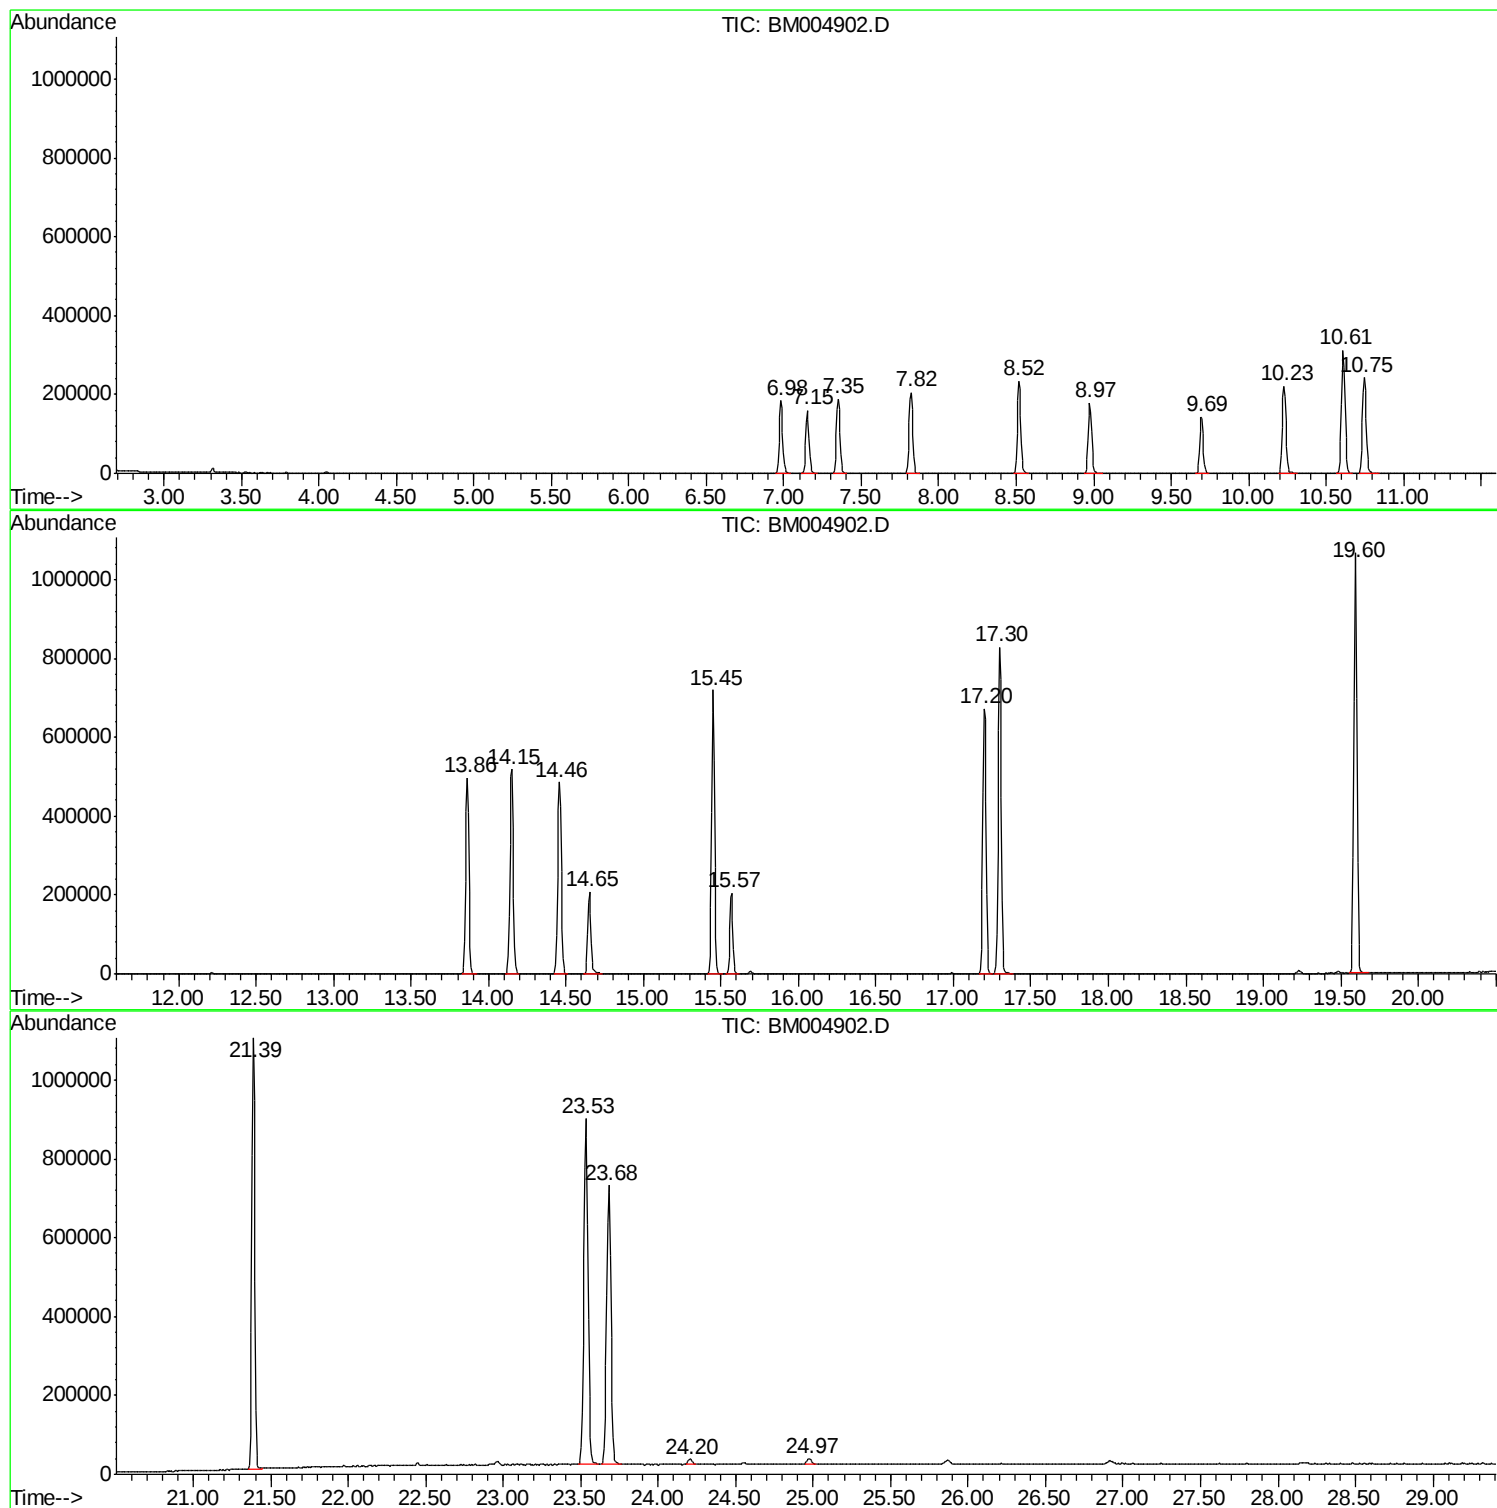

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040616\
Data File : BM004902.D
Acq On : 06 Apr 2016 13:24
Operator : UM/SJ
Sample : PB89480BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK80

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM040616\
Data File : BM004902.D
Acq On : 06 Apr 2016 13:24
Operator : UM/SJ
Sample : PB89480BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK80

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc