


Data Path : Z:\HPCHEM1\BNA M\Data\BM040616\
 Data File : BM004898.D
 Acq On : 06 Apr 2016 10:53
 Operator : UM/SJ
 Sample : DFTPP46
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP46

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM040116.M
 Title : SVOA CALIBRATION
 Last Update : Thu Apr 07 04:29:45 2016

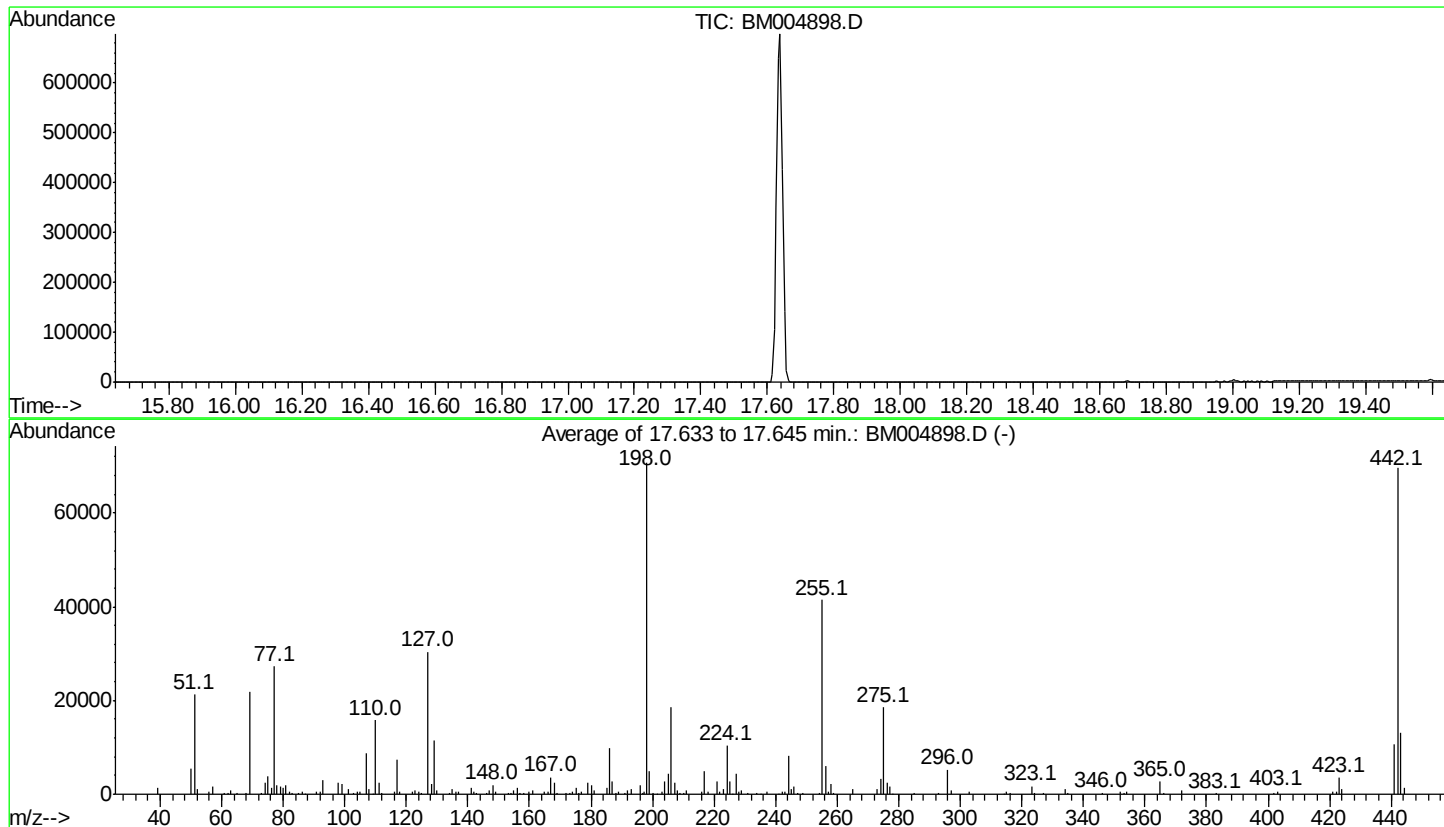

AutoFind: Scans 2541, 2542, 2543; Background Corrected with Scan 2535

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	21264	PASS
68	69	0.00	2	1.3	277	PASS
69	198	0.00	100	30.9	21846	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.0	30402	PASS
197	198	0.00	2	0.6	425	PASS
198	198	100	100	100.0	70728	PASS
199	198	5	9	6.9	4854	PASS
275	198	10	60	26.3	18567	PASS
365	198	1	100	3.7	2642	PASS
441	443	0.01	100	82.2	10683	PASS
442	198	50	100	98.4	69589	PASS
443	442	15	24	18.7	13003	PASS

m/z	Abundance
207.00	450.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z	Abundance
39.10	1808.0
50.10	6703.0
51.10	26400.0
52.00	1389.0
56.00	694.0
57.00	1905.0
61.00	338.0
62.00	407.0
63.00	1223.0
65.00	521.0
68.00	467.0
69.00	26408.0
73.00	354.0
74.10	2730.0
75.00	4696.0
76.00	1689.0
77.10	33456.0
78.00	2370.0
79.00	2013.0
80.00	1646.0
81.00	2214.0
82.00	512.0
83.00	609.0
85.00	393.0
86.00	564.0
87.00	356.0
90.90	454.0
92.00	624.0
93.00	3635.0
98.00	3081.0
99.00	2768.0
101.00	1417.0
103.00	425.0
104.00	800.0
105.00	865.0
107.00	10681.0
108.00	1477.0
110.00	18720.0
111.00	2857.0
112.00	376.0
116.00	564.0
117.00	8764.0
118.00	678.0
122.00	580.0
123.00	1015.0
124.00	474.0
125.00	406.0
127.00	35416.0
128.10	2595.0
129.00	13171.0
130.00	1180.0
133.90	349.0
135.00	1281.0
136.00	545.0
137.00	724.0
141.00	1657.0
142.00	599.0
143.00	452.0
146.10	305.0
147.00	941.0
148.00	2398.0
149.00	531.0
153.00	573.0
154.00	410.0
155.00	1026.0
156.00	1493.0
156.90	340.0
158.00	341.0
160.00	582.0
161.00	826.0
165.00	672.0
166.00	618.0
167.00	4074.0
168.00	2935.0
169.00	579.0
172.00	301.0
173.00	374.0
174.00	760.0
175.10	1534.0
176.00	336.0
177.00	630.0
179.00	2861.0
180.00	2228.0
181.00	969.0
185.10	1309.0
186.10	11282.0
187.10	3263.0
188.00	437.0
189.00	663.0
191.10	422.0
192.00	943.0
193.00	1017.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

196.00	2115.0
197.10	445.0
198.00	78816.0
199.00	5422.0
200.10	398.0
201.50	362.0
203.00	527.0
204.10	2970.0
205.10	4781.0
206.10	20456.0
207.10	2936.0
208.00	858.0
209.00	313.0
210.20	369.0
211.10	808.0
216.00	460.0
217.00	5404.0
218.00	660.0
221.10	2985.0
223.00	1322.0
224.10	11251.0
225.00	2860.0
227.00	4640.0
228.00	716.0
229.00	984.0
231.10	341.0
234.00	319.0
237.00	534.0
242.10	535.0
243.00	560.0
244.10	8563.0
245.00	1151.0
246.00	1727.0
247.00	408.0
249.00	379.0
254.10	355.0
255.10	43664.0
256.10	6784.0
257.00	539.0
258.00	2554.0
259.00	456.0
265.00	982.0
273.10	1270.0
274.10	3500.0
275.10	19360.0
276.10	2735.0
277.00	1766.0
278.00	411.0
285.00	340.0
293.00	395.0
296.00	5547.0
297.00	733.0
303.10	650.0
315.00	664.0
316.00	311.0
323.00	1652.0
324.00	337.0
334.10	1220.0
335.00	311.0
346.00	387.0
352.00	549.0
353.00	330.0
354.10	639.0
365.00	2436.0
366.00	323.0
372.10	993.0
383.10	301.0
402.00	389.0
403.00	513.0
421.00	469.0
422.00	431.0
423.10	3190.0
424.10	1137.0
441.10	9307.0
442.10	61504.0
443.10	12222.0
444.10	1147.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z	Abundance
39.00	1782.0
50.10	6081.0
51.10	24096.0
52.10	1301.0
56.00	661.0
57.00	1671.0
61.00	340.0
62.00	406.0
63.00	1003.0
65.00	542.0
68.00	366.0
69.00	25464.0
73.00	300.0
74.00	2835.0
75.10	4194.0
76.10	1322.0
77.10	31216.0
78.10	2408.0
79.00	1881.0
80.00	1631.0
81.00	1988.0
82.00	538.0
83.00	523.0
85.00	467.0
86.00	690.0
90.90	536.0
92.00	562.0
93.00	3574.0
98.00	2709.0
99.00	2348.0
101.00	1196.0
103.00	428.0
104.00	819.0
105.10	781.0
107.00	10132.0
108.00	1491.0
109.10	301.0
110.00	18480.0
111.00	2692.0
112.00	385.0
116.00	564.0
117.00	8508.0
118.00	696.0
122.00	658.0
123.00	916.0
124.00	470.0
125.00	453.0
127.00	35296.0
128.00	2694.0
129.00	13741.0
130.00	1100.0
133.90	443.0
135.00	1190.0
135.90	480.0
137.00	796.0
141.00	1765.0
142.00	594.0
143.00	455.0
146.00	403.0
147.10	1070.0
148.00	2162.0
149.00	628.0
153.00	623.0
153.90	422.0
155.00	1052.0
156.00	1576.0
157.00	339.0
158.00	339.0
160.00	533.0
161.00	902.0
165.00	753.0
166.00	623.0
167.00	4371.0
168.00	2628.0
169.00	409.0
172.00	436.0
173.00	403.0
174.00	791.0
175.00	1661.0
176.00	369.0
177.00	876.0
179.00	3026.0
180.00	2145.0
181.00	975.0
185.00	1536.0
186.10	11362.0
187.00	3209.0
188.00	311.0
189.00	716.0
191.00	351.0
192.00	838.0
193.10	1242.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

196.10	2397.0
196.80	536.0
197.10	498.0
198.00	83032.0
199.00	5790.0
200.00	414.0
203.00	622.0
204.00	3195.0
205.10	5277.0
206.10	21768.0
207.10	3238.0
208.00	835.0
209.00	348.0
210.20	330.0
211.00	942.0
216.10	488.0
217.00	5642.0
218.00	732.0
221.00	3326.0
221.80	805.0
223.00	1364.0
224.10	12255.0
225.10	3286.0
226.10	333.0
227.00	5152.0
228.00	752.0
229.00	1186.0
231.00	427.0
234.00	312.0
235.00	438.0
237.00	542.0
241.00	312.0
242.00	635.0
243.10	596.0
244.10	9719.0
245.00	1231.0
246.00	1861.0
247.00	414.0
249.00	399.0
254.10	466.0
255.10	49544.0
256.10	6918.0
257.00	610.0
258.10	2519.0
259.00	388.0
265.00	1359.0
273.00	1350.0
274.00	3879.0
275.10	22152.0
276.10	3009.0
277.00	1934.0
285.00	348.0
293.00	491.0
296.00	6159.0
297.00	803.0
303.00	715.0
314.10	439.0
315.00	680.0
316.00	468.0
323.10	2023.0
324.10	368.0
327.00	401.0
334.00	1356.0
335.00	433.0
346.00	497.0
352.10	623.0
353.00	460.0
354.00	791.0
365.00	3219.0
366.00	371.0
372.10	1117.0
383.00	317.0
402.00	477.0
403.00	658.0
421.00	726.0
422.10	698.0
423.10	4278.0
424.10	1322.0
441.10	12688.0
442.10	83232.0
443.10	15428.0
444.10	1491.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z	Abundance
39.00	862.0
50.10	3235.0
51.10	13297.0
52.00	682.0
56.00	319.0
57.00	1047.0
63.00	598.0
69.00	13666.0
74.00	1449.0
75.00	2291.0
76.10	855.0
77.10	17112.0
78.00	1098.0
79.00	1009.0
80.00	791.0
81.00	1334.0
82.00	347.0
85.90	301.0
91.00	319.0
92.00	355.0
93.00	1832.0
98.00	1533.0
99.00	1411.0
101.00	702.0
104.00	446.0
105.00	418.0
107.00	5569.0
108.00	669.0
110.00	10174.0
111.00	1504.0
116.00	326.0
117.00	4920.0
118.00	354.0
122.00	424.0
123.00	480.0
124.00	337.0
127.00	20496.0
128.00	1622.0
129.00	7745.0
130.00	594.0
135.00	734.0
136.00	303.0
136.90	424.0
141.00	1090.0
142.00	337.0
142.90	311.0
147.10	597.0
148.00	1310.0
149.00	325.0
155.00	568.0
156.00	1106.0
160.00	303.0
161.00	667.0
164.90	454.0
166.00	399.0
167.00	2619.0
168.00	1641.0
174.00	514.0
175.10	983.0
177.00	464.0
179.00	1699.0
180.00	1363.0
181.00	569.0
185.00	925.0
186.10	6765.0
187.00	1974.0
189.00	430.0
192.00	640.0
193.00	678.0
196.00	1292.0
197.10	334.0
198.00	50336.0
199.00	3352.0
202.90	360.0
204.10	1858.0
205.10	3006.0
206.10	13688.0
207.10	2370.0
208.00	499.0
211.00	568.0
216.00	312.0
217.00	3348.0
218.00	410.0
221.00	1913.0
221.80	484.0
223.00	920.0
224.10	7576.0
225.10	1958.0
227.00	3450.0
228.00	414.0
229.00	636.0
231.00	314.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

237.00	362.0
242.00	372.0
243.10	428.0
244.10	6434.0
245.10	752.0
246.00	1177.0
254.10	326.0
255.10	31064.0
256.00	4447.0
257.00	445.0
258.00	1881.0
265.00	795.0
273.00	914.0
274.00	2586.0
275.10	14191.0
276.00	1830.0
277.00	1263.0
292.90	331.0
296.00	4278.0
297.00	596.0
303.00	504.0
315.00	441.0
323.10	1563.0
324.00	305.0
327.00	328.0
334.10	925.0
346.00	325.0
352.00	365.0
353.00	395.0
354.00	470.0
365.00	2271.0
372.10	754.0
402.00	353.0
403.10	477.0
421.10	475.0
422.00	419.0
423.10	3119.0
424.10	869.0
441.10	10054.0
442.10	64032.0
443.10	11359.0
444.10	1105.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46