


Data Path : Z:\HPCHEM1\BNA M\DATA\BM040617\
Data File : BM009575.D
Acq On : 06 Apr 2017 01:33
Operator : SJ/MA
Sample : I2524-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB328

Manual Integrations
APPROVED

mohammad
4/6/2017 11:39:34 AM

Quant Time: Apr 06 04:06:57 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM040417-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 06 03:48:05 2017
Response via : Initial Calibration

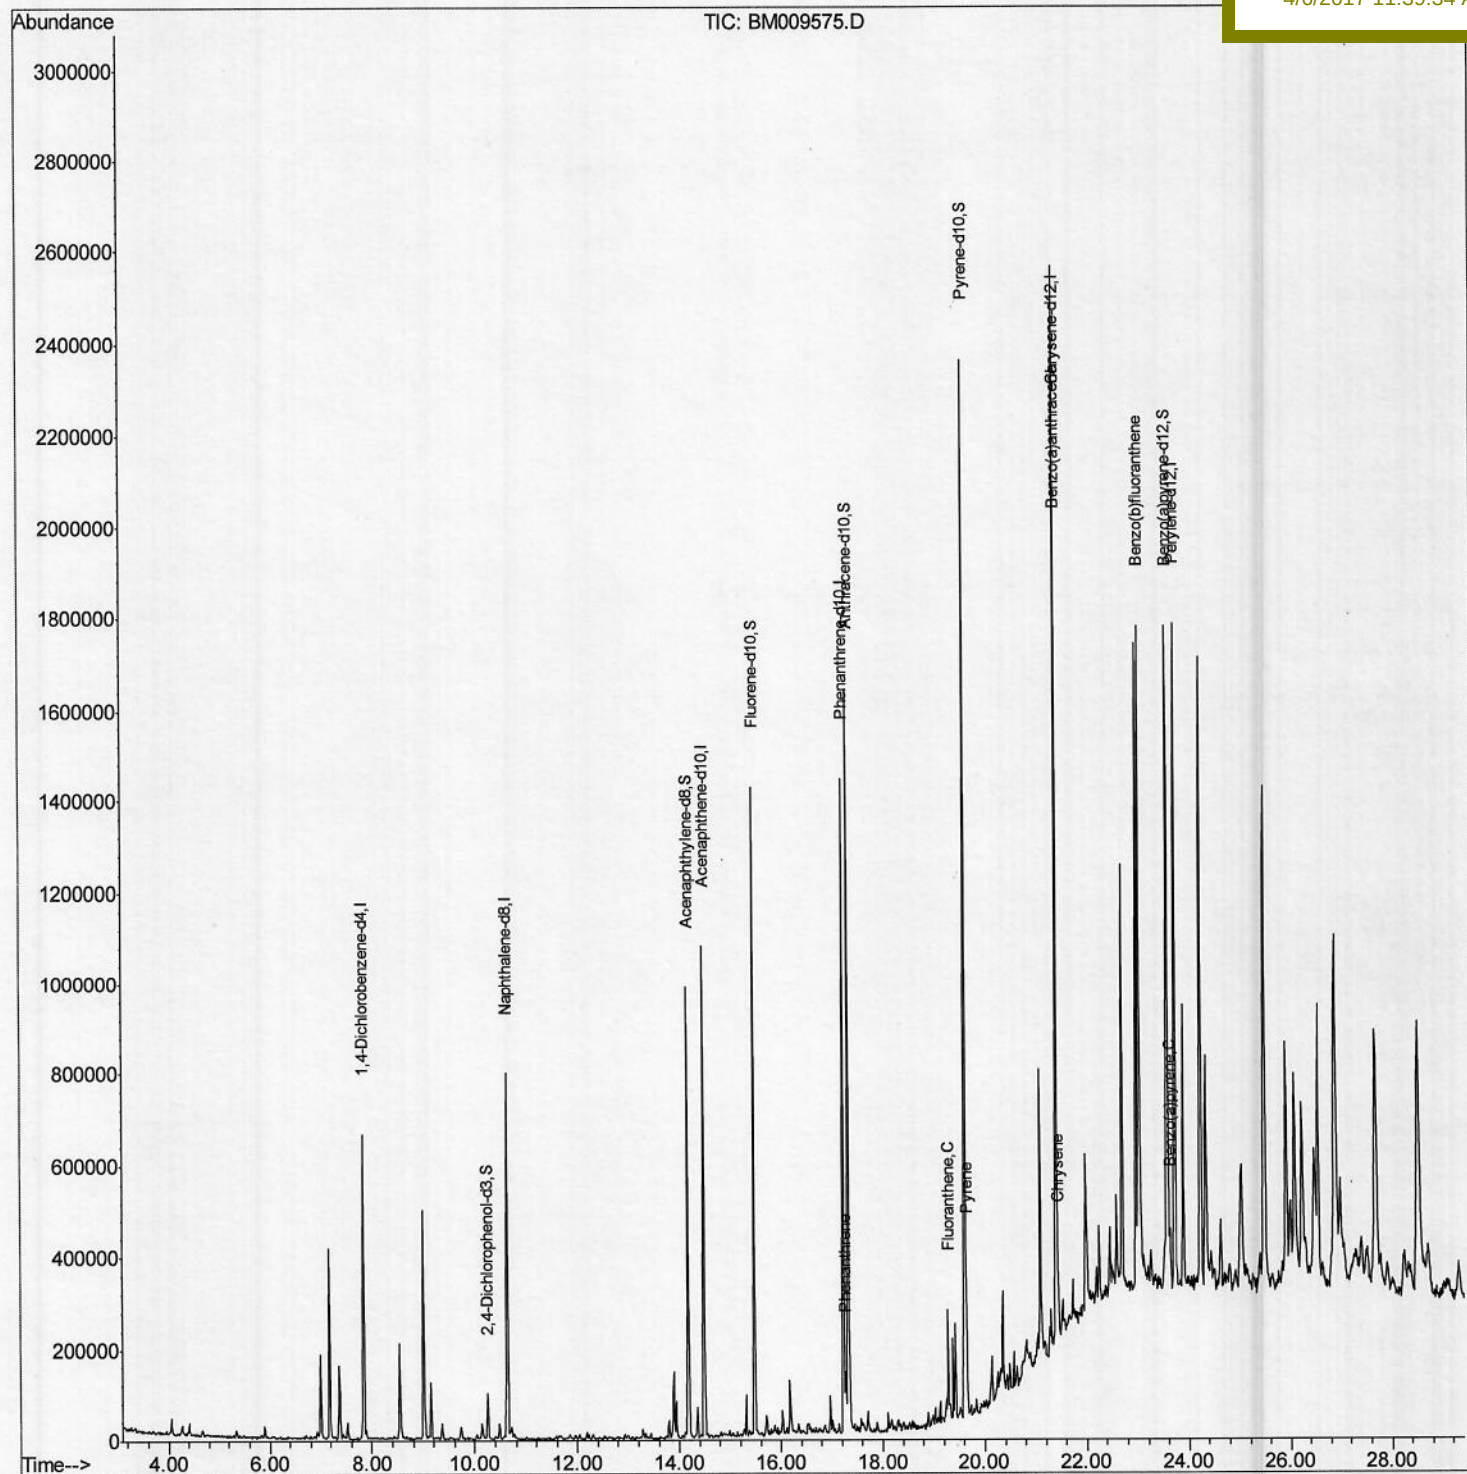

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM040617\
 Data File : BM009575.D
 Acq On : 06 Apr 2017 01:33
 Operator : SJ/MA
 Sample : I2524-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Apr 06 04:06:01 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM040417-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 06 03:48:05 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 CB328

Manual Integrations
 APPROVED

mohammad
 4/6/2017 11:39:34 AM

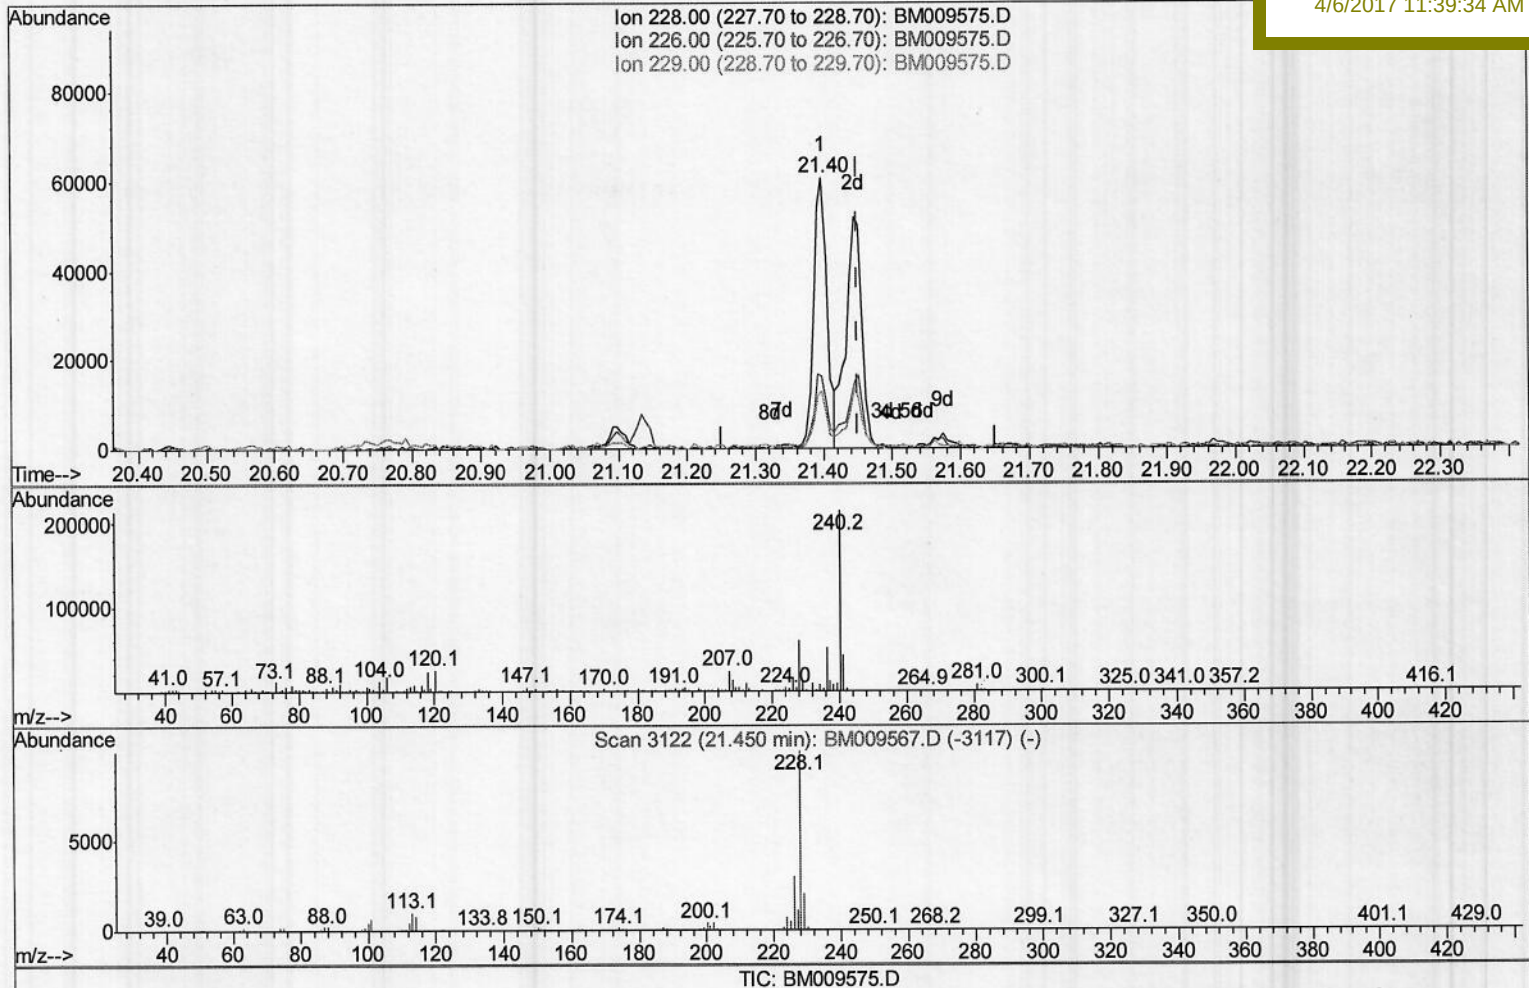

(22) Chrysene

21.398min (-0.053) 1.50ng/ui

response 82517

Ion	Exp%	Act%
228.00	100	100
226.00	31.30	26.53
229.00	20.80	20.83
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM040617\
 Data File : BM009575.D
 Acq On : 06 Apr 2017 01:33
 Operator : SJ/MA
 Sample : I2524-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB328

Quant Time: Apr 06 04:06:01 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM040417-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 06 03:48:05 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 4/6/2017 11:39:34 AM

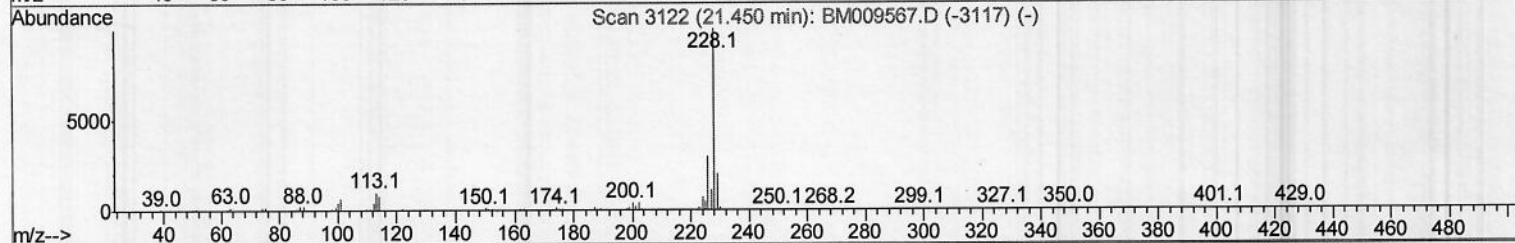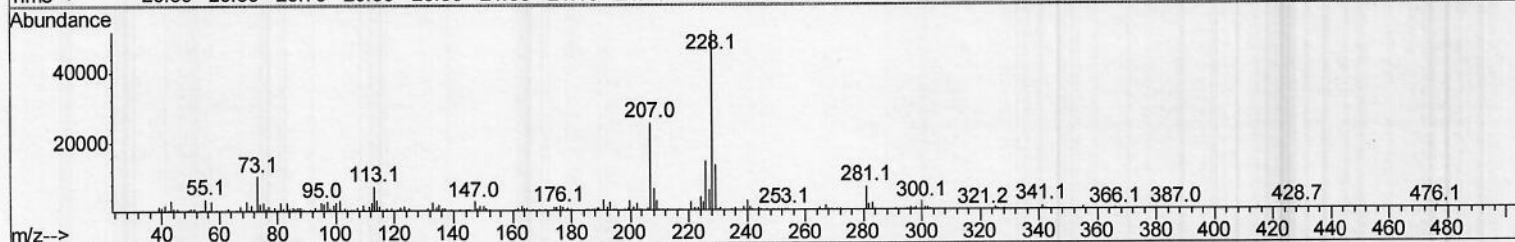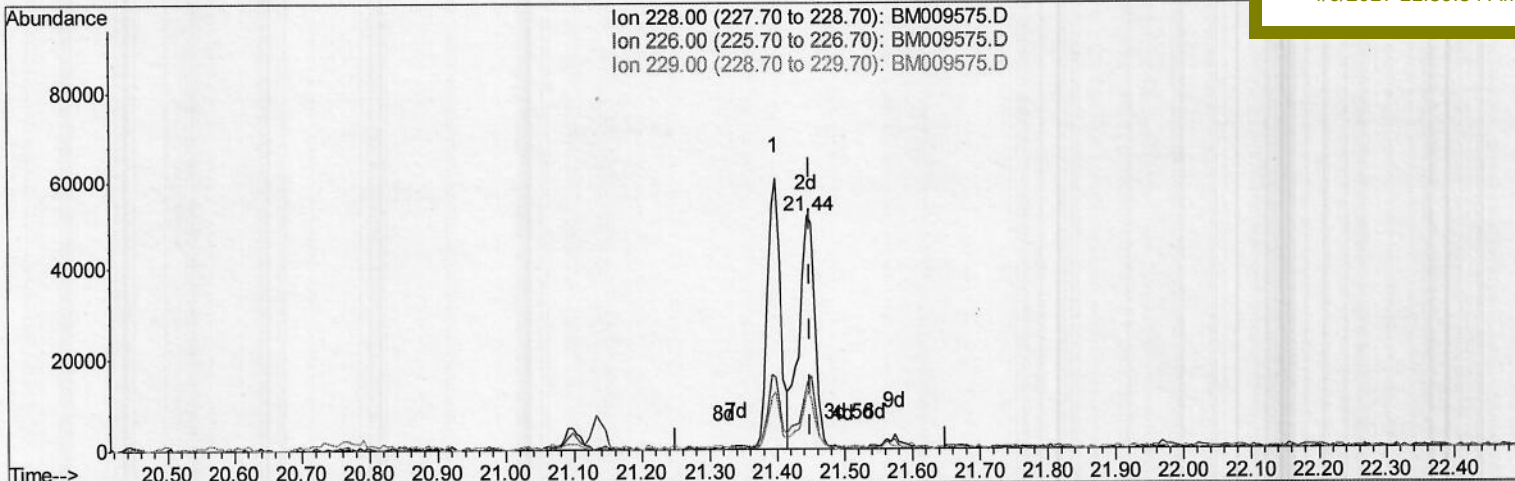

TIC: BM009575.D

(22) Chrysene

21.445min (-0.006) 1.53ng/ul m

response 84237

Ion	Exp%	Act%
228.00	100	100
226.00	31.30	28.18
229.00	20.80	26.07#
0.00	0.00	0.00

SJ
 04/10/2017

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040617\
 Data File : BM009575.D
 Acq On : 06 Apr 2017 01:33
 Operator : SJ/MA
 Sample : I2524-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB328

Quant Time: Apr 06 04:06:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM040417-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 06 03:48:05 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 4/6/2017 11:39:34 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	152318	20.00	nq/ul	0.00
2) Naphthalene-d8	10.64	136	572104	20.00	nq/ul	0.00
6) Acenaphthene-d10	14.49	164	327948	20.00	nq/ul	0.00
12) Phenanthrene-d10	17.23	188	776274	20.00	nq/ul	0.00
18) Chrysene-d12	21.41	240	1062240	20.00	nq/ul	0.00
23) Perylene-d12	23.73	264	1041376	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.25	165	34863	3.96	nq/uL	0.00
7) Acenaphthylene-d8	14.18	160	643352	20.02	nq/ul	0.00
10) Fluorene-d10	15.47	176	518130	22.41	nq/ul	0.00
15) Anthracene-d10	17.33	188	836836	22.53	nq/ul	0.00
19) Pyrene-d10	19.63	212	1048549	24.02	nq/ul	0.00
26) Benzo(a)pyrene-d12	23.58	264	993384	21.61	ng/ul	0.00
Target Compounds						
14) Phenanthrene	17.27	178	64364	1.47	nq/ul#	93
17) Fluoranthene	19.29	202	141785	2.61	nq/ul#	94
20) Pyrene	19.66	202	132329	2.29	nq/ul	96
21) Benzo(a)anthracene	21.40	228	81693	1.36	nq/ul	98
22) Chrysene	21.44	228	84237m	1.53	nq/ul	
24) Benzo(b)fluoranthene	23.03	252	114881	1.78	nq/ul#	72
27) Benzo(a)pyrene	23.63	252	69897	1.14	nq/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

95
 04/10/2017