

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040617\
 Data File : BM009558.D
 Acq On : 05 Apr 2017 15:22
 Operator : SJ/MA
 Sample : I2285-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB333

Quant Time: Apr 05 18:35:36 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM040417-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 05 13:39:58 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	120254	20.00	ng/ul	0.00
2) Naphthalene-d8	10.64	136	464444	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.49	164	269219	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.23	188	640368	20.00	ng/ul	0.00
18) Chrysene-d12	21.41	240	879857	20.00	ng/ul	0.00
23) Perylene-d12	23.73	264	848651	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.28	165	1151	0.16	ng/uL	0.02
7) Acenaphthylene-d8	14.18	160	325147	12.32	ng/ul	0.00
10) Fluorene-d10	15.48	176	323281	17.04	ng/ul	0.00
15) Anthracene-d10	17.33	188	508905	16.61	ng/ul	0.00
19) Pyrene-d10	19.63	212	612935	16.95	ng/ul	0.00
26) Benzo(a)pyrene-d12	23.58	264	282703	7.54	ng/ul	0.00
Target Compounds				Qvalue		
17) Fluoranthene	19.29	202	61421	1.37	ng/ul#	95
20) Pyrene	19.65	202	57254	1.20	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM040617\
Data File : BM009558.D
Acq On : 05 Apr 2017 15:22
Operator : SJ/MA
Sample : I2285-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB333

Quant Time: Apr 05 18:35:36 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM040417-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 05 13:39:58 2017
Response via : Initial Calibration




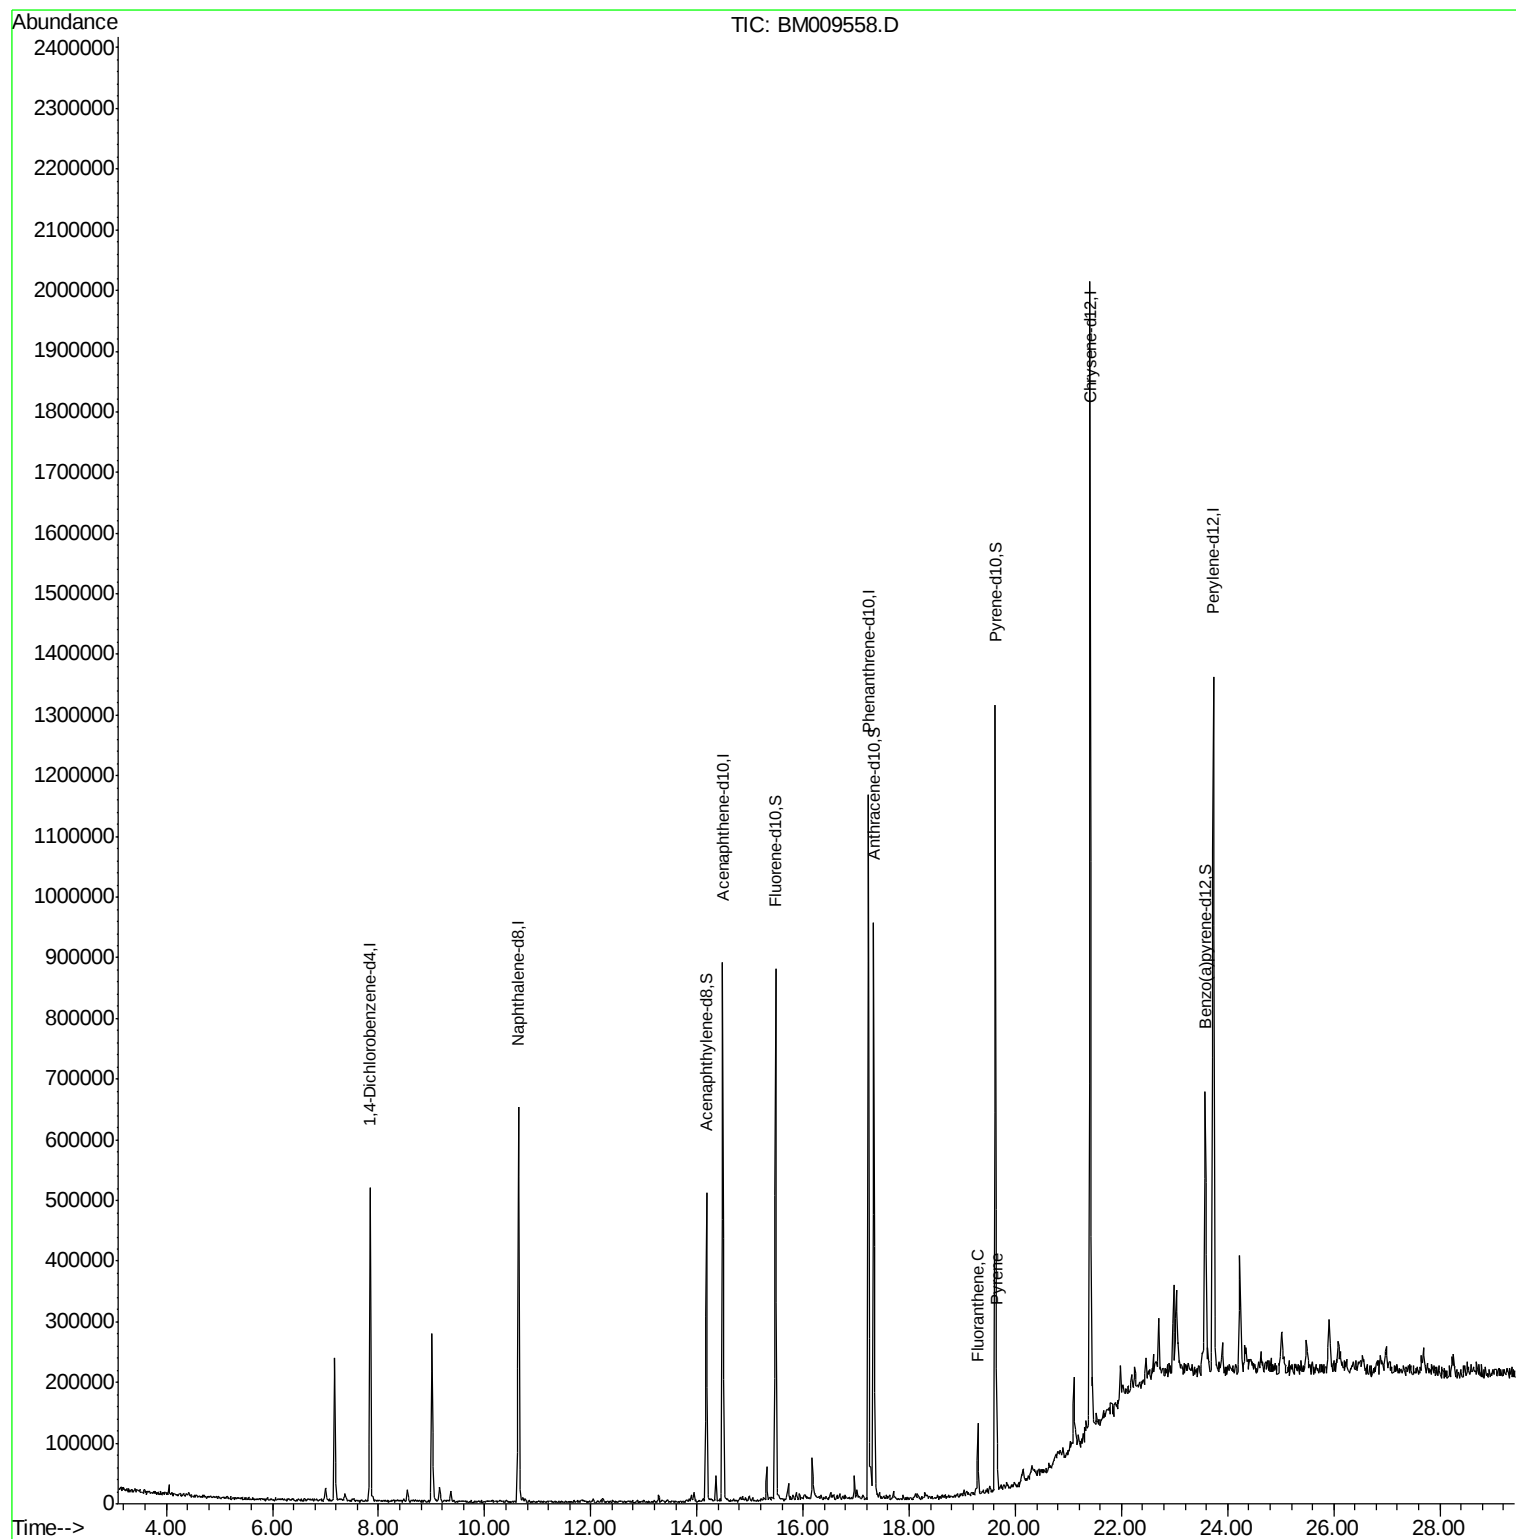


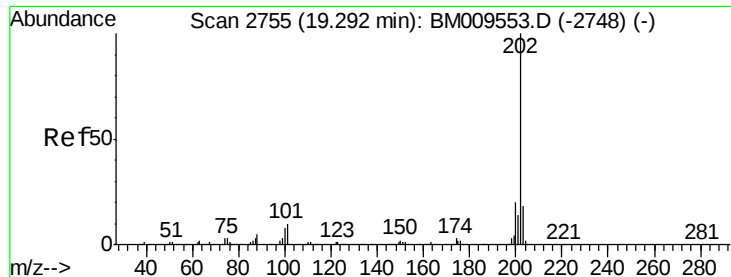

#17
Fluoranthene
 Concen: 1.37 ng/ul
 RT: 19.29 min Scan# 2755
 Delta R.T. -0.00 min
 Lab File: BM009558.D
 Acq: 05 Apr 2017 15:22

Instrument :
 BNA_M
 ClientSampleId :
 CB333

Tot Ion	Ratio	Lower	Upper
202	100		
101	10.9	9.8	14.8
100	6.9	7.5	11.3

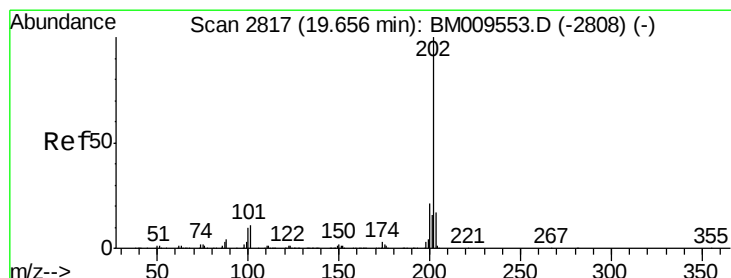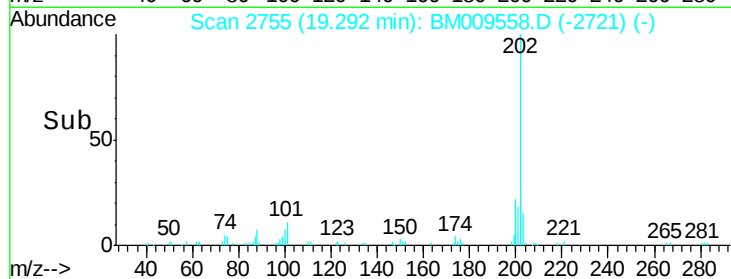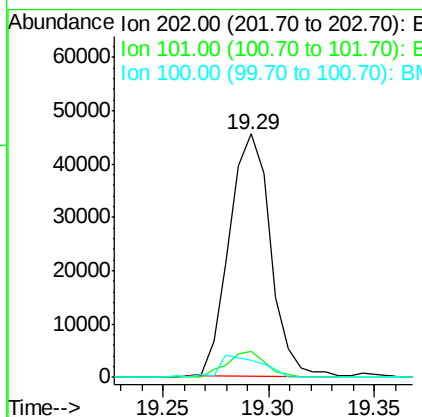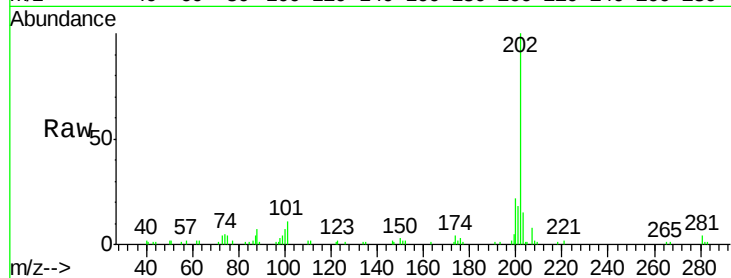

#20
Pyrene
 Concen: 1.20 ng/ul
 RT: 19.65 min Scan# 2816
 Delta R.T. -0.01 min
 Lab File: BM009558.D
 Acq: 05 Apr 2017 15:22

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.2	11.2	16.8
100	12.1	9.8	14.6

