




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034514.D
 Acq On : 06 Apr 2022 13:09
 Operator : CG/JU
 Sample : N2166-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R39

Manual IntegrationsAPPROVED

Quant Time: Apr 07 00:57:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

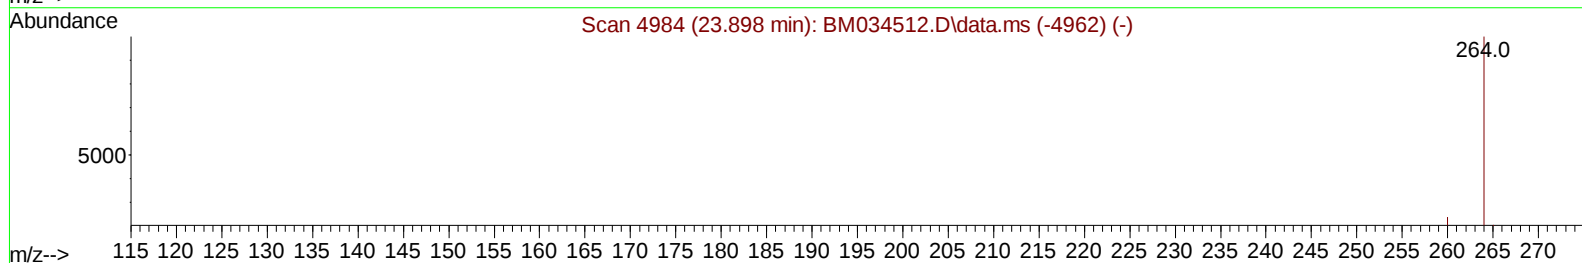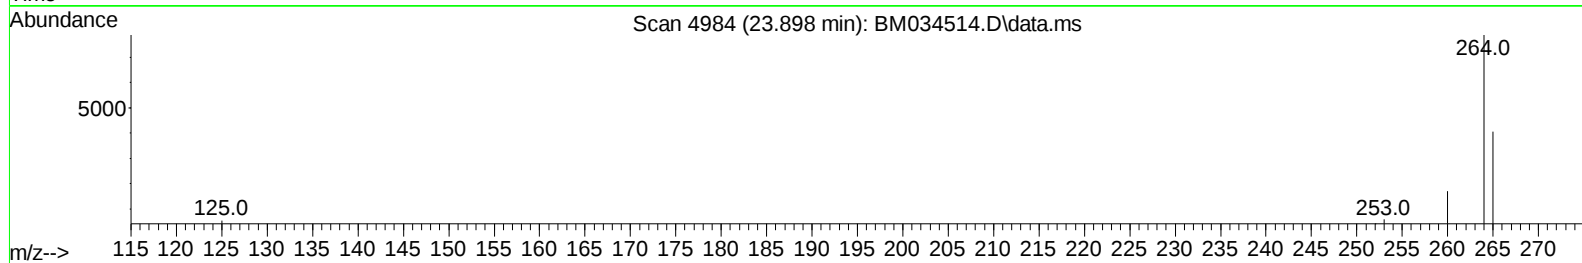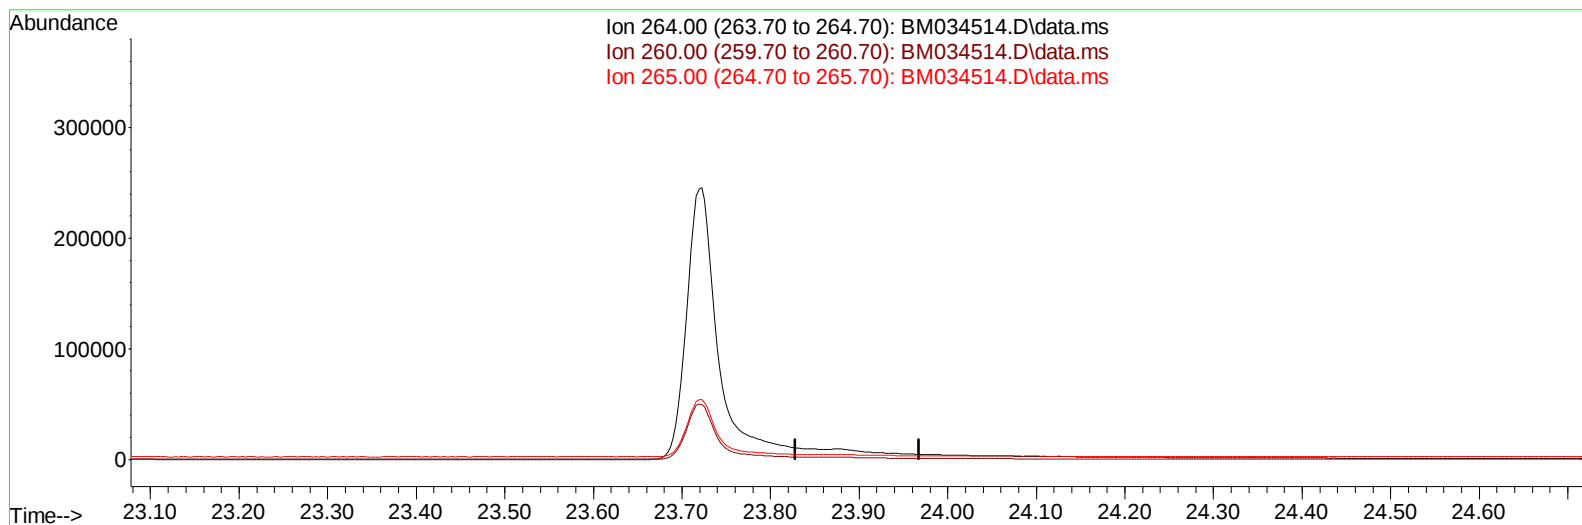

TIC: BM034514.D\data.ms

(23) Perylene-d12 (I)

23.898min (-23.898) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034514.D
 Acq On : 06 Apr 2022 13:09
 Operator : CG/JU
 Sample : N2166-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R39

Manual IntegrationsAPPROVED

Quant Time: Apr 07 00:57:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

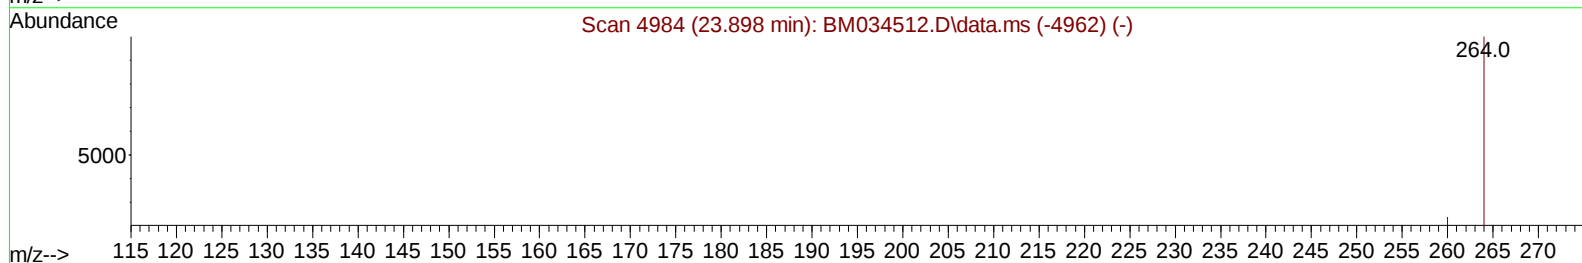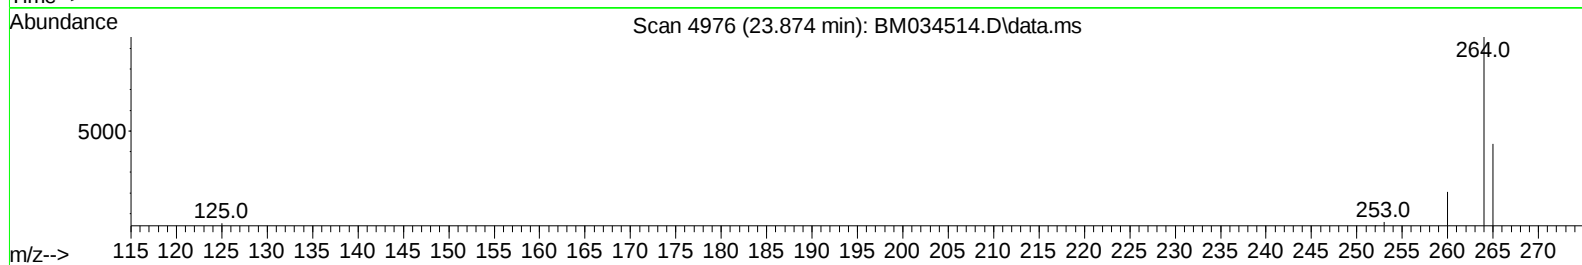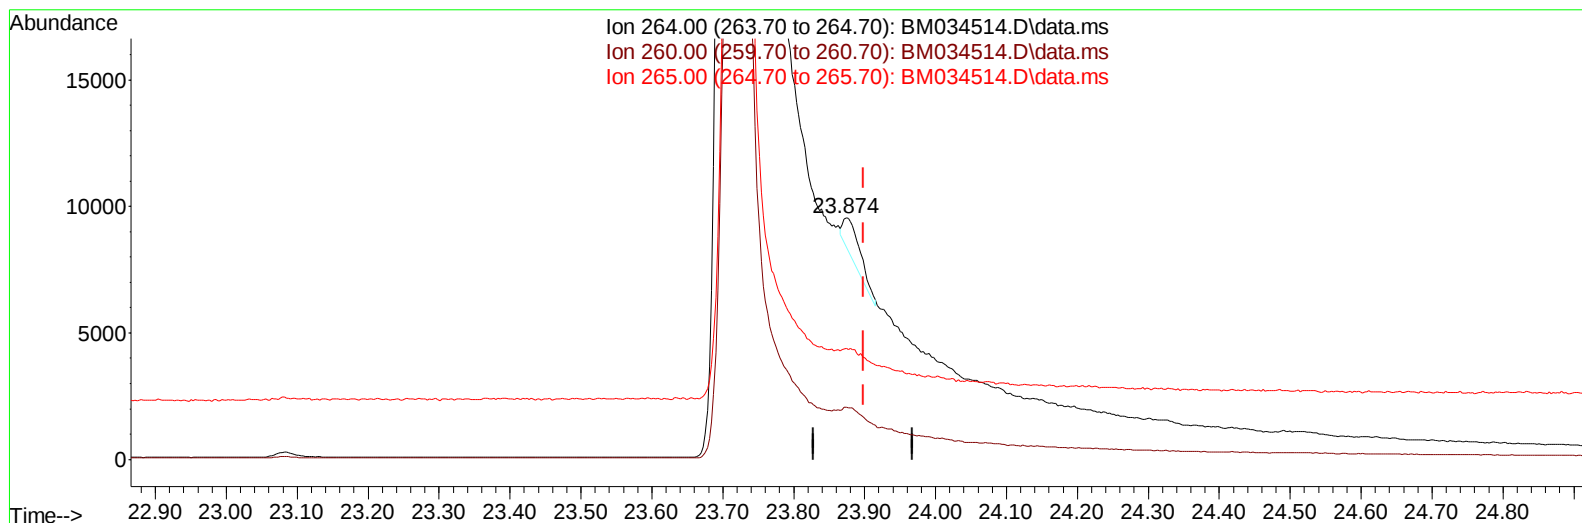

TIC: BM034514.D\data.ms

(23) Perylene-d12 (I)

23.874min (-0.024) 0.40 ng/ul m

response 2157

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	21.67#
265.00	95.30	45.87#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
 Data File : BM034514.D
 Acq On : 06 Apr 2022 13:09
 Operator : CG/JU
 Sample : N2166-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R39

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/07/2022
 Supervised By :Yogesh Patel 04/09/2022

Quant Time: Apr 07 00:57:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.912	152	3308	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.718	136	9060	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.555	164	4878	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.299	188	8707	0.400	ng/ul	-0.01
17) Chrysene-d12	21.521	240	5921	0.400	ng/ul	# 0.03
23) Perylene-d12	23.874	264	2157m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.292	96	18005	3.250	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	3466	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.324	212	7398	0.426	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040622\
Data File : BM034514.D
Acq On : 06 Apr 2022 13:09
Operator : CG/JU
Sample : N2166-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R39

Manual IntegrationsAPPROVED

Quant Time: Apr 07 00:57:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 11:50:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/07/2022
Supervised By :Yogesh Patel 04/09/2022

